


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV053120\
 Data File : VV016374.D
 Acq On : 31 May 2020 08:48
 Operator : SY/MD
 Sample : BFB36
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB36

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053020WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Mon Jun 01 12:19:30 2020

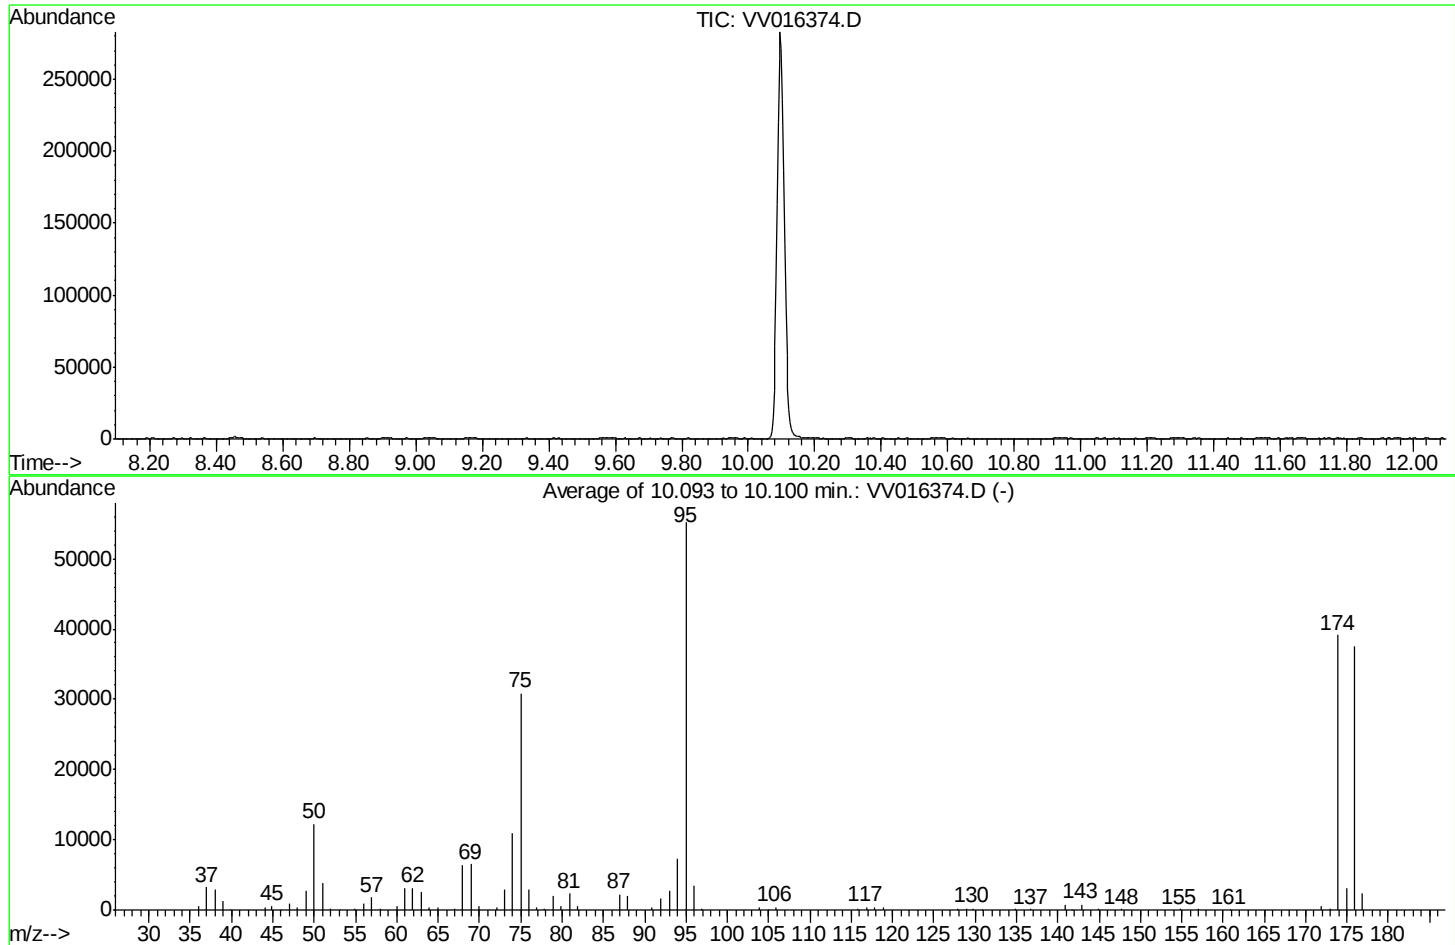

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.2	12250	PASS
75	95	30	80	55.8	30818	PASS
95	95	100	100	100.0	55189	PASS
96	95	5	9	6.3	3465	PASS
173	174	0.00	2	0.5	200	PASS
174	95	50	120	71.0	39165	PASS
175	174	5	9	7.7	3017	PASS
176	174	95	101	96.0	37605	PASS
177	176	5	9	6.1	2305	PASS

m/z	Abundance
35.90	603.0
37.00	3248.0
38.00	2915.0
39.00	1175.0
39.90	196.0
44.00	548.0
44.90	627.0
47.00	867.0
47.90	408.0
49.00	2776.0
50.00	11923.0
51.00	3795.0
51.90	227.0
53.10	106.0
54.90	236.0
55.90	920.0
57.00	1708.0
58.00	108.0
59.90	597.0
61.00	3237.0
62.00	3141.0
63.00	2489.0
64.00	299.0
65.00	336.0
67.00	176.0
68.00	6310.0
69.00	6367.0
70.00	560.0
72.00	300.0
73.00	2824.0
74.00	10668.0
75.00	29856.0
76.00	2772.0
76.90	412.0
77.80	218.0
78.90	2023.0
79.90	598.0
80.90	2207.0
81.90	526.0
87.00	2188.0
87.90	2024.0
90.80	259.0
92.00	1703.0
92.90	2628.0
94.00	6995.0
95.00	53328.0
96.00	3531.0
97.00	128.0
103.80	334.0
105.90	358.0
115.80	211.0
116.80	495.0
117.80	275.0
118.90	289.0
127.80	192.0
128.90	120.0
129.70	228.0
130.90	104.0
134.80	150.0
136.80	144.0
140.80	756.0
142.90	738.0
144.90	121.0
147.70	169.0
154.80	144.0
157.00	120.0
171.90	448.0
173.00	600.0
173.90	37000.0
174.90	2890.0
175.90	35288.0
176.90	2305.0

Instrument :
MSVOA_V
ClientSampleId :
BFB36

m/z	Abundance
36.00	637.0
37.00	3332.0
38.00	2943.0
39.00	1224.0
39.90	234.0
44.00	544.0
44.90	597.0
45.90	117.0
47.00	909.0
47.90	418.0
49.00	2865.0
50.00	12764.0
51.00	3944.0
51.90	216.0
53.10	107.0
54.90	251.0
55.90	933.0
57.00	1827.0
58.00	115.0
60.00	565.0
61.00	3219.0
62.00	3258.0
63.00	2567.0
63.90	336.0
65.00	354.0
67.00	200.0
68.00	6478.0
69.00	6767.0
70.00	575.0
72.10	326.0
73.00	3062.0
74.00	11331.0
75.00	32032.0
76.00	3001.0
76.90	423.0
77.90	249.0
78.90	2039.0
79.80	627.0
80.90	2420.0
81.90	519.0
86.90	2344.0
87.90	2086.0
90.80	294.0
92.00	1769.0
93.00	2773.0
94.00	7521.0
95.00	57216.0
96.00	3577.0
97.00	141.0
103.80	366.0
105.80	394.0
115.80	254.0
116.80	454.0
117.80	311.0
118.90	355.0
127.80	193.0
128.90	117.0
129.70	226.0
130.80	102.0
134.80	153.0
136.70	157.0
140.90	773.0
142.90	804.0
144.80	135.0
147.80	164.0
154.80	155.0
157.00	127.0
171.90	505.0
173.90	40504.0
174.90	3159.0
175.90	39056.0
176.90	2365.0

Instrument :
MSVOA_V
ClientSampleId :
BFB36

m/z	Abundance
36.00	632.0
37.00	3123.0
38.00	2716.0
39.00	1210.0
39.90	281.0
44.00	502.0
44.90	550.0
45.90	119.0
46.90	805.0
47.90	397.0
49.00	2708.0
50.00	12063.0
51.00	3577.0
51.90	184.0
54.90	201.0
56.00	880.0
57.00	1775.0
57.90	126.0
60.00	535.0
61.00	2803.0
61.90	3094.0
63.00	2418.0
63.90	347.0
64.90	330.0
67.00	180.0
68.00	6098.0
69.00	6346.0
70.00	520.0
72.00	327.0
73.00	2988.0
74.00	10686.0
75.00	30568.0
76.00	2794.0
76.90	372.0
77.90	254.0
78.90	1922.0
79.90	574.0
80.90	2318.0
81.90	480.0
86.90	2176.0
87.90	1997.0
90.80	301.0
92.00	1716.0
93.00	2685.0
94.00	7108.0
95.00	55024.0
96.00	3287.0
96.90	129.0
103.80	362.0
104.90	109.0
105.80	380.0
115.80	267.0
116.90	361.0
117.80	342.0
118.80	358.0
127.90	206.0
128.90	108.0
129.70	205.0
134.80	128.0
136.70	148.0
140.90	703.0
141.70	116.0
142.90	779.0
144.80	121.0
147.70	162.0
154.80	170.0
157.00	107.0
160.80	103.0
171.90	459.0
173.90	39992.0
174.90	3002.0
175.90	38472.0
176.90	2245.0

Instrument :
MSVOA_V
ClientSampleId :
BFB36

Scan 2788 (10.055 min): VV016374.D
BFB36

m/z	Abundance
39.90	191.0
44.10	220.0

Instrument :
MSVOA_V
ClientSampleId :
BFB36