

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053123\
 Data File : VV031296.D
 Acq On : 31 May 2023 15:03
 Operator : SY/MD
 Sample : 02950-11ME
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Jun 01 01:58:34 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jun 01 01:56:05 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	321467	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.796	117	312616	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.197	152	141238	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	102833	37.430	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	74.860%
7) Chloroethane-d5	1.529	69	76848	36.310	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	72.620%
11) 1,1-Dichloroethene-d2	2.043	65	55653	43.198	ug/L	-0.02
Spiked Amount	50.000	Range	60 - 125	Recovery	=	86.400%
21) 2-Butanone-d5	3.818	46	168802	115.309	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	115.310%
24) Chloroform-d	4.256	84	213619	43.952	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.900%
26) 1,2-Dichloroethane-d4	4.950	65	153471	46.729	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.460%
32) Benzene-d6	4.963	84	402459	47.489	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.980%
36) 1,2-Dichloropropane-d6	5.995	67	150126	59.204	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	118.400%
41) Toluene-d8	7.249	98	337996	42.732	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	85.460%
43) trans-1,3-Dichloroprop...	7.561	79	65045	51.128	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	102.260%
47) 2-Hexanone-d5	8.075	63	104574	105.772	ug/L	0.04
Spiked Amount	100.000	Range	45 - 130	Recovery	=	105.770%
56) 1,1,2,2-Tetrachloroeth...	10.172	84	192620	50.646	ug/L	0.01
Spiked Amount	50.000	Range	65 - 120	Recovery	=	101.300%
66) 1,2-Dichlorobenzene-d4	11.574	152	126779	49.951	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	99.900%
Target Compounds						
44) trans-1,3-Dichloropropene	7.564	75	2939	0.914	ug/L	Qvalue # 49


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053123\
Data File : VV031296.D
Acq On : 31 May 2023 15:03
Operator : SY/MD
Sample : 02950-11ME
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Jun 01 01:58:34 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jun 01 01:56:05 2023
Response via : Initial Calibration

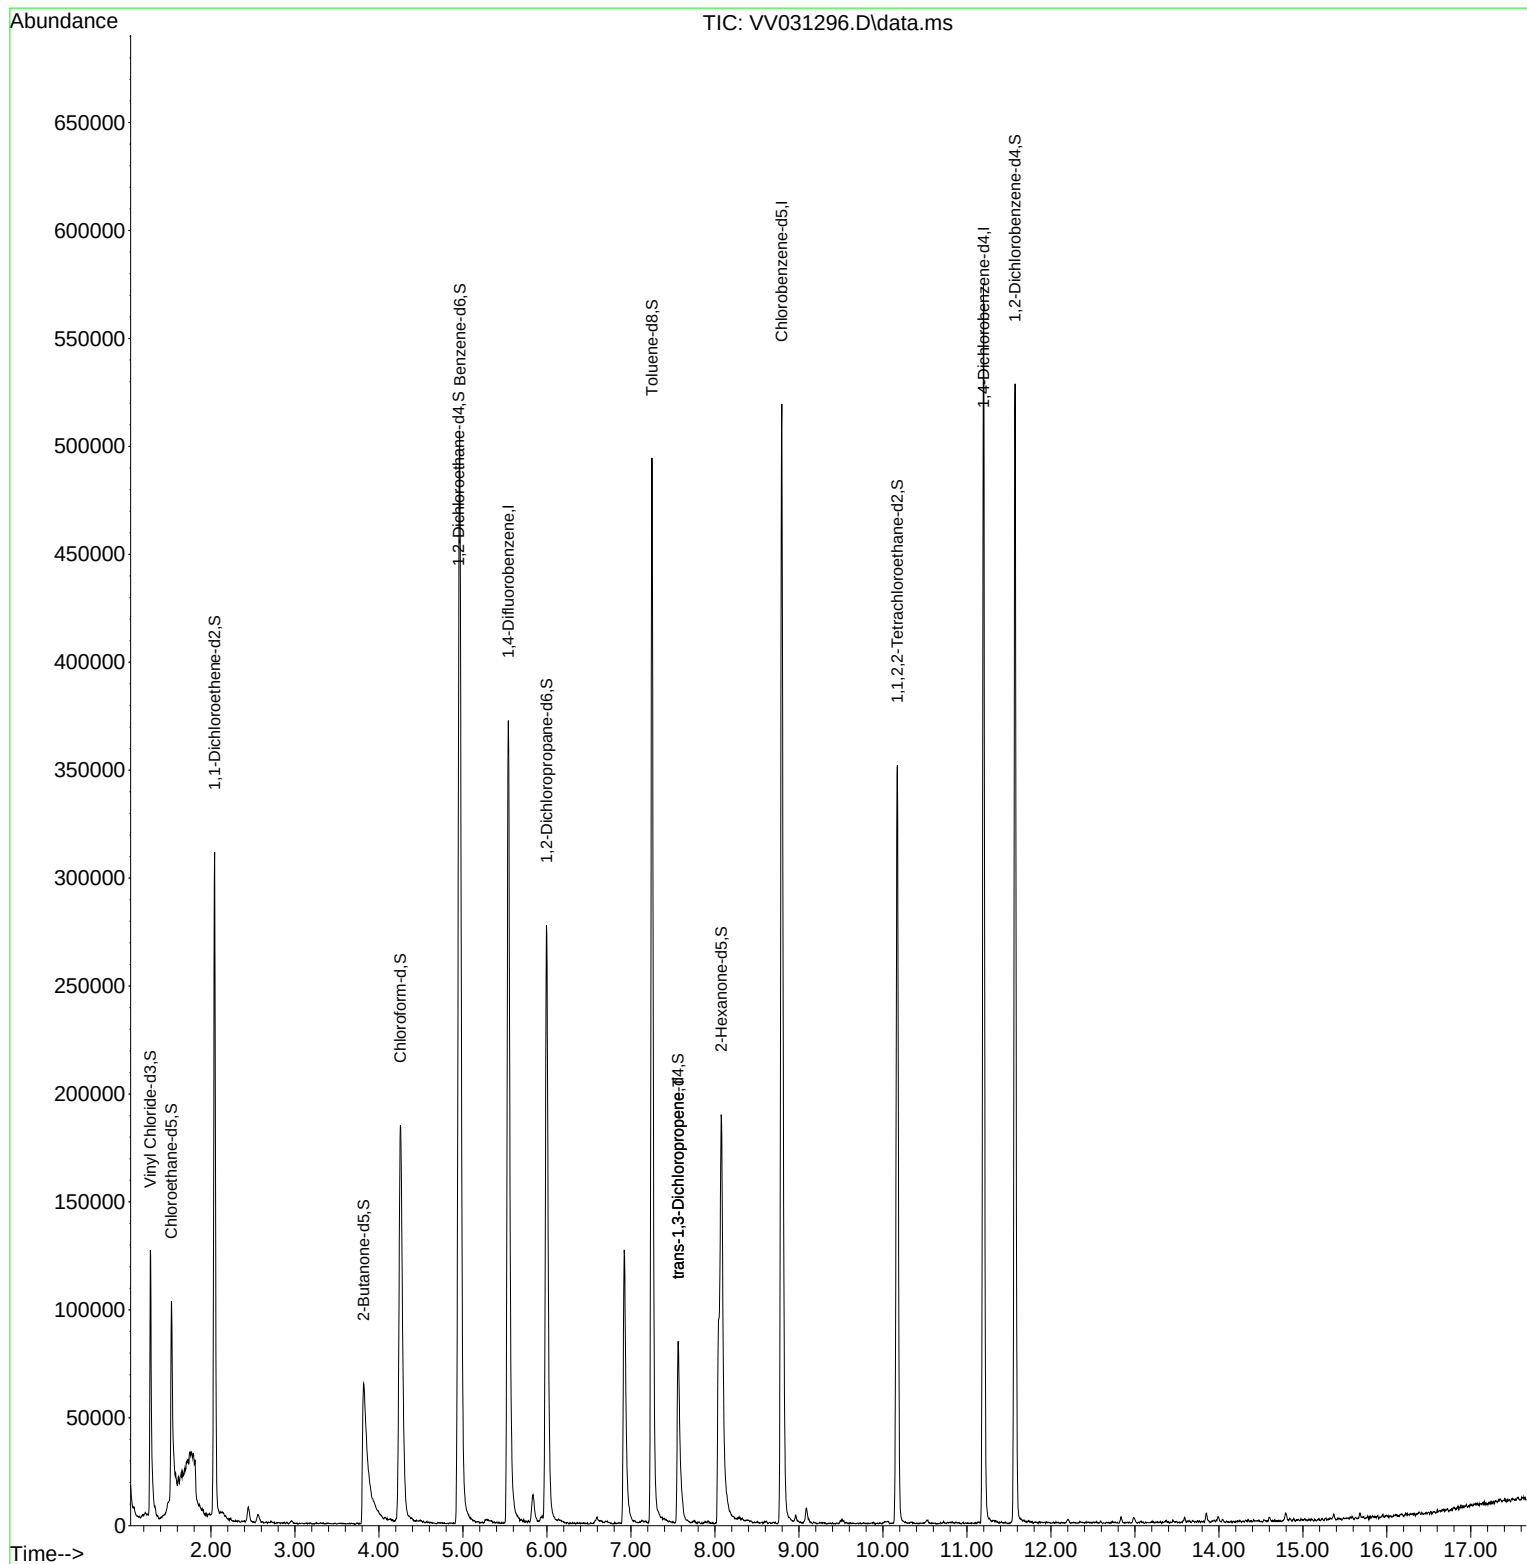

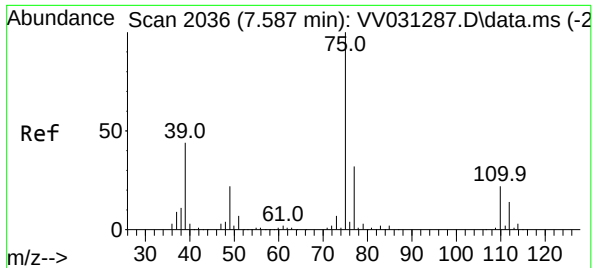

#44
 trans-1,3-Dichloropropene
 Concen: 0.914 ug/L
 RT: 7.564 min Scan# 20
 Delta R.T. -0.023 min
 Lab File: VV031296.D
 Acq: 31 May 2023 15:03

Instrument :
 MSVOA_V
 ClientSampleId :

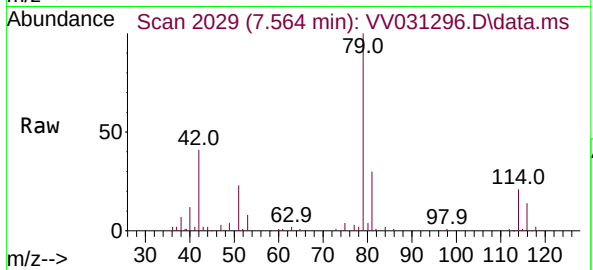

Tgt Ion: 75 Resp: 2939
 Ion Ratio Lower Upper
 75 100
 77 59.9 22.2 41.2#

