

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053123\
 Data File : VV031288.D
 Acq On : 31 May 2023 11:54
 Operator : SY/MD
 Sample : VV0531MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK347

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031288.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	89	rBV	148320	157492	13.73%	1.817%
2	1.536	147	154	166	rVB	141987	166199	14.48%	1.917%
3	2.063	308	318	332	rBV	262443	382432	33.33%	4.412%
4	2.452	432	439	449	rBV5	3812	5732	0.50%	0.066%
5	2.571	473	476	478	rBV2	564	285	0.02%	0.003%
6	2.661	501	504	506	rBV3	544	350	0.03%	0.004%
7	2.857	561	565	569	rBV2	359	356	0.03%	0.004%
8	2.928	586	587	591	rVB2	505	247	0.02%	0.003%
9	2.953	591	595	597	rBV3	335	284	0.02%	0.003%
10	3.079	633	634	638	rVB2	325	161	0.01%	0.002%
11	3.095	638	639	641	rVB2	267	79	0.01%	0.001%
12	3.111	641	644	646	rBV2	522	328	0.03%	0.004%
13	3.252	686	688	692	rVB2	427	222	0.02%	0.003%
14	3.281	692	697	702	rBV3	752	760	0.07%	0.009%
15	3.368	722	724	725	rBV	280	76	0.01%	0.001%
16	3.384	725	729	730	rVV	204	137	0.01%	0.002%
17	3.394	730	732	737	rVV2	472	403	0.04%	0.005%
18	3.416	737	739	742	rVV	565	312	0.03%	0.004%
19	3.449	745	749	753	rVV	541	425	0.04%	0.005%
20	3.468	753	755	760	rVB3	460	378	0.03%	0.004%
21	3.494	760	763	766	rBV	413	301	0.03%	0.003%
22	3.558	778	783	787	rBV3	512	422	0.04%	0.005%
23	3.577	787	789	790	rBV	254	116	0.01%	0.001%
24	3.597	793	795	800	rVB2	453	269	0.02%	0.003%
25	3.622	800	803	804	rBV	248	156	0.01%	0.002%
26	3.658	812	814	815	rBV	186	84	0.01%	0.001%
27	3.796	848	857	885	rBV	81846	235072	20.49%	2.712%
28	4.256	982	1000	1025	rBV	170849	472688	41.20%	5.453%
29	4.519	1080	1082	1086	rVB2	982	601	0.05%	0.007%
30	4.732	1145	1148	1150	rBV4	390	197	0.02%	0.002%
31	4.838	1179	1181	1184	rBV2	343	188	0.02%	0.002%
32	4.889	1194	1197	1199	rBV	402	269	0.02%	0.003%
33	4.960	1202	1219	1258	rBV3	410423	1147398	100.00%	13.236%
34	5.214	1297	1298	1301	rBV3	715	341	0.03%	0.004%
35	5.387	1348	1352	1353	rBV2	409	272	0.02%	0.003%
36	5.423	1360	1363	1365	rBV2	347	203	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053123\
 Data File : VV031288.D
 Acq On : 31 May 2023 11:54
 Operator : SY/MD
 Sample : VV0531MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK347

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	5.439	1365	1368	1370	rVB3	385	203	0.02%	0.002%
38	5.539	1386	1399	1441	rBV	346144	769956	67.10%	8.882%
39	5.995	1527	1541	1570	rBV	252315	557142	48.56%	6.427%
40	6.233	1613	1615	1618	rBV4	542	289	0.03%	0.003%
41	6.281	1628	1630	1635	rVB2	599	481	0.04%	0.006%
42	6.313	1635	1640	1644	rBV4	522	532	0.05%	0.006%
43	6.407	1665	1669	1670	rBV	290	188	0.02%	0.002%
44	6.439	1677	1679	1683	rBV2	316	206	0.02%	0.002%
45	6.468	1685	1688	1691	rBV2	476	274	0.02%	0.003%
46	6.545	1708	1712	1715	rBV2	818	715	0.06%	0.008%
47	6.657	1744	1747	1752	rBV4	444	423	0.04%	0.005%
48	6.709	1762	1763	1766	rBV	285	173	0.02%	0.002%
49	6.741	1771	1773	1774	rBV	362	143	0.01%	0.002%
50	6.809	1792	1794	1800	rBV2	573	422	0.04%	0.005%
51	6.834	1800	1802	1805	rBV2	398	243	0.02%	0.003%
52	6.854	1805	1808	1811	rVB2	813	570	0.05%	0.007%
53	6.866	1811	1812	1814	rVB	302	89	0.01%	0.001%
54	6.918	1814	1828	1862	rBV	114973	236683	20.63%	2.730%
55	7.249	1919	1931	1965	rBV	432629	793973	69.20%	9.159%
56	7.558	2018	2027	2049	rBV	86257	158794	13.84%	1.832%
57	7.792	2098	2100	2105	rVB	417	325	0.03%	0.004%
58	8.034	2165	2175	2208	rBV	254486	547734	47.74%	6.319%
59	8.436	2298	2300	2301	rBV2	406	138	0.01%	0.002%
60	8.612	2351	2355	2358	rBV2	692	451	0.04%	0.005%
61	8.632	2358	2361	2364	rBV3	731	550	0.05%	0.006%
62	8.789	2397	2410	2442	rBV	544505	930464	81.09%	10.734%
63	9.069	2495	2497	2498	rBV2	461	216	0.02%	0.002%
64	9.095	2503	2505	2508	rBV	372	198	0.02%	0.002%
65	9.127	2510	2515	2517	rBV	573	498	0.04%	0.006%
66	9.214	2540	2542	2544	rBV	464	319	0.03%	0.004%
67	9.294	2564	2567	2571	rBV2	618	396	0.03%	0.005%
68	9.317	2571	2574	2575	rBV2	381	210	0.02%	0.002%
69	9.342	2580	2582	2584	rBV2	362	167	0.01%	0.002%
70	9.374	2590	2592	2597	rBV2	391	230	0.02%	0.003%
71	9.471	2619	2622	2625	rBV3	688	540	0.05%	0.006%
72	9.680	2684	2687	2689	rBV	506	359	0.03%	0.004%
73	9.722	2693	2700	2702	rBV3	493	557	0.05%	0.006%
74	9.831	2731	2734	2736	rBV2	309	172	0.01%	0.002%
75	9.886	2748	2751	2757	rVB3	765	575	0.05%	0.007%
76	9.924	2762	2763	2766	rVB2	275	133	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053123\
 Data File : VV031288.D
 Acq On : 31 May 2023 11:54
 Operator : SY/MD
 Sample : VV0531MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK347

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	9.989	2779	2783	2785	rBV2	264	196	0.02%	0.002%
78	10.011	2786	2790	2793	rBV3	365	358	0.03%	0.004%
79	10.159	2823	2836	2858	rBV	350588	561258	48.92%	6.475%
80	10.288	2872	2876	2878	rBV4	905	676	0.06%	0.008%
81	10.390	2905	2908	2909	rBV	402	209	0.02%	0.002%
82	10.400	2909	2911	2912	rVB	452	118	0.01%	0.001%
83	10.413	2912	2915	2917	rBV2	549	448	0.04%	0.005%
84	10.448	2922	2926	2928	rBV2	399	303	0.03%	0.003%
85	10.516	2946	2947	2949	rBV2	374	118	0.01%	0.001%
86	10.554	2955	2959	2964	rBV5	677	676	0.06%	0.008%
87	10.577	2964	2966	2968	rBV	319	158	0.01%	0.002%
88	10.673	2991	2996	3001	rBV3	584	703	0.06%	0.008%
89	10.696	3002	3003	3007	rVB2	453	240	0.02%	0.003%
90	10.776	3026	3028	3029	rBV	260	102	0.01%	0.001%
91	10.837	3043	3047	3048	rBV2	421	336	0.03%	0.004%
92	11.091	3124	3126	3128	rBV	463	240	0.02%	0.003%
93	11.191	3146	3157	3181	rBV	504819	793291	69.14%	9.151%
94	11.567	3262	3274	3292	rBV	453197	726149	63.29%	8.377%
95	11.915	3379	3382	3385	rBV	479	421	0.04%	0.005%
96	12.712	3627	3630	3631	rBV	573	222	0.02%	0.003%
97	12.853	3672	3674	3678	rBV3	492	397	0.03%	0.005%
98	13.021	3723	3726	3728	rBV3	616	462	0.04%	0.005%
99	13.590	3899	3903	3905	rBV2	751	612	0.05%	0.007%




Sum of corrected areas: 8668659

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053123\
Data File : VV031288.D
Acq On : 31 May 2023 11:54
Operator : SY/MD
Sample : VV0531MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK347

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

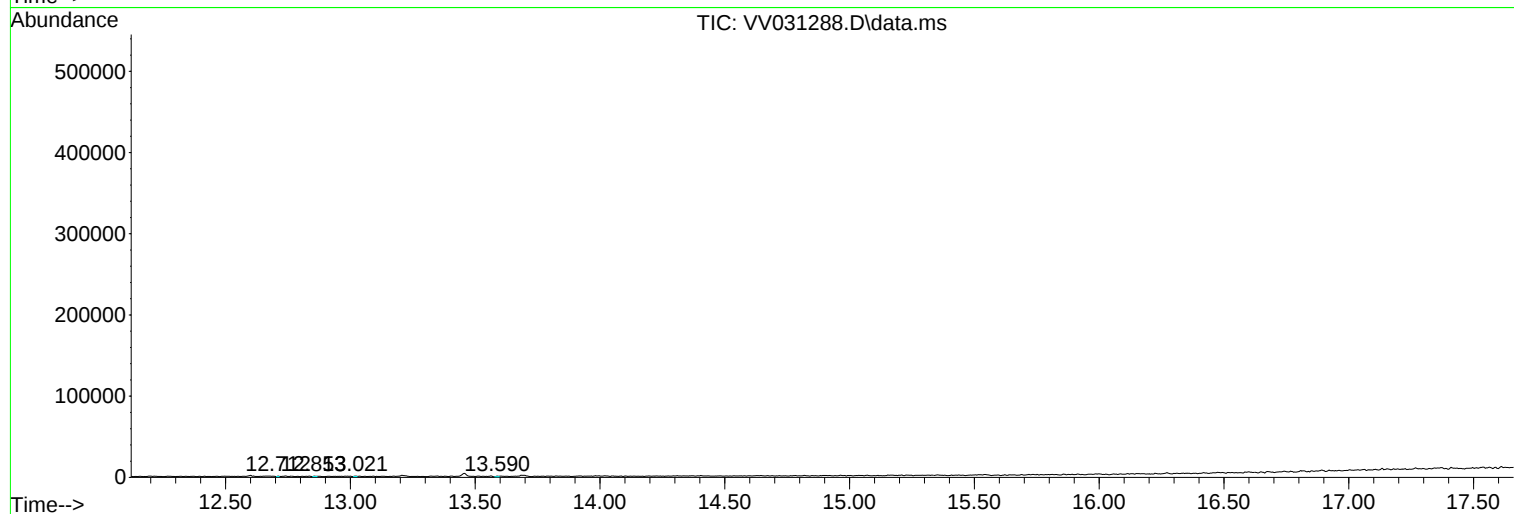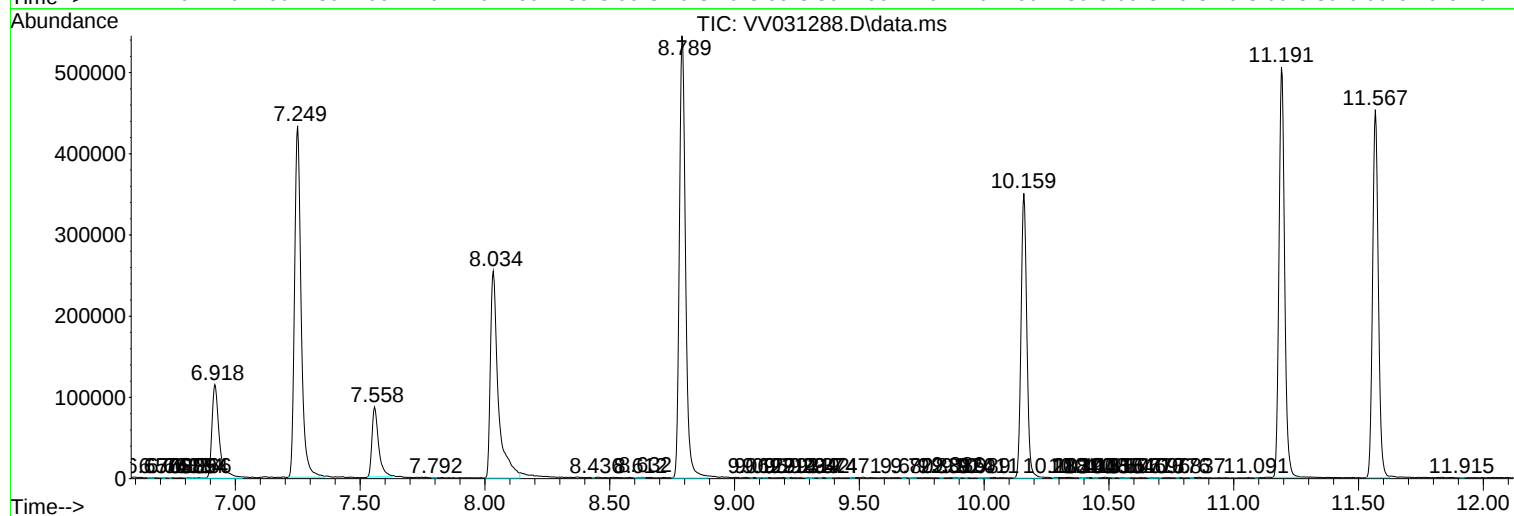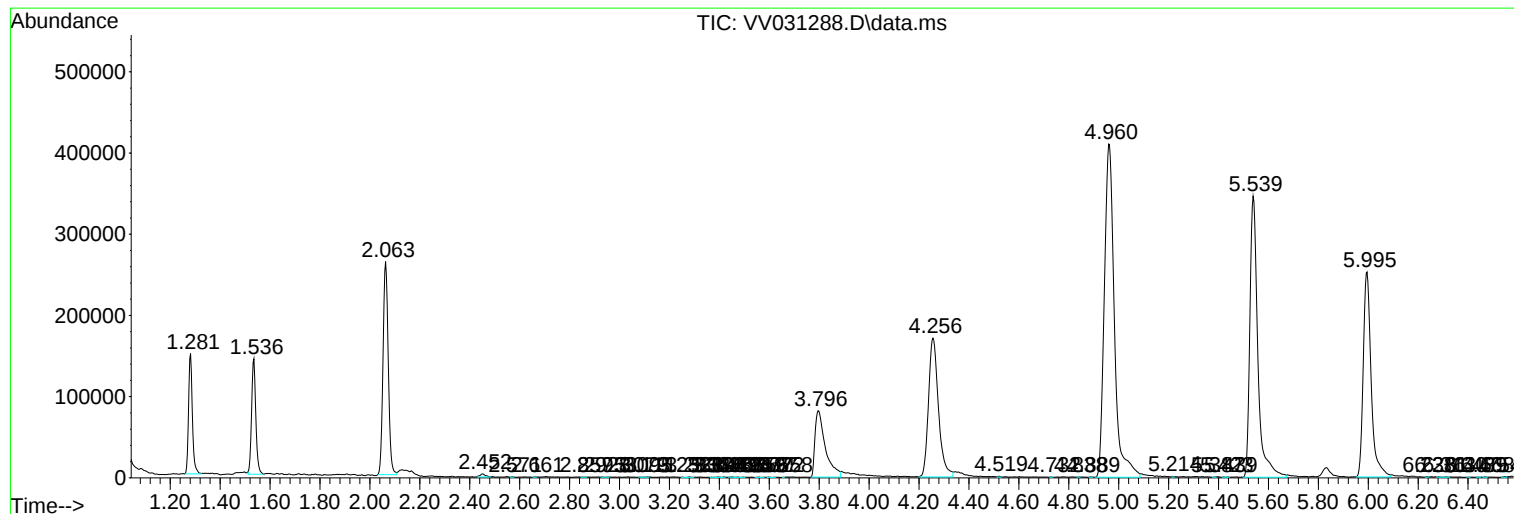

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053123\
Data File : VV031288.D
Acq On : 31 May 2023 11:54
Operator : SY/MD
Sample : VV0531MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK347

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053123\
Data File : VV031288.D
Acq On : 31 May 2023 11:54
Operator : SY/MD
Sample : VV0531MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK347

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------