

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053123\
 Data File : VV031293.D
 Acq On : 31 May 2023 13:51
 Operator : SY/MD
 Sample : 02961-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FP5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031293.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	90	rVB	140566	148634	13.64%	1.848%
2	1.536	147	154	166	rVB	132945	157054	14.41%	1.952%
3	2.063	309	318	331	rBV	246047	355521	32.62%	4.419%
4	2.237	370	372	378	rVB4	987	717	0.07%	0.009%
5	2.359	406	410	415	rBV3	594	584	0.05%	0.007%
6	2.426	428	431	434	rBV3	583	498	0.05%	0.006%
7	2.442	434	436	437	rBV2	669	339	0.03%	0.004%
8	2.690	510	513	514	rBV	398	197	0.02%	0.002%
9	2.770	535	538	541	rBV	359	255	0.02%	0.003%
10	2.921	583	585	587	rBV	184	53	0.00%	0.001%
11	2.957	592	596	598	rBV2	503	493	0.05%	0.006%
12	3.018	613	615	619	rVB2	329	208	0.02%	0.003%
13	3.044	619	623	625	rBV3	688	471	0.04%	0.006%
14	3.111	642	644	645	rBV	341	163	0.01%	0.002%
15	3.153	655	657	660	rVB	454	194	0.02%	0.002%
16	3.175	662	664	667	rVB3	423	218	0.02%	0.003%
17	3.195	667	670	672	rBV	403	247	0.02%	0.003%
18	3.259	687	690	692	rBV	353	187	0.02%	0.002%
19	3.272	692	694	696	rBV2	295	135	0.01%	0.002%
20	3.298	701	702	705	rVB	313	128	0.01%	0.002%
21	3.317	705	708	711	rBV	428	339	0.03%	0.004%
22	3.355	716	720	721	rBV	445	309	0.03%	0.004%
23	3.536	774	776	783	rVB2	444	384	0.04%	0.005%
24	3.571	783	787	788	rBV	470	314	0.03%	0.004%
25	3.655	811	813	815	rBV	276	129	0.01%	0.002%
26	3.667	815	817	818	rVV	203	58	0.01%	0.001%
27	3.748	840	842	845	rBV2	306	198	0.02%	0.002%
28	3.799	848	858	890	rBV2	74245	225088	20.65%	2.798%
29	4.166	969	972	975	rBV	759	528	0.05%	0.007%
30	4.259	986	1001	1028	rBV2	163238	440578	40.42%	5.477%
31	4.629	1114	1116	1120	rBV2	328	208	0.02%	0.003%
32	4.658	1124	1125	1131	rVB3	618	333	0.03%	0.004%
33	4.693	1131	1136	1139	rBV4	596	657	0.06%	0.008%
34	4.790	1162	1166	1168	rBV2	542	357	0.03%	0.004%
35	4.963	1203	1220	1267	rBV2	386861	1089975	100.00%	13.549%
36	5.458	1372	1374	1376	rVB	400	160	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053123\
 Data File : VV031293.D
 Acq On : 31 May 2023 13:51
 Operator : SY/MD
 Sample : 02961-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FP5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	5.471	1376	1378	1380	rBV	399	174	0.02%	0.002%
38	5.481	1380	1381	1383	rBV	258	129	0.01%	0.002%
39	5.542	1388	1400	1433	rBV2	313510	682719	62.64%	8.486%
40	5.995	1528	1541	1569	rBV	244685	531736	48.78%	6.610%
41	6.259	1620	1623	1626	rBV	487	279	0.03%	0.003%
42	6.336	1644	1647	1650	rVB2	447	332	0.03%	0.004%
43	6.413	1669	1671	1673	rBV2	491	215	0.02%	0.003%
44	6.478	1689	1691	1694	rBV2	292	115	0.01%	0.001%
45	6.497	1694	1697	1701	rVB3	631	424	0.04%	0.005%
46	6.564	1715	1718	1719	rBV	747	434	0.04%	0.005%
47	6.703	1759	1761	1764	rBV2	504	345	0.03%	0.004%
48	6.825	1797	1799	1802	rBV	495	273	0.03%	0.003%
49	6.854	1805	1808	1809	rVV	226	130	0.01%	0.002%
50	6.918	1816	1828	1850	rBV	108118	215034	19.73%	2.673%
51	7.249	1920	1931	1962	rBV	404142	741592	68.04%	9.218%
52	7.561	2018	2028	2054	rBV	78046	152035	13.95%	1.890%
53	7.796	2097	2101	2105	rVB3	595	540	0.05%	0.007%
54	7.860	2119	2121	2122	rBV2	280	144	0.01%	0.002%
55	7.886	2125	2129	2131	rBV2	659	509	0.05%	0.006%
56	7.969	2152	2155	2156	rBV2	342	157	0.01%	0.002%
57	8.034	2165	2175	2206	rBV	236736	509217	46.72%	6.330%
58	8.410	2288	2292	2297	rBV4	765	701	0.06%	0.009%
59	8.442	2300	2302	2304	rBV2	587	300	0.03%	0.004%
60	8.629	2356	2360	2361	rBV	351	204	0.02%	0.003%
61	8.651	2365	2367	2373	rVV3	546	381	0.03%	0.005%
62	8.789	2398	2410	2442	rBV	492450	837973	76.88%	10.416%
63	9.047	2487	2490	2492	rBV2	765	523	0.05%	0.007%
64	9.085	2500	2502	2503	rBV2	536	229	0.02%	0.003%
65	9.153	2521	2523	2526	rBV2	399	278	0.03%	0.003%
66	9.317	2572	2574	2579	rVB3	446	312	0.03%	0.004%
67	9.410	2599	2603	2605	rBV2	800	521	0.05%	0.006%
68	9.487	2623	2627	2629	rBV3	518	444	0.04%	0.006%
69	9.580	2654	2656	2661	rVB2	576	264	0.02%	0.003%
70	9.654	2677	2679	2682	rVB3	357	187	0.02%	0.002%
71	9.674	2682	2685	2686	rBV	388	153	0.01%	0.002%
72	9.709	2695	2696	2699	rVB	274	101	0.01%	0.001%
73	9.728	2699	2702	2705	rBV3	461	305	0.03%	0.004%
74	9.793	2714	2722	2725	rBV4	580	797	0.07%	0.010%
75	9.831	2732	2734	2737	rVB2	416	236	0.02%	0.003%
76	9.850	2737	2740	2742	rBV2	339	253	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053123\
 Data File : VV031293.D
 Acq On : 31 May 2023 13:51
 Operator : SY/MD
 Sample : 02961-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FP5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	10.008	2785	2789	2791	rBV4	495	359	0.03%	0.004%
78	10.117	2820	2823	2824	rBV	395	182	0.02%	0.002%
79	10.159	2824	2836	2855	rVV	336199	537797	49.34%	6.685%
80	10.522	2946	2949	2951	rBV2	613	431	0.04%	0.005%
81	10.702	3003	3005	3007	rVB2	324	150	0.01%	0.002%
82	10.735	3013	3015	3017	rVB3	302	93	0.01%	0.001%
83	11.050	3108	3113	3115	rBV2	546	620	0.06%	0.008%
84	11.120	3133	3135	3136	rBV	635	198	0.02%	0.002%
85	11.191	3146	3157	3176	rBV	448849	710537	65.19%	8.832%
86	11.567	3262	3274	3302	rBV	427284	685502	62.89%	8.521%
87	12.477	3555	3557	3560	rBV	434	224	0.02%	0.003%
88	12.583	3588	3590	3592	rBV	737	361	0.03%	0.004%
89	13.088	3745	3747	3749	rBV	502	290	0.03%	0.004%
90	13.506	3870	3877	3883	rBV4	845	1189	0.11%	0.015%
91	13.780	3960	3962	3965	rBV2	509	325	0.03%	0.004%




Sum of corrected areas: 8044864

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053123\
Data File : VV031293.D
Acq On : 31 May 2023 13:51
Operator : SY/MD
Sample : 02961-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FP5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

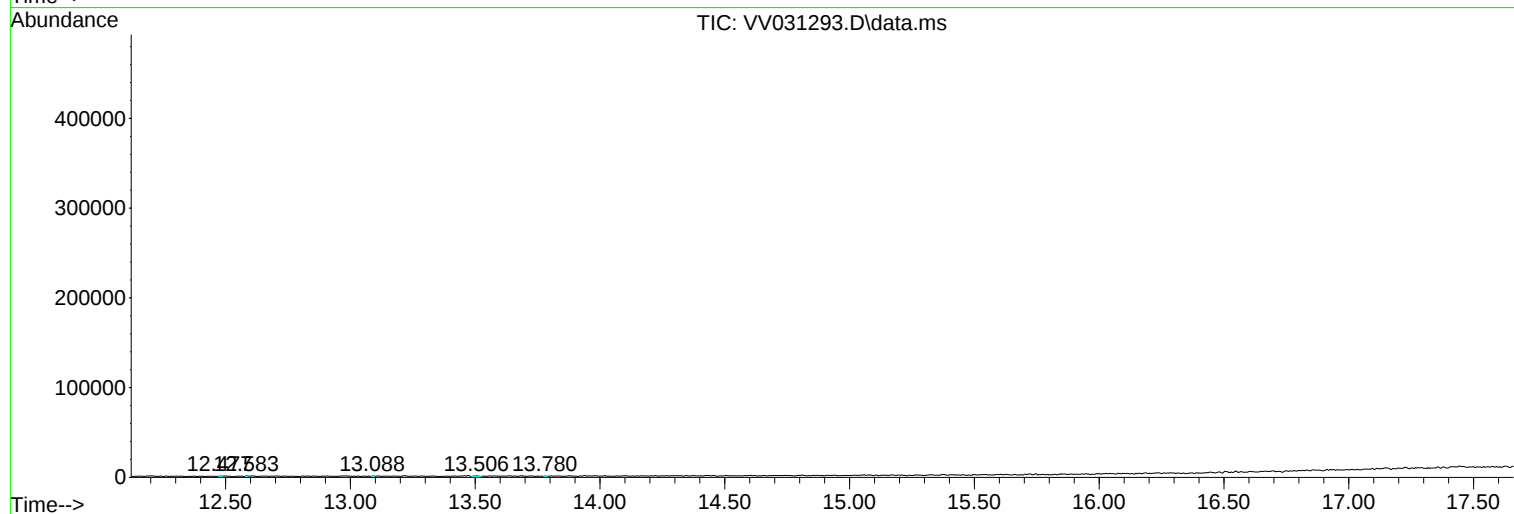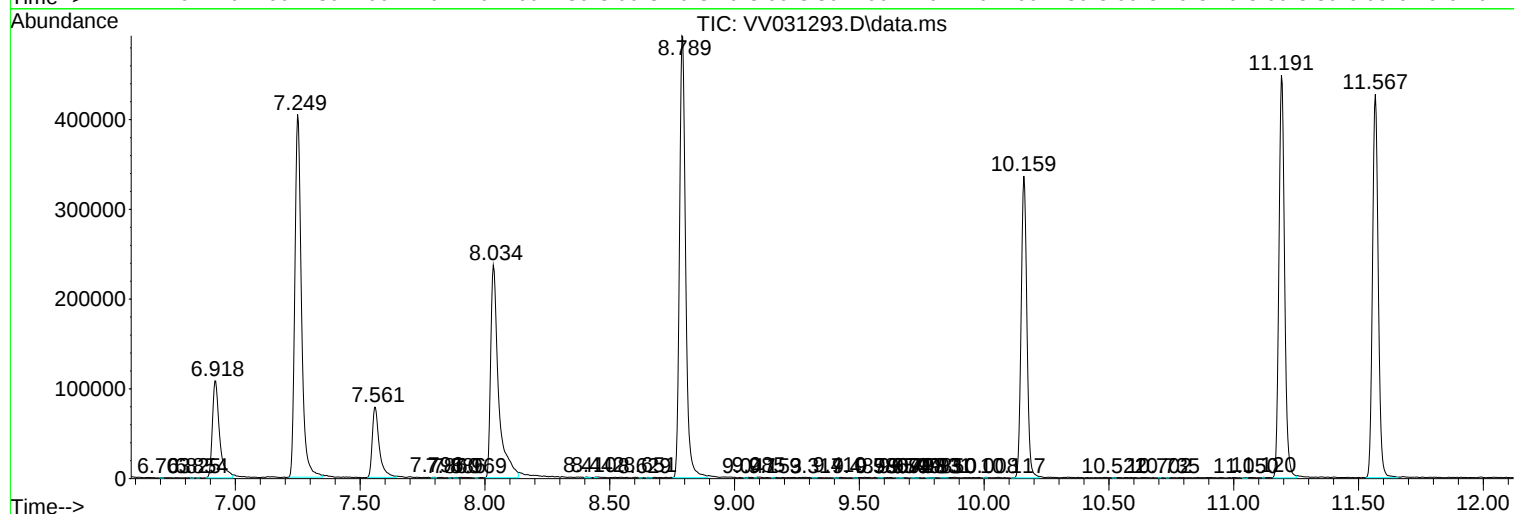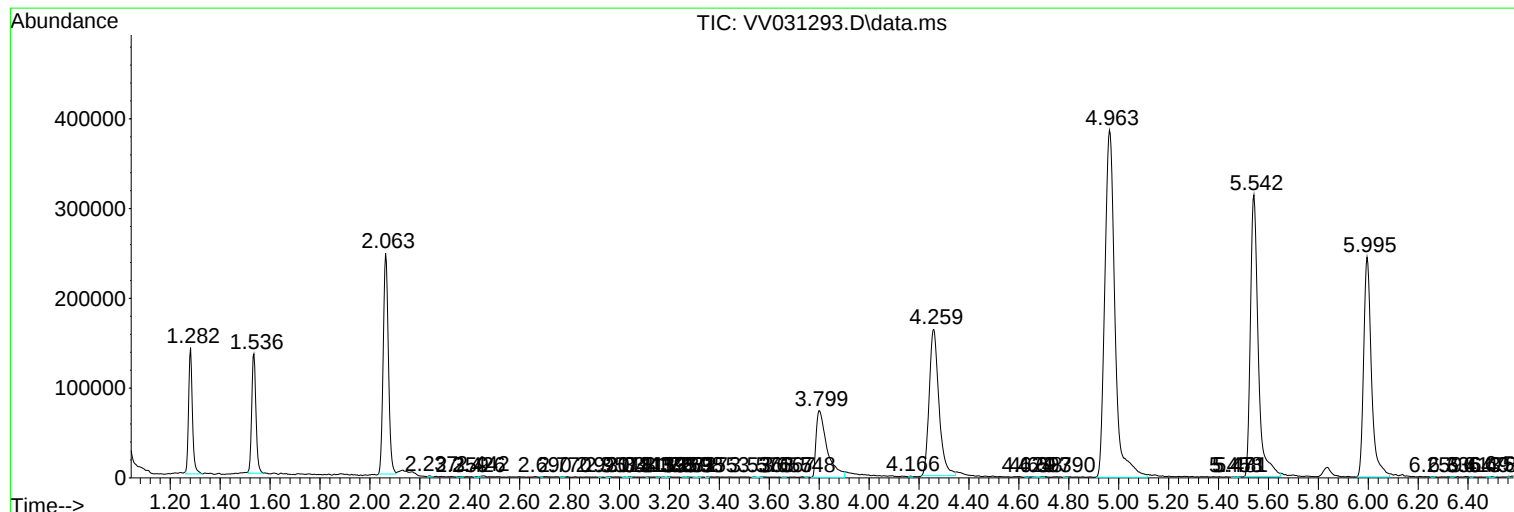

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053123\
Data File : VV031293.D
Acq On : 31 May 2023 13:51
Operator : SY/MD
Sample : 02961-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FP5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053123\
Data File : VV031293.D
Acq On : 31 May 2023 13:51
Operator : SY/MD
Sample : 02961-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FP5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------