

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053123\
 Data File : VV031300.D
 Acq On : 31 May 2023 16:37
 Operator : SY/MD
 Sample : 02961-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FQ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031300.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	90	rVB	127383	136602	13.61%	1.739%
2	1.536	147	154	165	rVB	124220	142800	14.23%	1.818%
3	2.063	309	318	331	rBV	228109	327954	32.68%	4.175%
4	2.314	394	396	398	rBV2	479	231	0.02%	0.003%
5	2.452	432	439	448	rBV8	1412	2171	0.22%	0.028%
6	2.703	513	517	518	rBV	476	358	0.04%	0.005%
7	2.764	534	536	540	rBV3	492	289	0.03%	0.004%
8	2.986	602	605	606	rBV	491	219	0.02%	0.003%
9	3.021	613	616	619	rVB2	350	201	0.02%	0.003%
10	3.037	619	621	622	rBV2	347	153	0.02%	0.002%
11	3.089	635	637	642	rVB	455	400	0.04%	0.005%
12	3.117	642	646	649	rBV3	589	362	0.04%	0.005%
13	3.134	649	651	652	rBV3	260	104	0.01%	0.001%
14	3.201	670	672	674	rBV2	269	121	0.01%	0.002%
15	3.217	674	677	679	rVB2	542	260	0.03%	0.003%
16	3.323	707	710	711	rBV	221	140	0.01%	0.002%
17	3.355	716	720	725	rBV2	593	482	0.05%	0.006%
18	3.484	757	760	763	rVB2	494	281	0.03%	0.004%
19	3.507	763	767	768	rBV	391	250	0.02%	0.003%
20	3.574	785	788	792	rVB	434	261	0.03%	0.003%
21	3.632	802	806	810	rVB3	429	337	0.03%	0.004%
22	3.670	814	818	820	rBV	213	162	0.02%	0.002%
23	3.706	826	829	830	rBV	224	111	0.01%	0.001%
24	3.732	834	837	843	rVB3	342	264	0.03%	0.003%
25	3.764	843	847	849	rBV2	587	379	0.04%	0.005%
26	3.799	849	858	891	rBV	75116	221633	22.09%	2.821%
27	4.259	984	1001	1024	rBV2	154849	427761	42.63%	5.446%
28	4.478	1067	1069	1070	rBV2	599	285	0.03%	0.004%
29	4.571	1097	1098	1100	rBV	311	123	0.01%	0.002%
30	4.645	1118	1121	1123	rBV4	395	281	0.03%	0.004%
31	4.831	1176	1179	1182	rBV2	329	217	0.02%	0.003%
32	4.876	1191	1193	1197	rBV2	418	299	0.03%	0.004%
33	4.966	1203	1221	1246	rBV2	364692	1003482	100.00%	12.775%
34	5.272	1312	1316	1318	rBV2	813	572	0.06%	0.007%
35	5.326	1330	1333	1337	rBV5	562	476	0.05%	0.006%
36	5.346	1337	1339	1342	rVB3	570	226	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053123\
 Data File : VV031300.D
 Acq On : 31 May 2023 16:37
 Operator : SY/MD
 Sample : 02961-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FQ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	5.445	1368	1370	1372	rBV	306	161	0.02%	0.002%
38	5.465	1372	1376	1380	rBV4	526	504	0.05%	0.006%
39	5.542	1385	1400	1437	rBV	326496	711422	70.90%	9.057%
40	5.831	1481	1490	1505	rVB2	11204	24671	2.46%	0.314%
41	5.928	1518	1520	1527	rVB3	393	332	0.03%	0.004%
42	5.995	1527	1541	1575	rBV	234056	512277	51.05%	6.522%
43	6.259	1619	1623	1627	rVB3	471	400	0.04%	0.005%
44	6.275	1627	1628	1630	rVB	386	125	0.01%	0.002%
45	6.288	1630	1632	1635	rBV3	778	413	0.04%	0.005%
46	6.301	1635	1636	1637	rBV3	414	128	0.01%	0.002%
47	6.352	1647	1652	1656	rBV5	665	716	0.07%	0.009%
48	6.445	1676	1681	1686	rBV2	615	570	0.06%	0.007%
49	6.522	1703	1705	1706	rBV2	443	195	0.02%	0.002%
50	6.641	1740	1742	1744	rBV2	461	199	0.02%	0.003%
51	6.722	1766	1767	1771	rVB	587	251	0.03%	0.003%
52	6.744	1771	1774	1775	rBV2	324	177	0.02%	0.002%
53	6.773	1780	1783	1784	rBV	319	192	0.02%	0.002%
54	6.921	1818	1829	1855	rBV	102868	206094	20.54%	2.624%
55	7.092	1879	1882	1886	rBV3	955	866	0.09%	0.011%
56	7.252	1919	1932	1962	rBV	381538	702144	69.97%	8.939%
57	7.561	2018	2028	2052	rBV	75768	144443	14.39%	1.839%
58	7.764	2088	2091	2096	rBV4	914	842	0.08%	0.011%
59	7.805	2101	2104	2106	rBV3	764	475	0.05%	0.006%
60	7.857	2118	2120	2125	rVB2	482	318	0.03%	0.004%
61	7.905	2132	2135	2136	rBV2	234	118	0.01%	0.002%
62	7.989	2160	2161	2164	rVB2	336	146	0.01%	0.002%
63	8.034	2165	2175	2212	rBV	229317	504297	50.25%	6.420%
64	8.346	2270	2272	2274	rBV2	644	201	0.02%	0.003%
65	8.468	2305	2310	2311	rBV2	620	522	0.05%	0.007%
66	8.526	2325	2328	2331	rBV4	565	390	0.04%	0.005%
67	8.571	2339	2342	2344	rBV3	526	293	0.03%	0.004%
68	8.628	2358	2360	2363	rBV2	402	266	0.03%	0.003%
69	8.683	2373	2377	2379	rVB3	622	342	0.03%	0.004%
70	8.792	2398	2411	2436	rBV	499311	854279	85.13%	10.875%
71	9.127	2514	2515	2518	rBV	268	152	0.02%	0.002%
72	9.246	2550	2552	2554	rBV2	225	96	0.01%	0.001%
73	9.374	2586	2592	2594	rBV4	637	662	0.07%	0.008%
74	9.445	2612	2614	2616	rVB	378	140	0.01%	0.002%
75	9.532	2639	2641	2645	rVB3	345	200	0.02%	0.003%
76	9.558	2647	2649	2650	rBV3	445	189	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053123\
 Data File : VV031300.D
 Acq On : 31 May 2023 16:37
 Operator : SY/MD
 Sample : 02961-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FQ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	9.580	2654	2656	2661	rVB2	570	319	0.03%	0.004%
78	9.622	2667	2669	2671	rBV2	233	133	0.01%	0.002%
79	9.677	2684	2686	2690	rVB2	678	364	0.04%	0.005%
80	9.825	2730	2732	2735	rVB2	417	157	0.02%	0.002%
81	9.963	2772	2775	2777	rBV2	323	210	0.02%	0.003%
82	10.024	2792	2794	2797	rBV2	506	295	0.03%	0.004%
83	10.043	2798	2800	2806	rVB3	643	533	0.05%	0.007%
84	10.159	2824	2836	2857	rBV	326421	516027	51.42%	6.569%
85	10.252	2863	2865	2870	rVB3	896	572	0.06%	0.007%
86	10.442	2919	2924	2928	rBV2	406	471	0.05%	0.006%
87	10.609	2972	2976	2979	rBV3	318	263	0.03%	0.003%
88	10.741	3014	3017	3019	rBV2	460	323	0.03%	0.004%
89	10.799	3031	3035	3040	rBV2	501	458	0.05%	0.006%
90	10.831	3040	3045	3048	rBV4	660	634	0.06%	0.008%
91	11.043	3107	3111	3114	rVB2	587	387	0.04%	0.005%
92	11.062	3114	3117	3119	rBV	528	266	0.03%	0.003%
93	11.191	3146	3157	3183	rBV	460489	734872	73.23%	9.355%
94	11.567	3263	3274	3293	rBV	406467	654411	65.21%	8.331%
95	12.172	3460	3462	3463	rBV	497	181	0.02%	0.002%
96	13.181	3773	3776	3778	rBV2	570	340	0.03%	0.004%
97	13.214	3782	3786	3791	rVV4	770	749	0.07%	0.010%
98	13.461	3858	3863	3870	rBV5	1077	1415	0.14%	0.018%
99	13.853	3980	3985	3988	rBV3	706	740	0.07%	0.009%
100	14.291	4119	4121	4127	rBV2	723	614	0.06%	0.008%




Sum of corrected areas: 7855189

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053123\
Data File : VV031300.D
Acq On : 31 May 2023 16:37
Operator : SY/MD
Sample : 02961-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FQ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

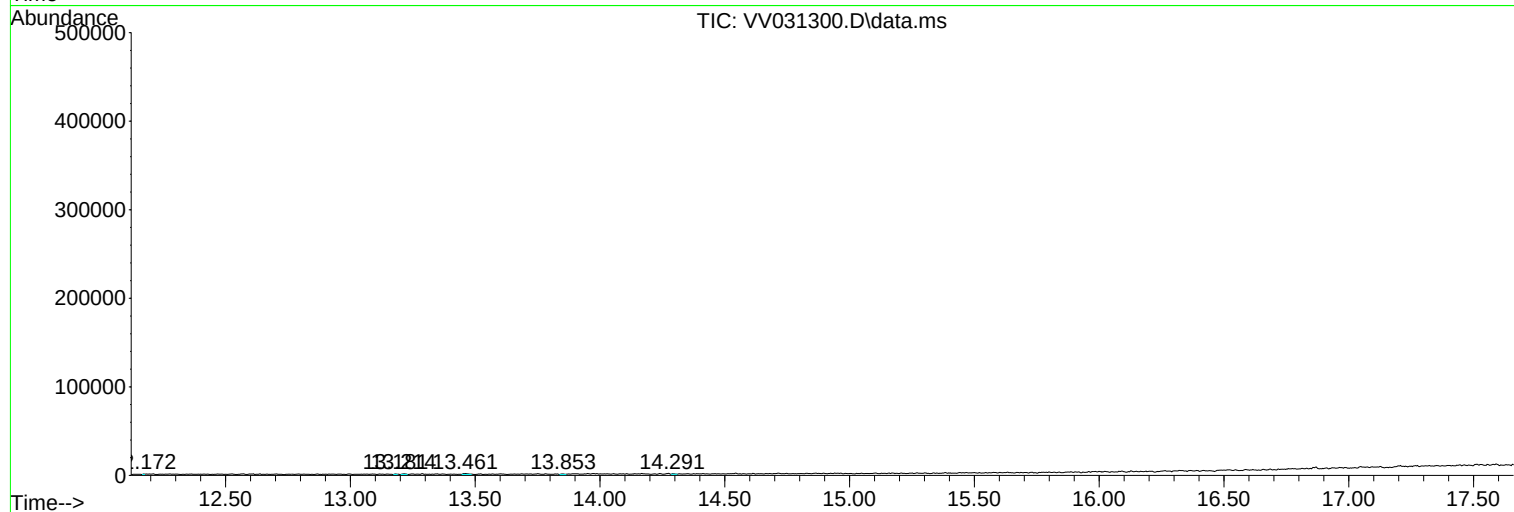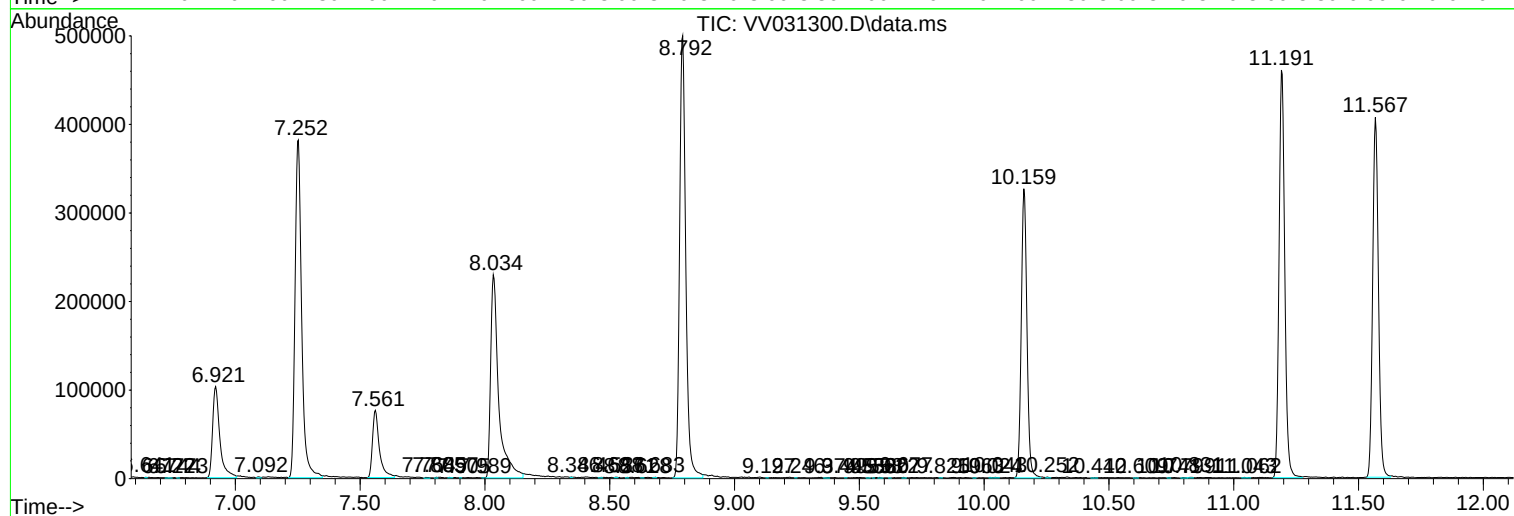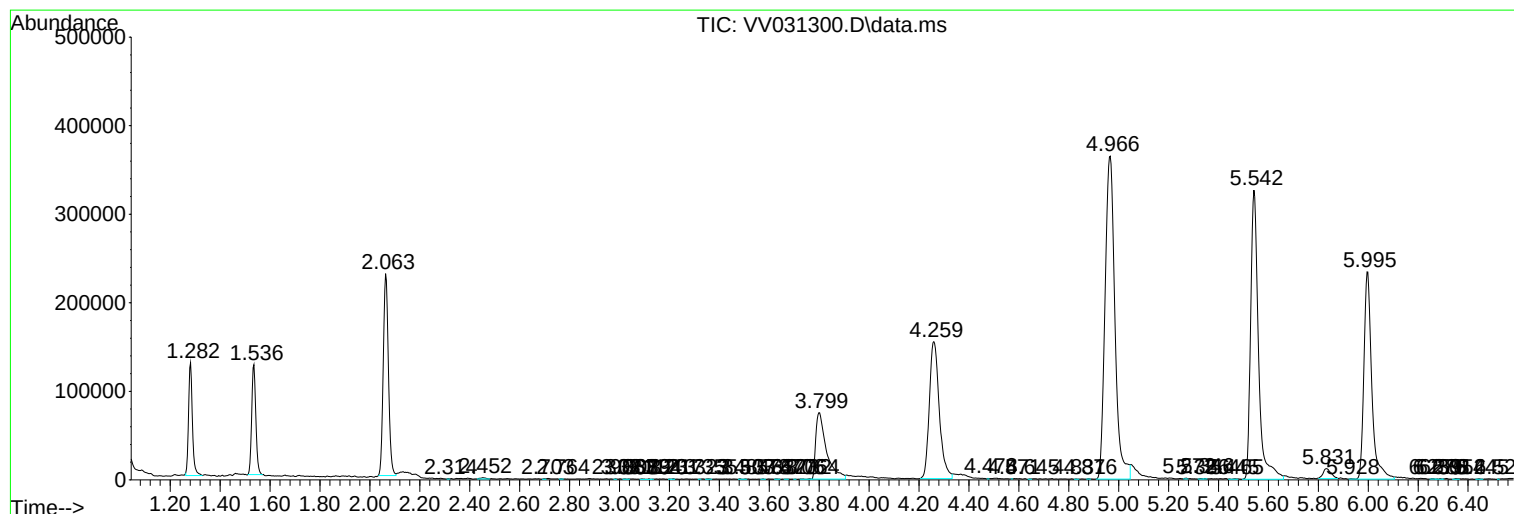

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053123\
Data File : VV031300.D
Acq On : 31 May 2023 16:37
Operator : SY/MD
Sample : 02961-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FQ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053123\
Data File : VV031300.D
Acq On : 31 May 2023 16:37
Operator : SY/MD
Sample : 02961-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FQ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------