

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053123\
 Data File : VV031303.D
 Acq On : 31 May 2023 17:50
 Operator : SY/MD
 Sample : 02961-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FQ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031303.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	87	rVB	129301	137696	13.36%	1.720%
2	1.536	147	154	168	rVB	129875	153415	14.89%	1.916%
3	2.063	309	318	332	rBV	232266	335583	32.57%	4.191%
4	2.378	414	416	422	rVB2	720	577	0.06%	0.007%
5	2.455	435	440	448	rVB6	1324	1800	0.17%	0.022%
6	2.545	466	468	470	rVB2	311	119	0.01%	0.001%
7	2.648	496	500	502	rBV2	641	459	0.04%	0.006%
8	2.953	591	595	597	rBV	515	458	0.04%	0.006%
9	2.995	604	608	610	rBV3	408	347	0.03%	0.004%
10	3.034	618	620	626	rVB2	337	222	0.02%	0.003%
11	3.063	626	629	631	rBV	332	211	0.02%	0.003%
12	3.079	631	634	637	rVV2	532	453	0.04%	0.006%
13	3.105	641	642	648	rVB2	430	281	0.03%	0.004%
14	3.269	691	693	698	rBV2	564	314	0.03%	0.004%
15	3.343	712	716	719	rBV2	399	295	0.03%	0.004%
16	3.362	720	722	724	rBV	276	149	0.01%	0.002%
17	3.462	751	753	756	rVB2	356	208	0.02%	0.003%
18	3.555	779	782	785	rBV2	604	285	0.03%	0.004%
19	3.574	785	788	790	rVB3	548	267	0.03%	0.003%
20	3.590	790	793	796	rVB2	607	365	0.04%	0.005%
21	3.603	796	797	798	rBV	249	95	0.01%	0.001%
22	3.616	798	801	806	rVB2	510	451	0.04%	0.006%
23	3.648	806	811	813	rBV3	521	411	0.04%	0.005%
24	3.661	813	815	818	rVB	427	178	0.02%	0.002%
25	3.690	822	824	825	rBV	366	159	0.02%	0.002%
26	3.751	839	843	844	rBV	289	227	0.02%	0.003%
27	3.764	845	847	849	rBV	406	171	0.02%	0.002%
28	3.799	849	858	887	rBV	78803	225988	21.93%	2.823%
29	4.259	986	1001	1025	rBV	157823	431218	41.85%	5.386%
30	4.703	1137	1139	1142	rBV3	464	230	0.02%	0.003%
31	4.767	1156	1159	1165	rVB2	882	615	0.06%	0.008%
32	4.793	1165	1167	1168	rBV	475	168	0.02%	0.002%
33	4.818	1173	1175	1179	rVB3	527	328	0.03%	0.004%
34	4.854	1184	1186	1188	rVB	310	144	0.01%	0.002%
35	4.870	1188	1191	1195	rBV2	513	451	0.04%	0.006%
36	4.886	1195	1196	1198	rBV	322	111	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW053123\
 Data File : VW031303.D
 Acq On : 31 May 2023 17:50
 Operator : SY/MD
 Sample : 02961-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FQ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	4.963	1204	1220	1244	rBV2	380735	1030438	100.00%	12.870%
38	5.359	1340	1343	1347	rVB4	525	412	0.04%	0.005%
39	5.384	1347	1351	1353	rBV3	488	347	0.03%	0.004%
40	5.458	1372	1374	1377	rVB2	575	272	0.03%	0.003%
41	5.542	1388	1400	1436	rBV	325351	706912	68.60%	8.829%
42	5.834	1479	1491	1503	rBV4	12470	27877	2.71%	0.348%
43	5.995	1526	1541	1572	rBV	243180	529800	51.42%	6.617%
44	6.252	1618	1621	1623	rBV4	488	317	0.03%	0.004%
45	6.294	1632	1634	1637	rBV3	355	212	0.02%	0.003%
46	6.339	1646	1648	1651	rVB2	478	260	0.03%	0.003%
47	6.362	1651	1655	1658	rBV2	389	361	0.04%	0.005%
48	6.384	1658	1662	1664	rBV	416	286	0.03%	0.004%
49	6.429	1674	1676	1680	rVV	367	259	0.03%	0.003%
50	6.564	1714	1718	1719	rBV2	791	524	0.05%	0.007%
51	6.641	1737	1742	1745	rBV3	1026	764	0.07%	0.010%
52	6.670	1747	1751	1753	rBV3	675	501	0.05%	0.006%
53	6.731	1764	1770	1772	rBV3	587	522	0.05%	0.007%
54	6.760	1776	1779	1783	rVB3	439	319	0.03%	0.004%
55	6.786	1783	1787	1788	rBV2	341	233	0.02%	0.003%
56	6.822	1795	1798	1804	rVB2	340	253	0.02%	0.003%
57	6.921	1818	1829	1857	rBV2	105407	210547	20.43%	2.630%
58	7.252	1919	1932	1962	rBV	392652	722750	70.14%	9.027%
59	7.561	2018	2028	2056	rBV	78849	152127	14.76%	1.900%
60	7.799	2099	2102	2103	rBV2	438	284	0.03%	0.004%
61	7.870	2122	2124	2127	rBV3	480	346	0.03%	0.004%
62	7.931	2141	2143	2148	rVB3	459	354	0.03%	0.004%
63	8.034	2165	2175	2211	rBV	245644	523842	50.84%	6.543%
64	8.696	2378	2381	2386	rVB3	681	550	0.05%	0.007%
65	8.728	2386	2391	2392	rBV2	441	347	0.03%	0.004%
66	8.792	2399	2411	2432	rBV	505020	851024	82.59%	10.629%
67	9.075	2495	2499	2501	rBV3	447	355	0.03%	0.004%
68	9.156	2522	2524	2526	rBV2	529	323	0.03%	0.004%
69	9.262	2554	2557	2559	rBV	478	223	0.02%	0.003%
70	9.381	2590	2594	2597	rBV2	372	320	0.03%	0.004%
71	9.410	2601	2603	2609	rVB2	445	359	0.03%	0.004%
72	9.439	2609	2612	2613	rBV2	385	190	0.02%	0.002%
73	9.609	2662	2665	2669	rVB3	873	504	0.05%	0.006%
74	9.664	2681	2682	2683	rBV3	330	116	0.01%	0.001%
75	9.731	2698	2703	2708	rVB4	668	725	0.07%	0.009%
76	9.773	2708	2716	2718	rBV3	484	572	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053123\
 Data File : VV031303.D
 Acq On : 31 May 2023 17:50
 Operator : SY/MD
 Sample : 02961-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FQ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	9.850	2737	2740	2741	rBV	333	139	0.01%	0.002%
78	9.905	2755	2757	2758	rBV	429	198	0.02%	0.002%
79	9.982	2778	2781	2784	rBV3	271	227	0.02%	0.003%
80	10.046	2799	2801	2803	rBV2	398	249	0.02%	0.003%
81	10.082	2807	2812	2815	rVB3	492	467	0.05%	0.006%
82	10.159	2825	2836	2861	rBV	334325	534026	51.83%	6.670%
83	10.397	2908	2910	2913	rBV3	284	178	0.02%	0.002%
84	10.445	2923	2925	2928	rBV3	477	298	0.03%	0.004%
85	10.526	2947	2950	2955	rVB2	484	324	0.03%	0.004%
86	10.796	3031	3034	3035	rBV	349	189	0.02%	0.002%
87	10.815	3037	3040	3046	rBV3	476	431	0.04%	0.005%
88	10.866	3052	3056	3058	rBV2	606	523	0.05%	0.007%
89	10.924	3072	3074	3075	rBV	402	142	0.01%	0.002%
90	10.998	3095	3097	3099	rBV	325	151	0.01%	0.002%
91	11.034	3104	3108	3111	rBV3	528	492	0.05%	0.006%
92	11.194	3144	3158	3183	rBV	456676	733341	71.17%	9.159%
93	11.567	3263	3274	3294	rBV	420347	670584	65.08%	8.376%
94	11.796	3340	3345	3348	rBV4	635	617	0.06%	0.008%
95	12.034	3414	3419	3421	rBV4	567	471	0.05%	0.006%
96	12.619	3597	3601	3603	rBV2	577	337	0.03%	0.004%
97	12.763	3642	3646	3652	rVB4	698	800	0.08%	0.010%
98	12.789	3652	3654	3656	rBV	412	240	0.02%	0.003%
99	12.908	3688	3691	3694	rBV3	758	513	0.05%	0.006%
100	13.259	3797	3800	3802	rBV	511	315	0.03%	0.004%




Sum of corrected areas: 8006428

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053123\
Data File : VV031303.D
Acq On : 31 May 2023 17:50
Operator : SY/MD
Sample : 02961-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FQ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

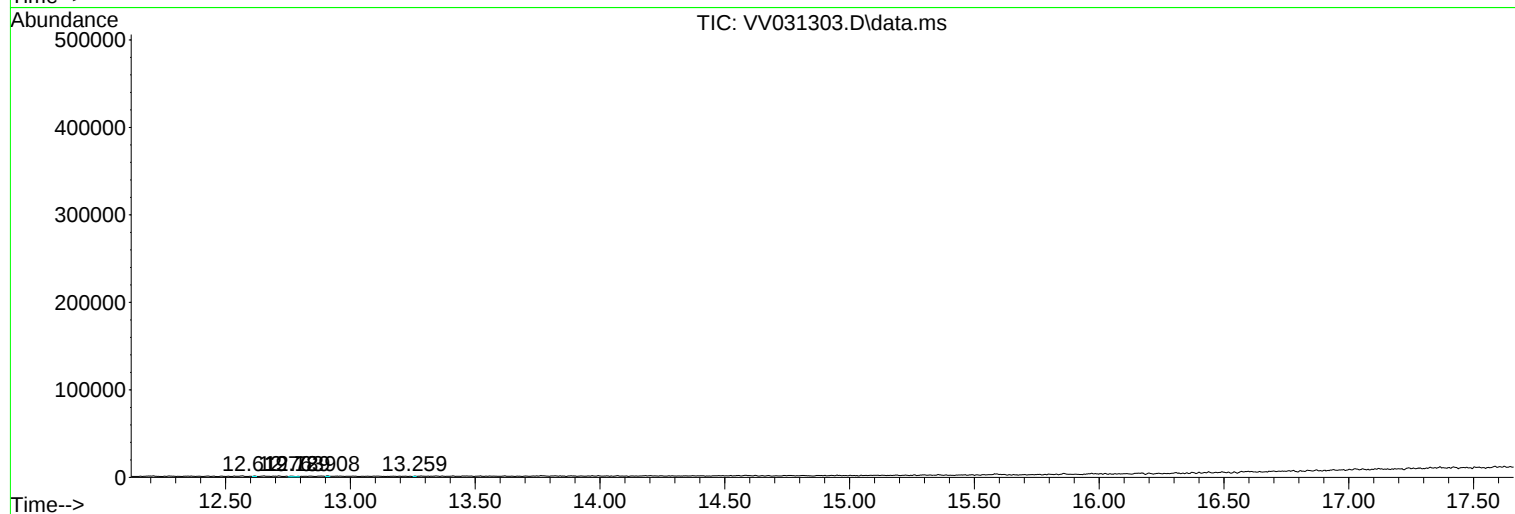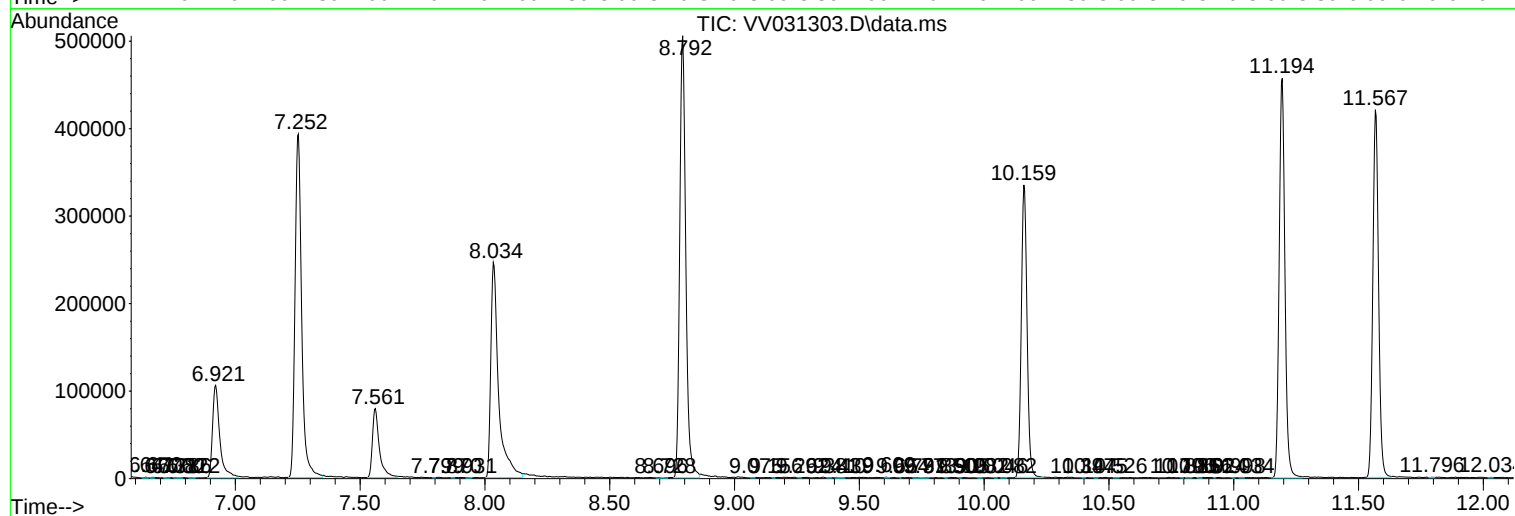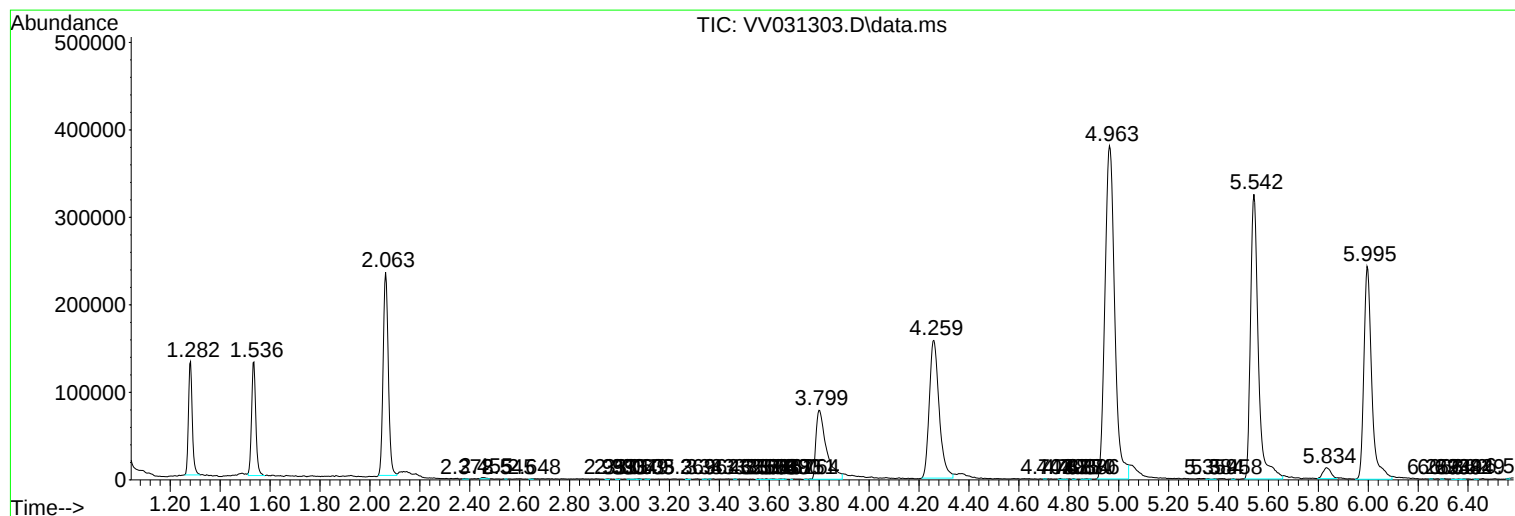

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053123\
Data File : VV031303.D
Acq On : 31 May 2023 17:50
Operator : SY/MD
Sample : 02961-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FQ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053123\
Data File : VV031303.D
Acq On : 31 May 2023 17:50
Operator : SY/MD
Sample : 02961-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FQ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------