

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053123\
 Data File : VV031304.D
 Acq On : 31 May 2023 18:14
 Operator : SY/MD
 Sample : 02961-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FP2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031304.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	69	74	88	rVB	84735	91622	11.23%	1.423%
2	1.532	147	153	165	rVB	93019	110922	13.60%	1.722%
3	2.063	309	318	330	rBV	158496	230352	28.24%	3.577%
4	2.452	435	439	445	rVB6	1160	1344	0.16%	0.021%
5	2.687	510	512	513	rBV6	372	169	0.02%	0.003%
6	2.799	543	547	550	rBV2	773	522	0.06%	0.008%
7	2.822	550	554	555	rBV2	360	207	0.03%	0.003%
8	2.867	567	568	573	rBV4	365	257	0.03%	0.004%
9	2.966	597	599	602	rVB3	376	159	0.02%	0.002%
10	2.998	608	609	611	rBV	399	150	0.02%	0.002%
11	3.101	638	641	642	rBV	793	371	0.05%	0.006%
12	3.137	650	652	654	rBV2	325	165	0.02%	0.003%
13	3.220	675	678	682	rVB4	428	345	0.04%	0.005%
14	3.404	733	735	737	rBV2	281	173	0.02%	0.003%
15	3.490	758	762	763	rBV	287	196	0.02%	0.003%
16	3.500	763	765	768	rVB2	482	296	0.04%	0.005%
17	3.545	773	779	782	rBV4	567	527	0.06%	0.008%
18	3.593	791	794	799	rVB3	395	300	0.04%	0.005%
19	3.625	799	804	807	rBV2	533	579	0.07%	0.009%
20	3.728	832	836	838	rBV3	287	215	0.03%	0.003%
21	3.799	849	858	888	rBV	77995	235176	28.83%	3.652%
22	4.259	984	1001	1021	rBV	131525	352855	43.26%	5.479%
23	4.709	1139	1141	1144	rBV2	388	205	0.03%	0.003%
24	4.809	1169	1172	1174	rVB2	445	229	0.03%	0.004%
25	4.822	1174	1176	1180	rVB3	820	455	0.06%	0.007%
26	4.841	1180	1182	1189	rBV3	539	487	0.06%	0.008%
27	4.876	1190	1193	1195	rBV3	385	296	0.04%	0.005%
28	4.966	1202	1221	1242	rBV2	300545	815694	100.00%	12.666%
29	5.223	1299	1301	1305	rVB5	936	620	0.08%	0.010%
30	5.330	1330	1334	1335	rBV3	560	386	0.05%	0.006%
31	5.339	1335	1337	1338	rBV	499	161	0.02%	0.003%
32	5.404	1355	1357	1360	rVB3	806	429	0.05%	0.007%
33	5.542	1387	1400	1418	rBV	250482	522302	64.03%	8.110%
34	5.834	1480	1491	1502	rBV5	9604	20764	2.55%	0.322%
35	5.998	1526	1542	1570	rBV	193864	431108	52.85%	6.694%
36	6.249	1618	1620	1623	rBV	394	208	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW053123\
 Data File : VW031304.D
 Acq On : 31 May 2023 18:14
 Operator : SY/MD
 Sample : 02961-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FP2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	6.297	1629	1635	1637	rBV2	688	649	0.08%	0.010%
38	6.358	1652	1654	1656	rBV2	411	184	0.02%	0.003%
39	6.391	1660	1664	1666	rBV3	365	305	0.04%	0.005%
40	6.445	1679	1681	1685	rBV4	392	258	0.03%	0.004%
41	6.510	1697	1701	1704	rBV2	273	248	0.03%	0.004%
42	6.571	1716	1720	1722	rBV3	825	625	0.08%	0.010%
43	6.738	1770	1772	1775	rBV2	512	278	0.03%	0.004%
44	6.757	1775	1778	1779	rVB	524	283	0.03%	0.004%
45	6.789	1785	1788	1789	rBV2	319	170	0.02%	0.003%
46	6.866	1810	1812	1818	rVB2	655	439	0.05%	0.007%
47	6.921	1818	1829	1855	rBV	84338	175560	21.52%	2.726%
48	7.175	1906	1908	1909	rBV	408	154	0.02%	0.002%
49	7.252	1920	1932	1963	rBV	288711	543667	66.65%	8.442%
50	7.468	1998	1999	2002	rBV2	391	268	0.03%	0.004%
51	7.522	2014	2016	2018	rBV2	564	215	0.03%	0.003%
52	7.561	2018	2028	2055	rBV	64886	125406	15.37%	1.947%
53	7.780	2094	2096	2100	rBV3	426	308	0.04%	0.005%
54	7.825	2108	2110	2113	rBV2	517	237	0.03%	0.004%
55	7.873	2120	2125	2126	rBV5	2978	2115	0.26%	0.033%
56	7.979	2156	2158	2160	rBV2	319	207	0.03%	0.003%
57	8.034	2165	2175	2208	rBV	227893	478515	58.66%	7.431%
58	8.648	2364	2366	2368	rBV2	319	179	0.02%	0.003%
59	8.718	2385	2388	2391	rBV2	344	207	0.03%	0.003%
60	8.792	2399	2411	2437	rBV	405098	688896	84.46%	10.697%
61	9.018	2477	2481	2484	rVB3	943	619	0.08%	0.010%
62	9.040	2484	2488	2491	rBV3	654	541	0.07%	0.008%
63	9.079	2498	2500	2501	rBV2	295	147	0.02%	0.002%
64	9.124	2513	2514	2518	rVB	395	219	0.03%	0.003%
65	9.146	2518	2521	2522	rBV	520	287	0.04%	0.004%
66	9.198	2533	2537	2540	rBV3	521	442	0.05%	0.007%
67	9.291	2564	2566	2568	rBV2	390	214	0.03%	0.003%
68	9.336	2578	2580	2586	rVB3	439	449	0.06%	0.007%
69	9.365	2586	2589	2592	rBV2	732	503	0.06%	0.008%
70	9.410	2600	2603	2604	rBV	445	256	0.03%	0.004%
71	9.448	2612	2615	2617	rBV	525	351	0.04%	0.005%
72	9.590	2657	2659	2664	rVB3	495	343	0.04%	0.005%
73	9.735	2703	2704	2708	rBV	414	289	0.04%	0.004%
74	9.825	2730	2732	2733	rBV	391	175	0.02%	0.003%
75	9.879	2746	2749	2752	rBV3	531	297	0.04%	0.005%
76	9.911	2757	2759	2761	rBV2	578	309	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053123\
 Data File : VV031304.D
 Acq On : 31 May 2023 18:14
 Operator : SY/MD
 Sample : 02961-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0FP2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	9.972	2775	2778	2780	rBV	582	367	0.04%	0.006%
78	10.050	2797	2802	2806	rBV3	610	664	0.08%	0.010%
79	10.108	2818	2820	2822	rBV	477	199	0.02%	0.003%
80	10.159	2825	2836	2852	rBV	292574	471564	57.81%	7.323%
81	10.333	2881	2890	2900	rBV4	6987	10857	1.33%	0.169%
82	10.429	2918	2920	2922	rBV	461	157	0.02%	0.002%
83	10.574	2961	2965	2968	rBV2	395	365	0.04%	0.006%
84	10.616	2975	2978	2981	rVB2	500	351	0.04%	0.005%
85	10.632	2981	2983	2989	rVB2	740	443	0.05%	0.007%
86	10.661	2989	2992	2994	rBV	619	399	0.05%	0.006%
87	10.751	3017	3020	3023	rVB3	564	311	0.04%	0.005%
88	10.866	3053	3056	3059	rBV3	676	435	0.05%	0.007%
89	11.059	3115	3116	3118	rBV2	281	150	0.02%	0.002%
90	11.191	3147	3157	3179	rBV	361894	575674	70.57%	8.939%
91	11.567	3262	3274	3295	rBV	332726	528382	64.78%	8.205%
92	11.876	3367	3370	3373	rBV3	526	388	0.05%	0.006%
93	12.030	3415	3418	3419	rBV2	524	223	0.03%	0.003%
94	12.300	3500	3502	3504	rBV2	551	291	0.04%	0.005%
95	12.374	3522	3525	3529	rVB4	600	436	0.05%	0.007%
96	12.770	3645	3648	3649	rBV	459	238	0.03%	0.004%
97	13.217	3783	3787	3792	rBV6	1200	1263	0.15%	0.020%
98	13.869	3987	3990	3992	rBV3	720	528	0.06%	0.008%
99	13.937	4008	4011	4014	rBV2	990	659	0.08%	0.010%
100	14.037	4039	4042	4045	rBV2	627	458	0.06%	0.007%




Sum of corrected areas: 6439862

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053123\
Data File : VV031304.D
Acq On : 31 May 2023 18:14
Operator : SY/MD
Sample : 02961-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FP2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

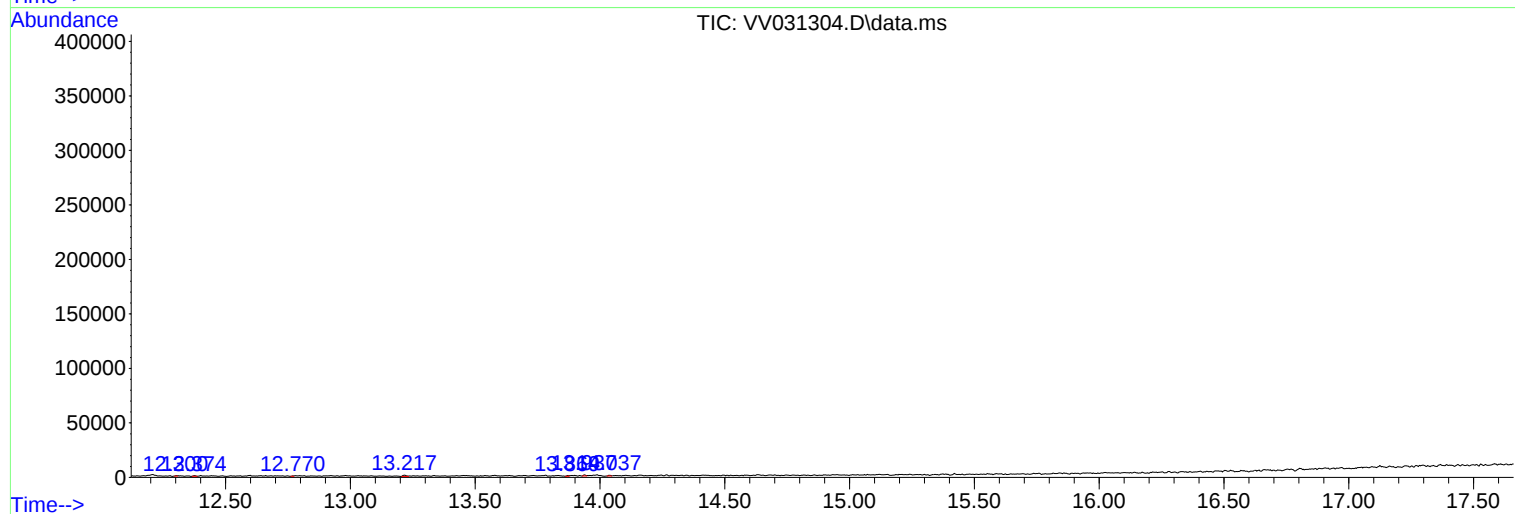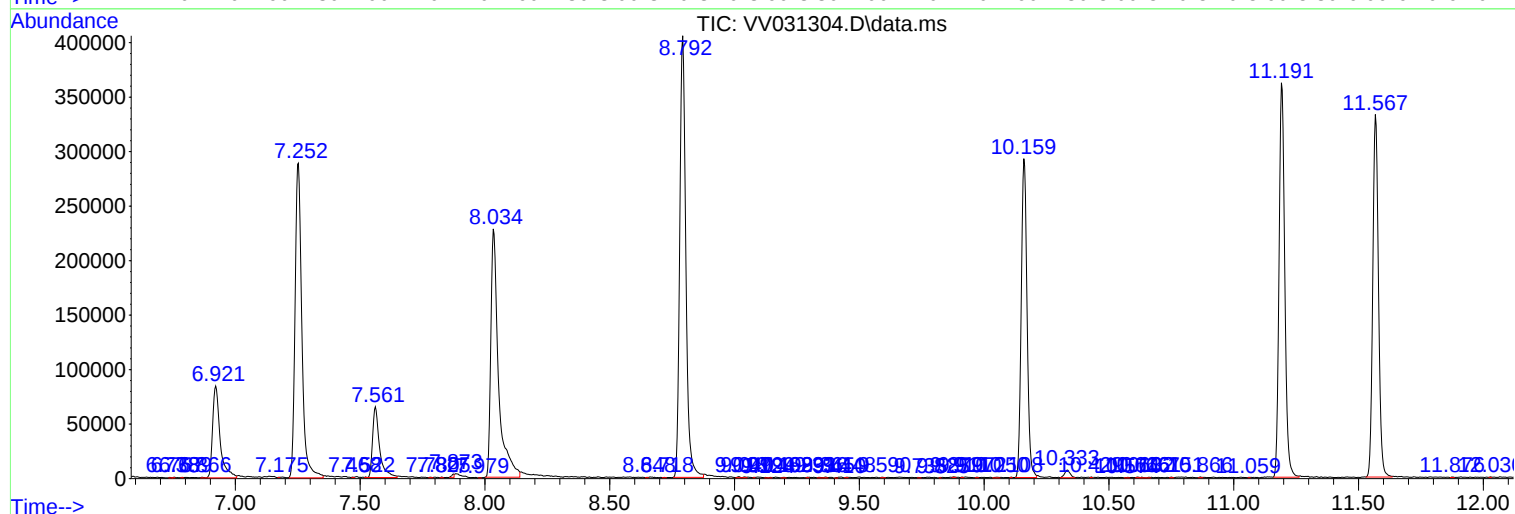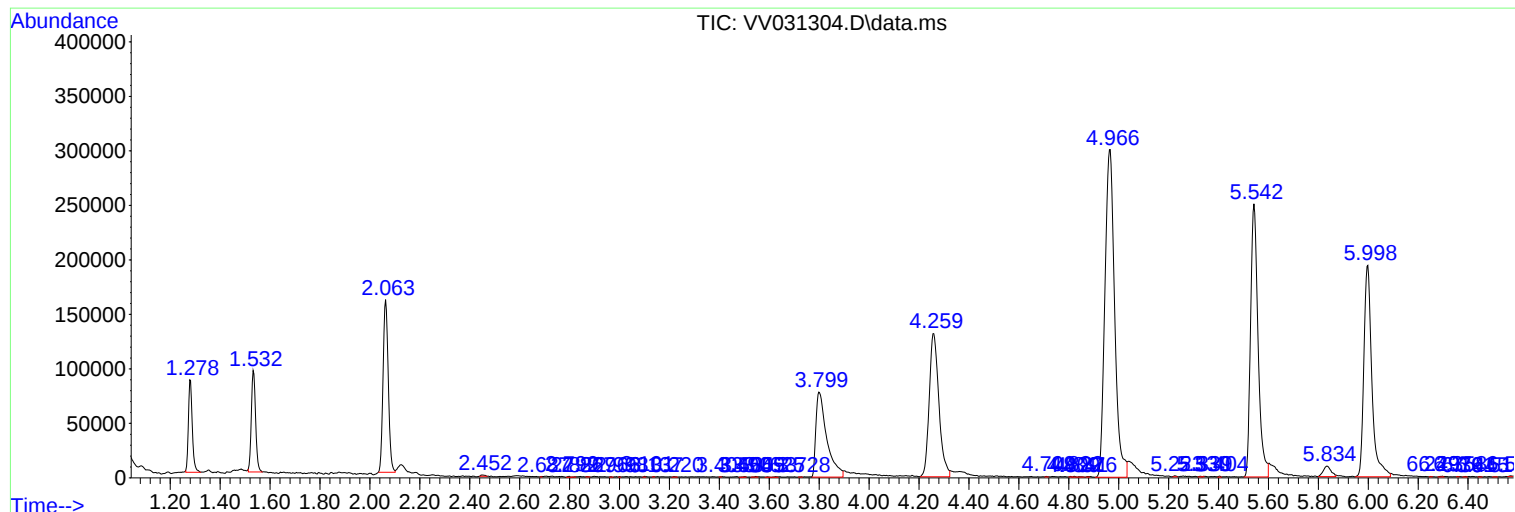

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053123\
Data File : VV031304.D
Acq On : 31 May 2023 18:14
Operator : SY/MD
Sample : 02961-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FP2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053123\
Data File : VV031304.D
Acq On : 31 May 2023 18:14
Operator : SY/MD
Sample : 02961-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0FP2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------