

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053123\
 Data File : VV031305.D
 Acq On : 31 May 2023 18:38
 Operator : SY/MD
 Sample : 02991-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C18

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031305.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	92	rVB	123287	131899	13.08%	1.633%
2	1.532	147	153	165	rVB	124285	144393	14.32%	1.788%
3	2.063	308	318	331	rBV	227632	331917	32.93%	4.110%
4	2.497	450	453	456	rBV2	663	502	0.05%	0.006%
5	2.590	479	482	487	rBV4	810	695	0.07%	0.009%
6	2.712	512	520	536	rVB4	4321	9405	0.93%	0.116%
7	2.793	543	545	550	rVB3	424	279	0.03%	0.003%
8	2.815	550	552	555	rVB	416	204	0.02%	0.003%
9	2.831	555	557	559	rBV2	328	150	0.01%	0.002%
10	2.844	559	561	563	rBV2	262	106	0.01%	0.001%
11	2.896	573	577	579	rBV2	492	397	0.04%	0.005%
12	2.979	600	603	604	rBV	308	145	0.01%	0.002%
13	2.992	604	607	609	rVV	384	187	0.02%	0.002%
14	3.034	617	620	622	rBV2	402	256	0.03%	0.003%
15	3.114	642	645	646	rBV	246	121	0.01%	0.001%
16	3.233	680	682	686	rVV3	609	333	0.03%	0.004%
17	3.288	689	699	702	rBV4	500	864	0.09%	0.011%
18	3.304	702	704	706	rBV	316	135	0.01%	0.002%
19	3.342	714	716	717	rBV	227	120	0.01%	0.001%
20	3.378	724	727	728	rBV	272	150	0.01%	0.002%
21	3.391	728	731	734	rVV2	451	305	0.03%	0.004%
22	3.445	745	748	752	rVB2	252	169	0.02%	0.002%
23	3.465	752	754	756	rVB2	290	95	0.01%	0.001%
24	3.478	756	758	762	rVB	331	166	0.02%	0.002%
25	3.513	762	769	771	rBV4	414	377	0.04%	0.005%
26	3.606	795	798	800	rBV	338	210	0.02%	0.003%
27	3.661	811	815	817	rVV	257	190	0.02%	0.002%
28	3.712	828	831	832	rBV	360	223	0.02%	0.003%
29	3.764	846	847	849	rVB	281	96	0.01%	0.001%
30	3.802	849	859	885	rBV	77766	228958	22.71%	2.835%
31	4.259	986	1001	1027	rBV	154861	421769	41.84%	5.222%
32	4.609	1108	1110	1114	rVB4	657	416	0.04%	0.005%
33	4.744	1150	1152	1155	rBV2	415	319	0.03%	0.004%
34	4.770	1158	1160	1165	rBV2	259	277	0.03%	0.003%
35	4.828	1176	1178	1181	rVB2	426	231	0.02%	0.003%
36	4.844	1181	1183	1186	rBV3	327	257	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053123\
 Data File : VV031305.D
 Acq On : 31 May 2023 18:38
 Operator : SY/MD
 Sample : 02991-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C18

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	4.963	1203	1220	1246	rBV3	370872	1008065	100.00%	12.482%
38	5.317	1326	1330	1333	rBV4	574	544	0.05%	0.007%
39	5.333	1333	1335	1338	rVV2	736	438	0.04%	0.005%
40	5.358	1341	1343	1347	rVB3	891	643	0.06%	0.008%
41	5.391	1347	1353	1355	rBV5	588	635	0.06%	0.008%
42	5.445	1366	1370	1374	rBV3	571	554	0.05%	0.007%
43	5.542	1387	1400	1442	rBV	329660	713614	70.79%	8.836%
44	5.838	1483	1492	1508	rVB8	11695	28038	2.78%	0.347%
45	5.995	1527	1541	1570	rBV	234761	515721	51.16%	6.386%
46	6.236	1611	1616	1618	rBV2	868	869	0.09%	0.011%
47	6.301	1635	1636	1640	rBV	248	208	0.02%	0.003%
48	6.320	1640	1642	1643	rVV2	462	158	0.02%	0.002%
49	6.355	1651	1653	1654	rBV2	372	187	0.02%	0.002%
50	6.445	1679	1681	1682	rBV	271	119	0.01%	0.001%
51	6.487	1691	1694	1698	rBV2	441	457	0.05%	0.006%
52	6.516	1700	1703	1705	rVB2	442	238	0.02%	0.003%
53	6.567	1713	1719	1721	rBV4	1009	916	0.09%	0.011%
54	6.677	1751	1753	1756	rBV3	317	172	0.02%	0.002%
55	6.773	1780	1783	1788	rBV4	498	465	0.05%	0.006%
56	6.792	1788	1789	1793	rVV2	318	151	0.01%	0.002%
57	6.921	1818	1829	1852	rBV	101632	201712	20.01%	2.498%
58	7.249	1919	1931	1965	rBV	380665	703585	69.80%	8.712%
59	7.519	2013	2015	2016	rBV2	577	217	0.02%	0.003%
60	7.561	2018	2028	2056	rVV	75865	147337	14.62%	1.824%
61	7.802	2099	2103	2106	rBV4	522	391	0.04%	0.005%
62	7.911	2121	2137	2157	rBV2	96427	177147	17.57%	2.193%
63	8.034	2166	2175	2211	rBV	240986	511304	50.72%	6.331%
64	8.413	2291	2293	2295	rBV3	588	291	0.03%	0.004%
65	8.657	2367	2369	2371	rBV	345	168	0.02%	0.002%
66	8.670	2371	2373	2377	rVB3	936	652	0.06%	0.008%
67	8.792	2399	2411	2438	rBV	505209	857439	85.06%	10.617%
68	9.034	2484	2486	2489	rVB2	571	252	0.02%	0.003%
69	9.149	2521	2522	2524	rBV	386	154	0.02%	0.002%
70	9.342	2580	2582	2585	rBV2	489	231	0.02%	0.003%
71	9.403	2599	2601	2602	rBV	291	134	0.01%	0.002%
72	9.609	2661	2665	2666	rBV2	441	304	0.03%	0.004%
73	9.654	2677	2679	2680	rBV	244	106	0.01%	0.001%
74	9.677	2683	2686	2689	rVV2	401	356	0.04%	0.004%
75	9.747	2704	2708	2709	rBV2	369	282	0.03%	0.003%
76	9.898	2750	2755	2761	rBV3	519	730	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053123\
 Data File : VV031305.D
 Acq On : 31 May 2023 18:38
 Operator : SY/MD
 Sample : 02991-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C18

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

77	9.953	2770	2772	2773	rVB3	364	93	0.01%	0.001%
78	9.963	2773	2775	2781	rVB3	555	418	0.04%	0.005%
79	9.992	2781	2784	2786	rBV2	411	256	0.03%	0.003%
80	10.040	2796	2799	2802	rBV3	703	442	0.04%	0.005%
81	10.159	2824	2836	2860	rBV	332991	532332	52.81%	6.591%
82	10.333	2881	2890	2902	rBV	12566	20048	1.99%	0.248%
83	10.455	2926	2928	2930	rBV	461	238	0.02%	0.003%
84	10.535	2949	2953	2959	rBV3	659	802	0.08%	0.010%
85	10.625	2980	2981	2984	rBV2	284	164	0.02%	0.002%
86	10.686	2995	3000	3004	rBV2	519	602	0.06%	0.007%
87	10.770	3024	3026	3028	rVB	417	126	0.01%	0.002%
88	10.812	3037	3039	3041	rBV	424	259	0.03%	0.003%
89	10.853	3050	3052	3058	rBV3	524	326	0.03%	0.004%
90	10.918	3068	3072	3077	rBV3	652	696	0.07%	0.009%
91	10.982	3091	3092	3093	rVB	436	84	0.01%	0.001%
92	11.111	3130	3132	3135	rBV	357	184	0.02%	0.002%
93	11.149	3143	3144	3145	rBV	311	100	0.01%	0.001%
94	11.194	3145	3158	3180	rVV	456149	720926	71.52%	8.927%
95	11.381	3214	3216	3217	rBV2	375	118	0.01%	0.001%
96	11.522	3258	3260	3262	rBV	578	191	0.02%	0.002%
97	11.567	3262	3274	3290	rBV	397730	644593	63.94%	7.981%
98	12.577	3585	3588	3591	rBV3	468	415	0.04%	0.005%
99	12.683	3618	3621	3623	rBV	543	430	0.04%	0.005%
100	13.332	3818	3823	3827	rBV2	1040	1001	0.10%	0.012%




Sum of corrected areas: 8076144

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053123\
Data File : VV031305.D
Acq On : 31 May 2023 18:38
Operator : SY/MD
Sample : 02991-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C18

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

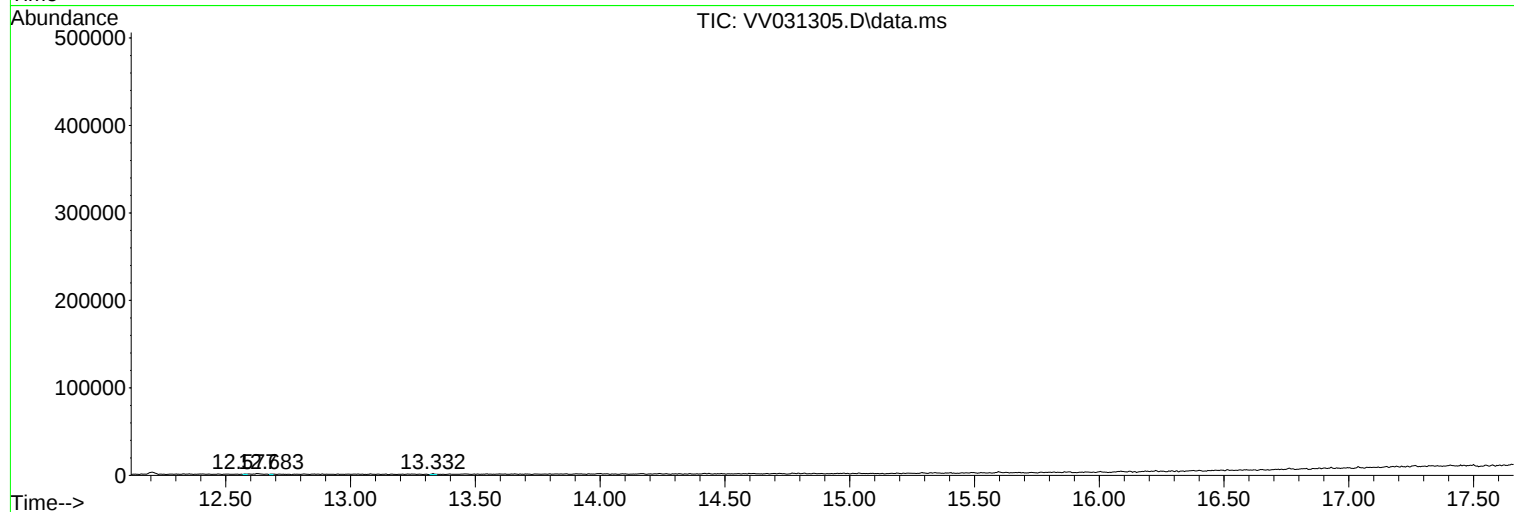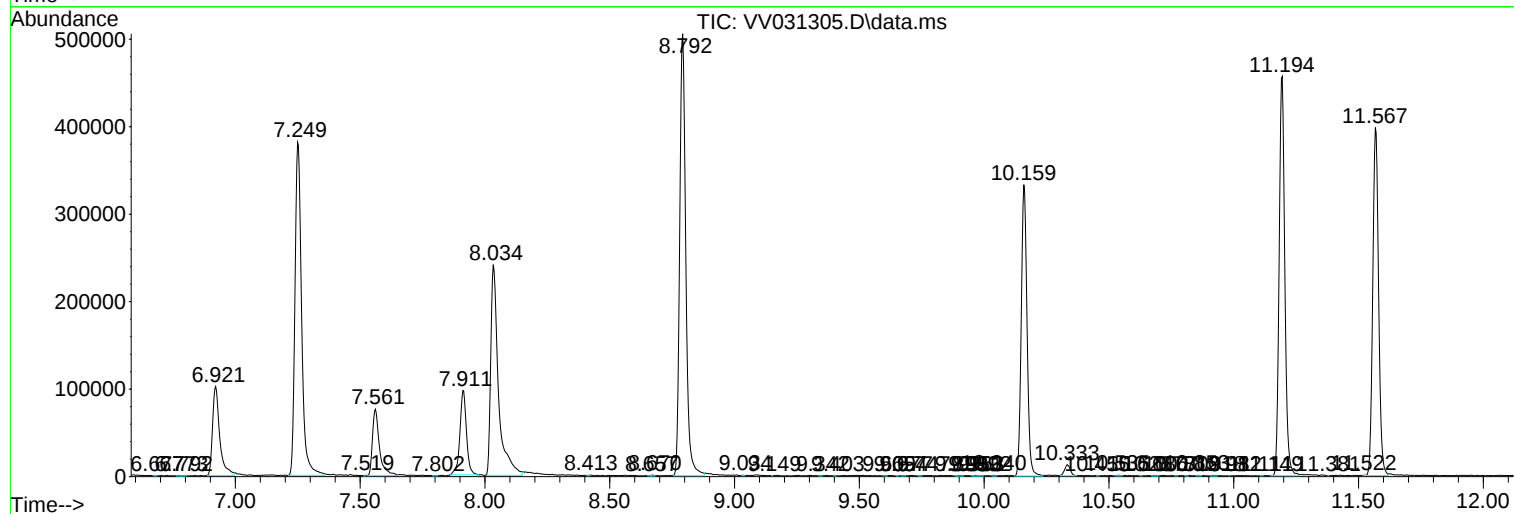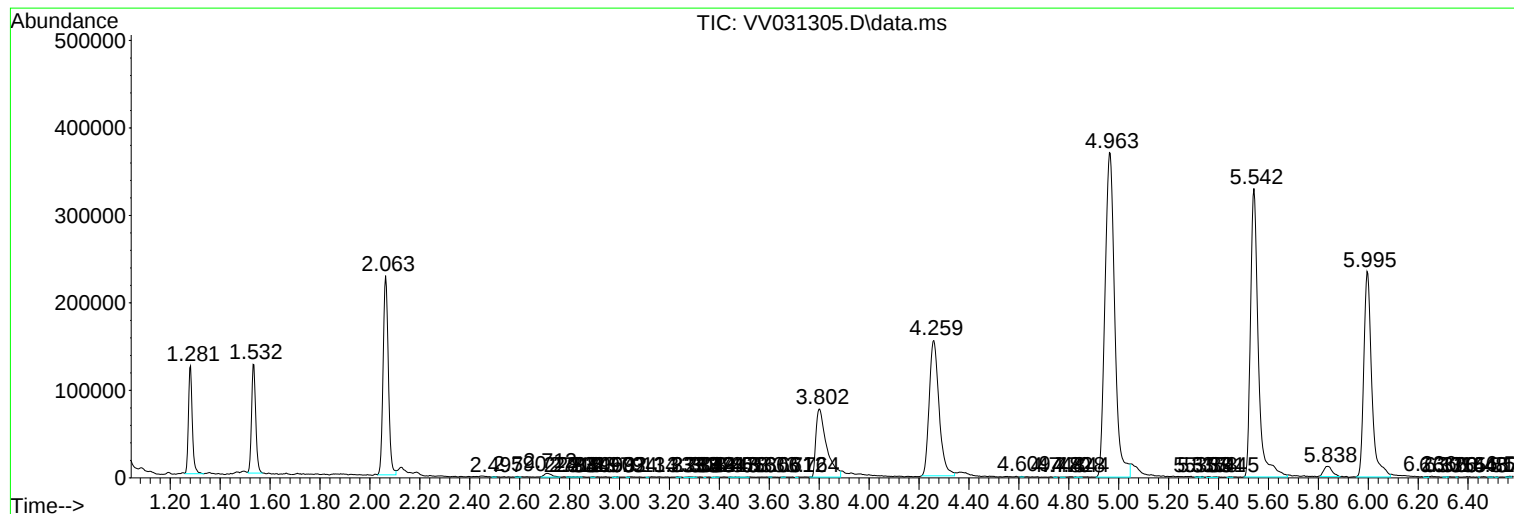

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053123\
Data File : VV031305.D
Acq On : 31 May 2023 18:38
Operator : SY/MD
Sample : 02991-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C18

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053123\
Data File : VV031305.D
Acq On : 31 May 2023 18:38
Operator : SY/MD
Sample : 02991-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C18

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------