

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053123\
 Data File : VV031308.D
 Acq On : 31 May 2023 19:51
 Operator : SY/MD
 Sample : 02991-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C23

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

Signal : TIC: VV031308.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	87	rVB	124340	128229	9.92%	1.362%
2	1.536	147	154	171	rVB	121606	146541	11.33%	1.557%
3	2.063	309	318	331	rBV	223415	319460	24.71%	3.394%
4	2.487	447	450	454	rVB4	878	586	0.05%	0.006%
5	2.510	454	457	460	rBV2	568	479	0.04%	0.005%
6	2.523	460	461	465	rVB2	747	247	0.02%	0.003%
7	2.568	473	475	479	rBV2	527	326	0.03%	0.003%
8	2.638	494	497	500	rBV	547	412	0.03%	0.004%
9	2.706	511	518	527	rVB3	4208	6655	0.51%	0.071%
10	2.796	544	546	551	rVB2	601	395	0.03%	0.004%
11	2.819	551	553	554	rBV	450	174	0.01%	0.002%
12	3.008	610	612	616	rVB2	280	180	0.01%	0.002%
13	3.028	616	618	619	rBV2	485	212	0.02%	0.002%
14	3.056	624	627	632	rBV3	384	365	0.03%	0.004%
15	3.121	644	647	650	rBV	478	273	0.02%	0.003%
16	3.169	660	662	664	rBV2	290	152	0.01%	0.002%
17	3.288	698	699	702	rBV	326	195	0.02%	0.002%
18	3.400	730	734	740	rBV3	537	526	0.04%	0.006%
19	3.507	765	767	769	rBV	183	125	0.01%	0.001%
20	3.523	770	772	774	rVV	406	193	0.01%	0.002%
21	3.545	777	779	783	rVB	499	294	0.02%	0.003%
22	3.564	783	785	787	rBV	146	107	0.01%	0.001%
23	3.587	789	792	793	rBV	358	181	0.01%	0.002%
24	3.664	810	816	819	rVB2	778	714	0.06%	0.008%
25	3.687	819	823	824	rBV2	534	399	0.03%	0.004%
26	3.722	832	834	836	rBV	386	230	0.02%	0.002%
27	3.754	842	844	846	rBV2	222	72	0.01%	0.001%
28	3.818	846	864	897	rBV2	138410	481308	37.23%	5.114%
29	4.259	986	1001	1026	rBV	155960	416662	32.23%	4.427%
30	4.626	1112	1115	1121	rVB5	470	456	0.04%	0.005%
31	4.654	1121	1124	1128	rBV2	620	596	0.05%	0.006%
32	4.835	1178	1180	1183	rBV	387	209	0.02%	0.002%
33	4.963	1203	1220	1242	rBV2	370809	980097	75.81%	10.414%
34	5.455	1371	1373	1378	rBV2	474	303	0.02%	0.003%
35	5.490	1382	1384	1387	rBV3	459	231	0.02%	0.002%
36	5.542	1387	1400	1442	rBV	309544	678974	52.52%	7.214%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053123\
 Data File : VV031308.D
 Acq On : 31 May 2023 19:51
 Operator : SY/MD
 Sample : 02991-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C23

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
 Title : VOC Analysis

37	5.770	1469	1471	1473	rBV2	849	443	0.03%	0.005%
38	5.841	1480	1493	1512	rBV3	95560	213404	16.51%	2.267%
39	5.995	1529	1541	1568	rBV	229925	495291	38.31%	5.263%
40	6.439	1675	1679	1681	rBV2	516	337	0.03%	0.004%
41	6.494	1691	1696	1699	rVB2	429	338	0.03%	0.004%
42	6.513	1699	1702	1704	rBV2	401	240	0.02%	0.003%
43	6.577	1716	1722	1723	rBV5	978	925	0.07%	0.010%
44	6.764	1776	1780	1781	rBV	297	201	0.02%	0.002%
45	6.876	1813	1815	1817	rBV	246	110	0.01%	0.001%
46	6.921	1817	1829	1856	rBV2	100433	201682	15.60%	2.143%
47	7.166	1903	1905	1906	rBV2	562	125	0.01%	0.001%
48	7.249	1919	1931	1956	rBV	376881	685778	53.04%	7.286%
49	7.561	2018	2028	2053	rBV2	74386	144000	11.14%	1.530%
50	7.786	2096	2098	2101	rBV3	635	394	0.03%	0.004%
51	7.912	2123	2137	2165	rBV	747834	1292877	100.00%	13.737%
52	8.034	2165	2175	2215	rBV	248298	514702	39.81%	5.469%
53	8.358	2274	2276	2283	rBV5	741	674	0.05%	0.007%
54	8.709	2382	2385	2386	rBV2	646	276	0.02%	0.003%
55	8.793	2399	2411	2440	rBV	485930	813111	62.89%	8.639%
56	9.262	2554	2557	2560	rBV2	594	471	0.04%	0.005%
57	9.490	2622	2628	2632	rBV4	1142	1242	0.10%	0.013%
58	9.632	2670	2672	2674	rBV	334	173	0.01%	0.002%
59	9.985	2780	2782	2783	rBV	427	148	0.01%	0.002%
60	10.159	2822	2836	2858	rBV	326228	524495	40.57%	5.573%
61	10.333	2882	2890	2900	rBV4	10035	15528	1.20%	0.165%
62	10.477	2933	2935	2938	rBV2	544	389	0.03%	0.004%
63	10.619	2977	2979	2983	rVB3	605	350	0.03%	0.004%
64	10.641	2984	2986	2988	rVV3	441	135	0.01%	0.001%
65	10.799	3032	3035	3039	rBV3	763	624	0.05%	0.007%
66	10.921	3072	3073	3074	rBV3	336	77	0.01%	0.001%
67	10.966	3085	3087	3090	rBV2	442	187	0.01%	0.002%
68	11.046	3107	3112	3118	rBV5	882	1197	0.09%	0.013%
69	11.130	3136	3138	3144	rVB3	966	672	0.05%	0.007%
70	11.191	3146	3157	3179	rBV	429986	691996	53.52%	7.353%
71	11.567	3263	3274	3290	rBV	400803	637025	49.27%	6.768%
72	11.931	3384	3387	3389	rBV2	575	401	0.03%	0.004%
73	12.204	3468	3472	3479	rVB6	2482	2734	0.21%	0.029%
74	12.326	3508	3510	3512	rBV	459	201	0.02%	0.002%
75	12.503	3561	3565	3566	rBV3	532	409	0.03%	0.004%
76	12.551	3577	3580	3581	rBV2	719	423	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053123\
Data File : VV031308.D
Acq On : 31 May 2023 19:51
Operator : SY/MD
Sample : 02991-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C23

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Title : VOC Analysis

77	13.172	3771	3773	3775	rBV2	582	288	0.02%	0.003%
78	13.217	3784	3787	3793	rBV4	805	760	0.06%	0.008%
79	13.593	3902	3904	3905	rBV4	540	278	0.02%	0.003%




Sum of corrected areas: 9411669

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053123\
Data File : VV031308.D
Acq On : 31 May 2023 19:51
Operator : SY/MD
Sample : 02991-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

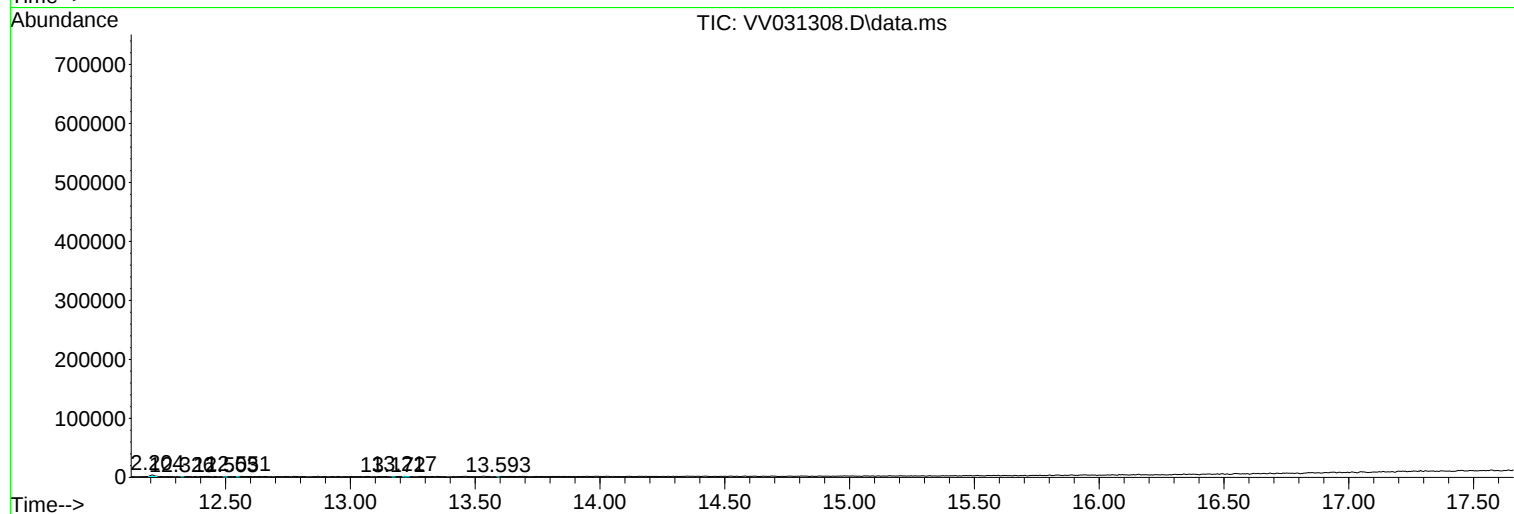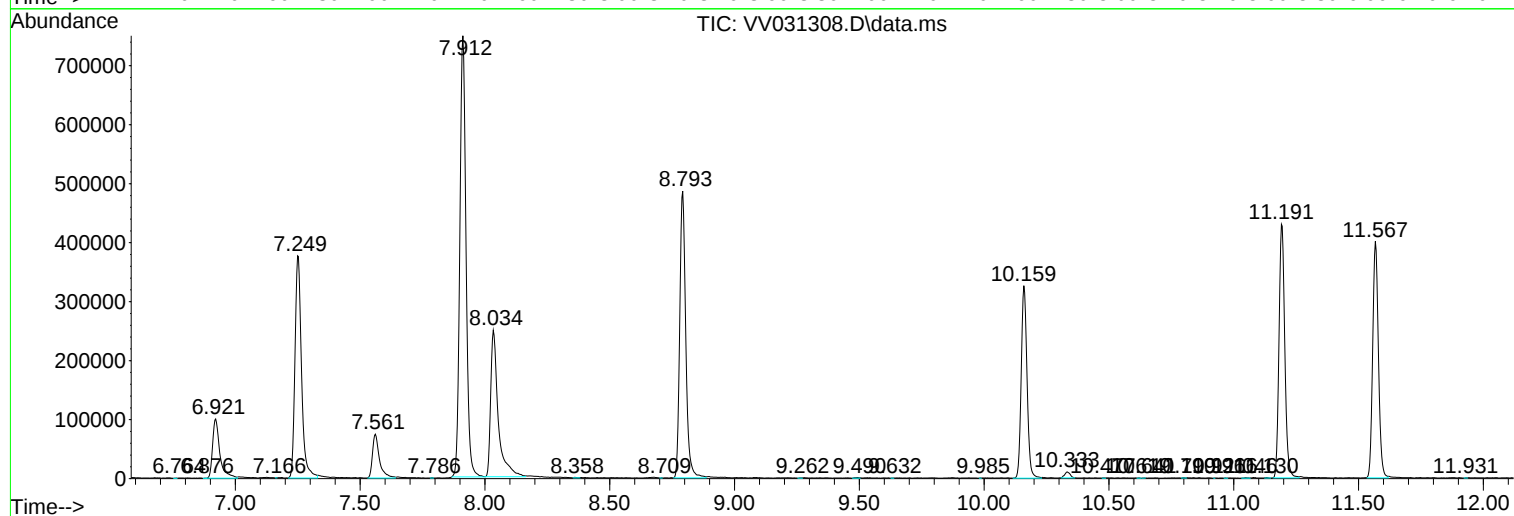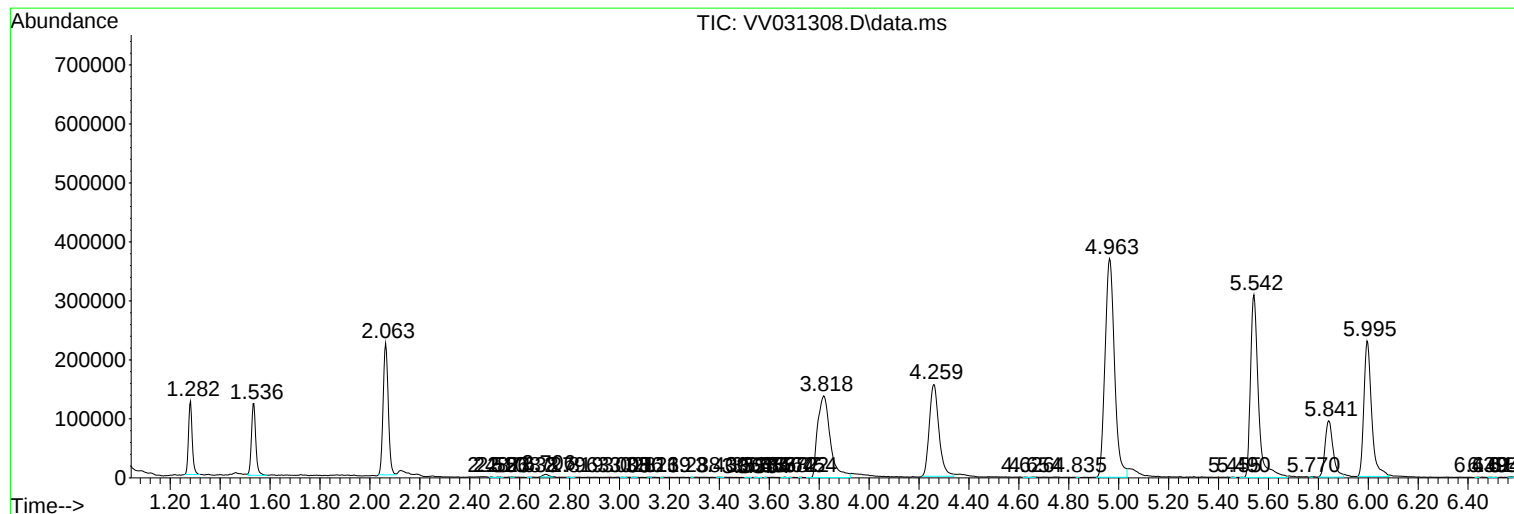

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053123\
Data File : VV031308.D
Acq On : 31 May 2023 19:51
Operator : SY/MD
Sample : 02991-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053123\
Data File : VV031308.D
Acq On : 31 May 2023 19:51
Operator : SY/MD
Sample : 02991-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------