
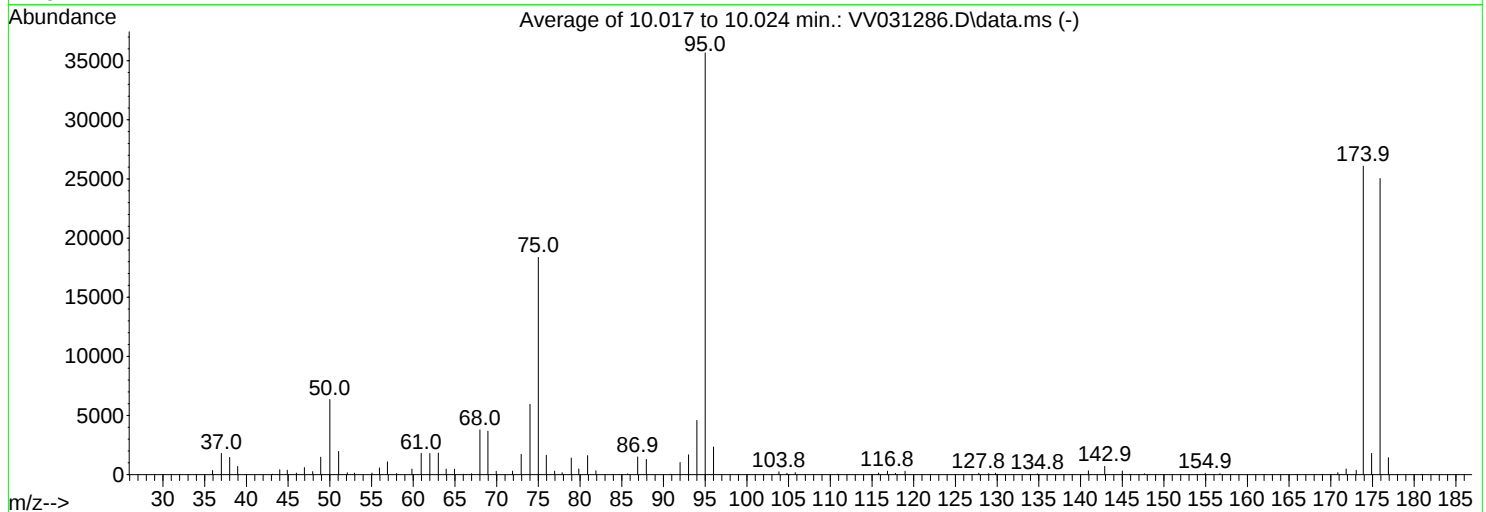


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053123\
Data File : VV031286.D
Acq On : 31 May 2023 09:32
Operator : SY/MD
Sample : BFB381
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB381

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM051923WMA.M
Title : VOC Analysis
Last Update : Thu Jun 01 01:56:05 2023

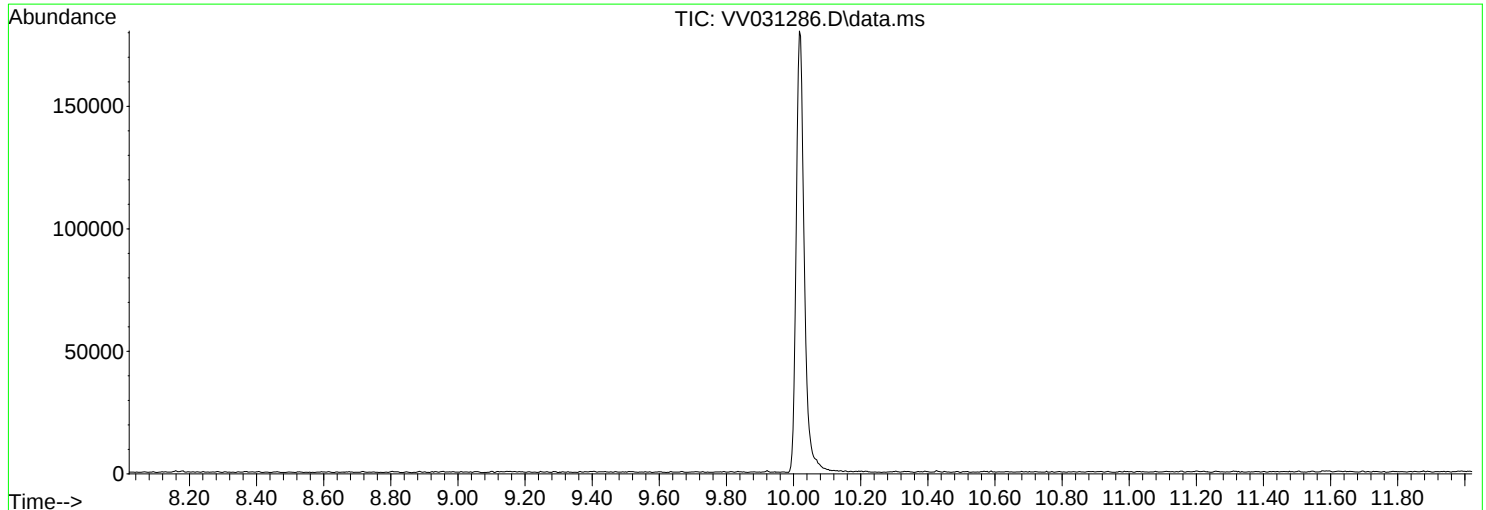

AutoFind: Scans 2792, 2793, 2794; Background Corrected with Scan 2781

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.8	6353	PASS
75	95	30	80	51.5	18373	PASS
95	95	100	100	100.0	35664	PASS
96	95	5	9	6.6	2344	PASS
173	174	0.00	2	1.4	372	PASS
174	95	50	120	73.1	26083	PASS
175	174	5	9	6.9	1802	PASS
176	174	95	105	96.0	25045	PASS
177	176	5	10	5.7	1428	PASS

m/z	Abundance
39.90	334.0
44.10	320.0

Instrument :
MSVOA_V
ClientSampleId :
BFB381

m/z	Abundance
36.00	350.0
37.00	1754.0
38.00	1449.0
39.00	686.0
39.80	368.0
44.00	751.0
44.90	421.0
46.00	147.0
47.00	569.0
47.90	286.0
48.90	1466.0
50.00	6889.0
51.10	2084.0
52.10	193.0
53.00	118.0
55.00	107.0
56.00	520.0
56.90	1227.0
58.00	161.0
59.90	461.0
61.00	1762.0
62.00	1870.0
63.00	1927.0
64.00	436.0
64.90	504.0
66.40	106.0
68.00	3887.0
69.00	4054.0
70.00	275.0
71.90	351.0
72.90	1930.0
74.00	6434.0
75.00	19800.0
76.00	1720.0
76.90	277.0
77.90	138.0
78.90	1428.0
79.80	521.0
80.90	1707.0
81.90	362.0
86.90	1633.0
87.90	1404.0
90.90	122.0
92.00	1097.0
93.00	1741.0
94.00	4805.0
95.00	36968.0
96.00	2521.0
103.90	216.0
104.80	128.0
105.80	157.0
115.80	113.0
116.80	290.0
117.80	202.0
118.90	254.0
127.80	110.0
129.00	117.0
129.80	201.0
134.80	111.0
141.00	322.0
142.90	733.0
145.00	326.0
145.90	113.0
147.60	138.0
155.00	138.0
156.70	166.0
170.90	191.0
171.90	454.0
173.00	508.0
173.90	26640.0
174.90	1894.0
175.90	26048.0
176.90	1373.0

Instrument :
MSVOA_V
ClientSampleId :
BFB381

m/z	Abundance
35.90	358.0
37.00	1855.0
38.00	1518.0
38.90	684.0
39.80	333.0
44.00	770.0
44.90	380.0
46.00	141.0
46.90	613.0
48.00	235.0
48.90	1535.0
50.00	6546.0
51.00	2043.0
52.10	157.0
53.00	159.0
55.10	136.0
56.00	595.0
56.90	1135.0
58.00	136.0
59.80	505.0
60.90	1828.0
62.00	1838.0
63.00	1852.0
64.00	494.0
64.90	447.0
67.00	102.0
68.00	3923.0
69.00	3771.0
70.00	292.0
71.90	318.0
73.00	1757.0
74.00	6093.0
75.00	18952.0
76.00	1729.0
76.90	326.0
77.90	171.0
79.00	1441.0
79.90	501.0
80.90	1695.0
81.90	325.0
85.70	107.0
86.90	1573.0
87.90	1335.0
92.00	1074.0
93.00	1770.0
94.00	4695.0
95.00	36992.0
96.00	2439.0
103.80	252.0
104.80	137.0
105.80	189.0
110.90	107.0
115.80	131.0
116.90	307.0
117.80	128.0
119.00	286.0
127.80	127.0
129.00	118.0
129.80	160.0
134.90	115.0
141.00	334.0
142.90	736.0
145.00	340.0
147.70	104.0
154.90	134.0
156.70	112.0
170.80	185.0
171.80	489.0
173.10	609.0
173.90	26824.0
174.90	1804.0
175.90	25752.0
176.90	1446.0

Instrument :
MSVOA_V
ClientSampleId :
BFB381

m/z	Abundance
35.90	329.0
37.00	1784.0
38.00	1432.0
38.90	682.0
39.80	271.0
43.10	109.0
44.00	692.0
44.90	343.0
46.00	108.0
46.90	593.0
48.00	239.0
48.90	1412.0
50.00	5625.0
51.00	1781.0
52.10	137.0
52.90	138.0
55.10	147.0
55.90	608.0
56.90	894.0
59.80	458.0
60.90	1798.0
62.00	1644.0
63.00	1685.0
63.90	495.0
65.00	425.0
66.00	115.0
67.00	135.0
68.00	3572.0
68.90	3210.0
69.90	270.0
71.90	244.0
73.00	1463.0
74.00	5337.0
75.00	16368.0
75.90	1478.0
77.00	301.0
77.80	165.0
79.00	1343.0
79.90	464.0
80.90	1418.0
81.90	286.0
85.70	111.0
86.90	1298.0
88.00	1111.0
92.00	904.0
93.00	1541.0
94.00	4243.0
95.00	33032.0
96.00	2073.0
103.80	245.0
104.80	109.0
105.80	195.0
115.80	149.0
116.90	306.0
119.00	300.0
127.80	130.0
130.00	112.0
140.90	307.0
142.90	642.0
145.00	290.0
154.90	114.0
170.80	149.0
171.80	540.0
173.90	24784.0
174.90	1707.0
175.90	23336.0
176.90	1465.0

Instrument :
MSVOA_V
ClientSampleId :
BFB381