

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053124\
 Data File : VV035926.D
 Acq On : 31 May 2024 13:49
 Operator : SY/MD
 Sample : P2659-19
 Misc : 5.58g/10.0mL/MSVOA_V/SOIL/A
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: May 31 23:02:57 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri May 31 22:59:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	621420	25.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	592548	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	221352	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	155651	13.624	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	54.480%
7) Chloroethane-d5	1.529	69	139909	15.358	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	61.440%
11) 1,1-Dichloroethene-d2	2.053	65	70379	13.838	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	55.360%
21) 2-Butanone-d5	3.841	46	80687	30.782	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	61.560%
24) Chloroform-d	4.246	84	321880	16.292	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	65.160%
26) 1,2-Dichloroethane-d4	4.941	65	184373	17.799	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	71.200%
32) Benzene-d6	4.957	84	580029	16.468	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	65.880%
36) 1,2-Dichloropropane-d6	5.986	67	207661	18.722	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	74.880%
41) Toluene-d8	7.243	98	447391	14.396	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	57.600%
43) trans-1,3-Dichloroprop...	7.555	79	70114	15.417	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	61.680%
47) 2-Hexanone-d5	8.034	63	52540	34.961	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	69.920%
56) 1,1,2,2-Tetrachloroeth...	10.149	84	178033	21.479	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	85.920%
66) 1,2-Dichlorobenzene-d4	11.558	152	151384	18.650	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	74.600%#
Target Compounds						Qvalue
16) Methylene chloride	2.445	84	41462	2.949	ug/L	98
48) 2-Hexanone	8.034	43	6982	1.615	ug/L #	71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV053124\
Data File : VV035926.D
Acq On : 31 May 2024 13:49
Operator : SY/MD
Sample : P2659-19
Misc : 5.58g/10.0mL/MSVOA_V/SOIL/A
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: May 31 23:02:57 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM053024SMA.M
Quant Title : VOC Analysis
QLast Update : Fri May 31 22:59:48 2024
Response via : Initial Calibration

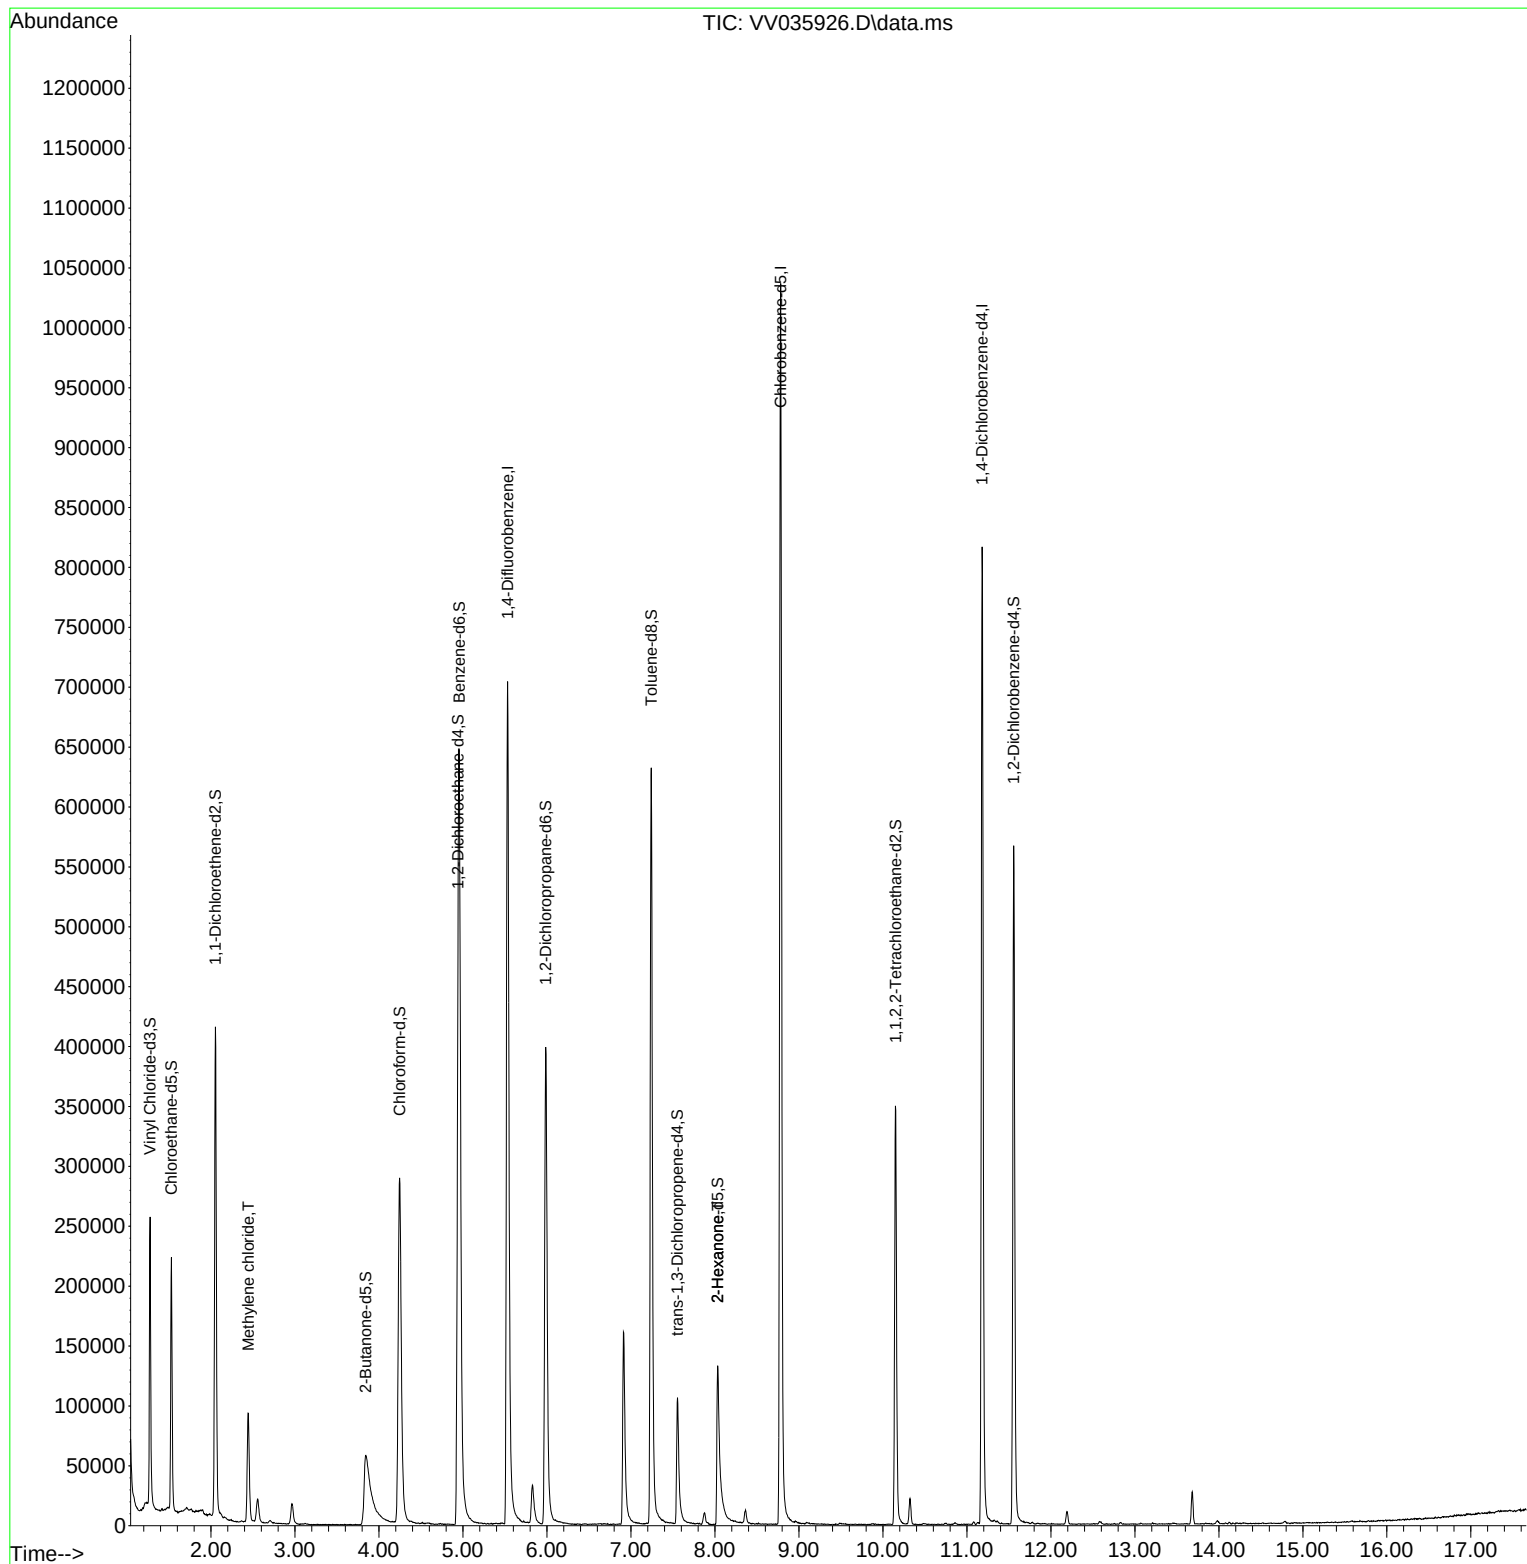

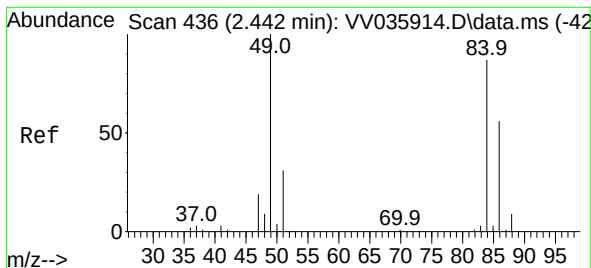

#16

Methylene chloride

Concen: 2.949 ug/L

RT: 2.445 min Scan# 41

Delta R.T. 0.003 min

Lab File: VV035926.D

Acq: 31 May 2024 13:49

Instrument :

MSVOA_V

ClientSampleId :





Tgt Ion: 84 Resp: 41462

Ion Ratio Lower Upper

84 100

86 62.9 44.6 82.8

49 112.5 81.1 150.5

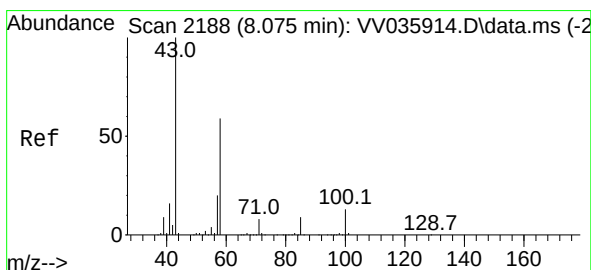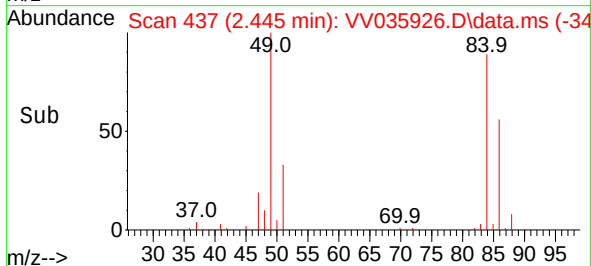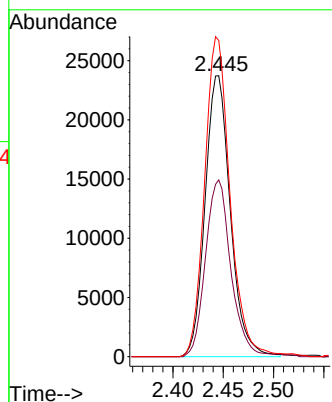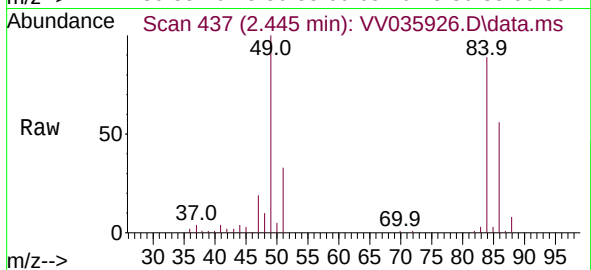

#48

2-Hexanone

Concen: 1.615 ug/L

RT: 8.034 min Scan# 2175

Delta R.T. -0.042 min

Lab File: VV035926.D

Acq: 31 May 2024 13:49

Tgt Ion: 43 Resp: 6982

Ion Ratio Lower Upper

43 100

58 40.0 45.4 68.0#

57 45.7 15.8 23.8#

100 6.3 9.8 14.8#

