

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060121\
 Data File : VV021454.D
 Acq On : 01 Jun 2021 12:48
 Operator : SY/MD
 Sample : VV0601WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK182

Quant Time: Jun 02 00:50:07 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 02 00:49:39 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	256211	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	235782	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	134238	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	61748	5.696	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	114.000%	
7) Chloroethane-d5	1.565	69	50214	4.854	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	97.000%	
11) 1,1-Dichloroethene-d2	2.102	63	79733	3.880	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	77.600%	
20) 2-Butanone-d5	3.918	46	138262	35.483	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	70.960%	
24) Chloroform-d	4.349	84	123446	4.106	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	82.200%	
26) 1,2-Dichloroethane-d4	5.034	65	56467	4.085	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	81.800%	
32) Benzene-d6	5.050	84	258244	4.552	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	91.000%	
36) 1,2-Dichloropropane-d6	6.072	67	77805	4.229	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	84.600%	
41) Toluene-d8	7.317	98	248834	4.784	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	95.600%	
43) trans-1,3-Dichloroprop...	7.625	79	32452	4.238	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	84.800%	
46) 2-Hexanone-d5	8.092	63	125737	34.874	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	69.740%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	56810	3.831	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	76.600%	
66) 1,2-Dichlorobenzene-d4	11.625	152	102561	4.433	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	88.600%	
Target Compounds						Qvalue
16) Methylene chloride	2.503	84	16911	0.810	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060121\
Data File : VV021454.D
Acq On : 01 Jun 2021 12:48
Operator : SY/MD
Sample : VV0601WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK182

Quant Time: Jun 02 00:50:07 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 02 00:49:39 2021
Response via : Initial Calibration

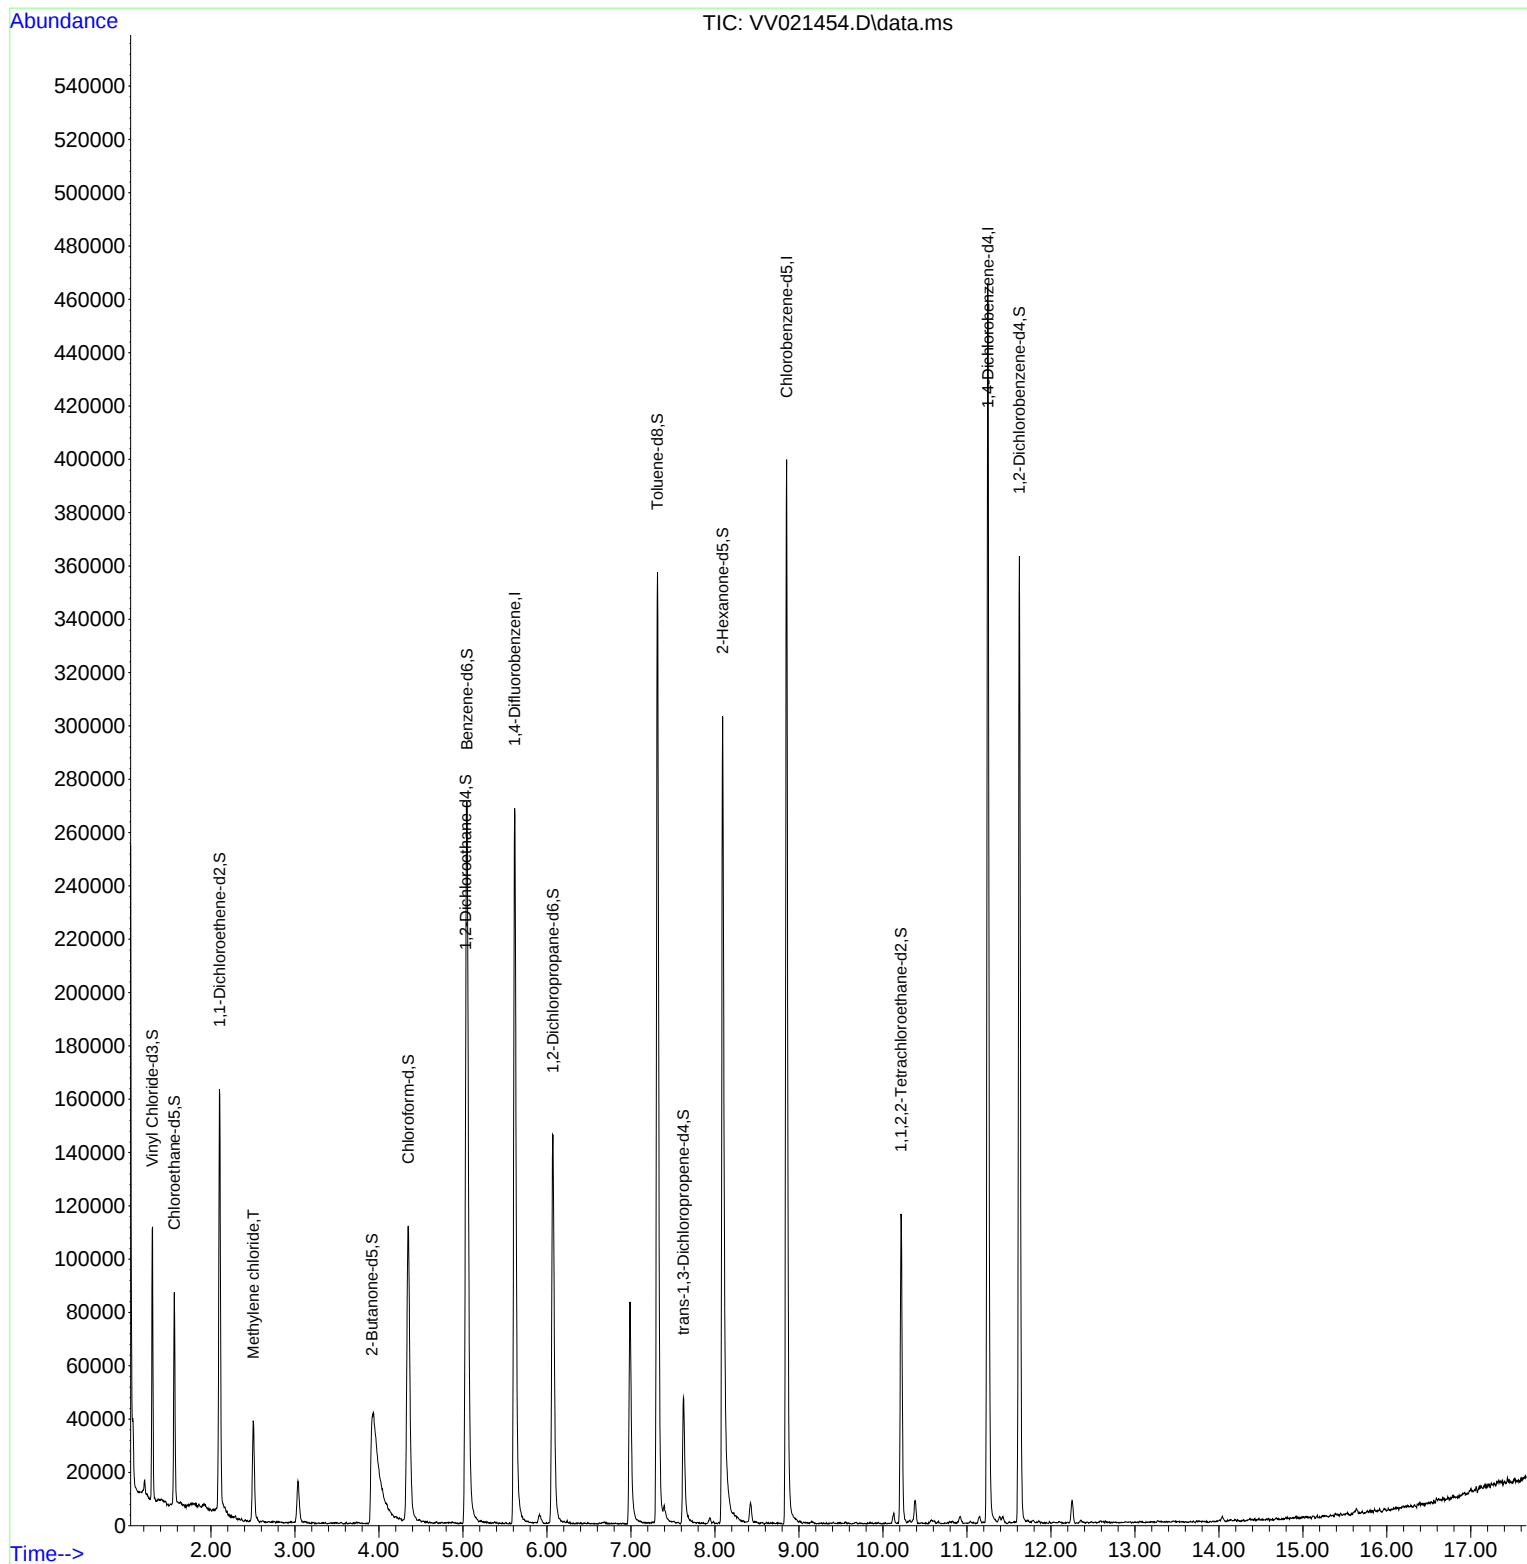

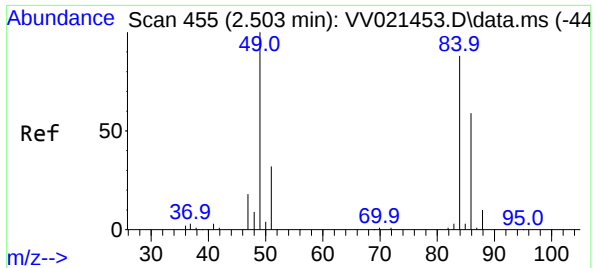

#16
Methylene chloride
Concen: 0.810 ug/L
RT: 2.503 min Scan# 455
Delta R.T. 0.000 min
Lab File: VV021454.D
Acq: 01 Jun 2021 12:48

Instrument :
MSVOA_V
ClientSampleId :
VBLK182

Tgt Ion: 84 Resp: 16911

Ion	Ratio	Lower	Upper
84	100		
86	63.1	44.7	82.9
49	111.6	82.7	153.5

