

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060121\
 Data File : VV021455.D
 Acq On : 01 Jun 2021 13:14
 Operator : SY/MD
 Sample : M2568-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GP1

Quant Time: Jun 02 00:50:12 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 02 00:49:39 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	237784	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	219592	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	123185	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	41617	4.137	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	82.800%
7) Chloroethane-d5	1.564	69	43508	4.532	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.600%
11) 1,1-Dichloroethene-d2	2.105	63	58496	3.067	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	61.400%
20) 2-Butanone-d5	3.918	46	194540	53.795	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	107.600%
24) Chloroform-d	4.349	84	128361	4.600	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.000%
26) 1,2-Dichloroethane-d4	5.037	65	62175	4.847	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.000%
32) Benzene-d6	5.050	84	248429	4.702	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.000%
36) 1,2-Dichloropropane-d6	6.072	67	81502	4.757	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.200%
41) Toluene-d8	7.317	98	221948	4.581	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.600%
43) trans-1,3-Dichloroprop...	7.628	79	32193	4.514	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.200%
46) 2-Hexanone-d5	8.091	63	165543	49.299	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	98.600%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	63510	4.599	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.000%
66) 1,2-Dichlorobenzene-d4	11.625	152	104032	4.900	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.000%
Target Compounds						
					Qvalue	
16) Methylene chloride	2.506	84	11071	0.571	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060121\
Data File : VV021455.D
Acq On : 01 Jun 2021 13:14
Operator : SY/MD
Sample : M2568-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GP1


Quant Time: Jun 02 00:50:12 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 02 00:49:39 2021
Response via : Initial Calibration

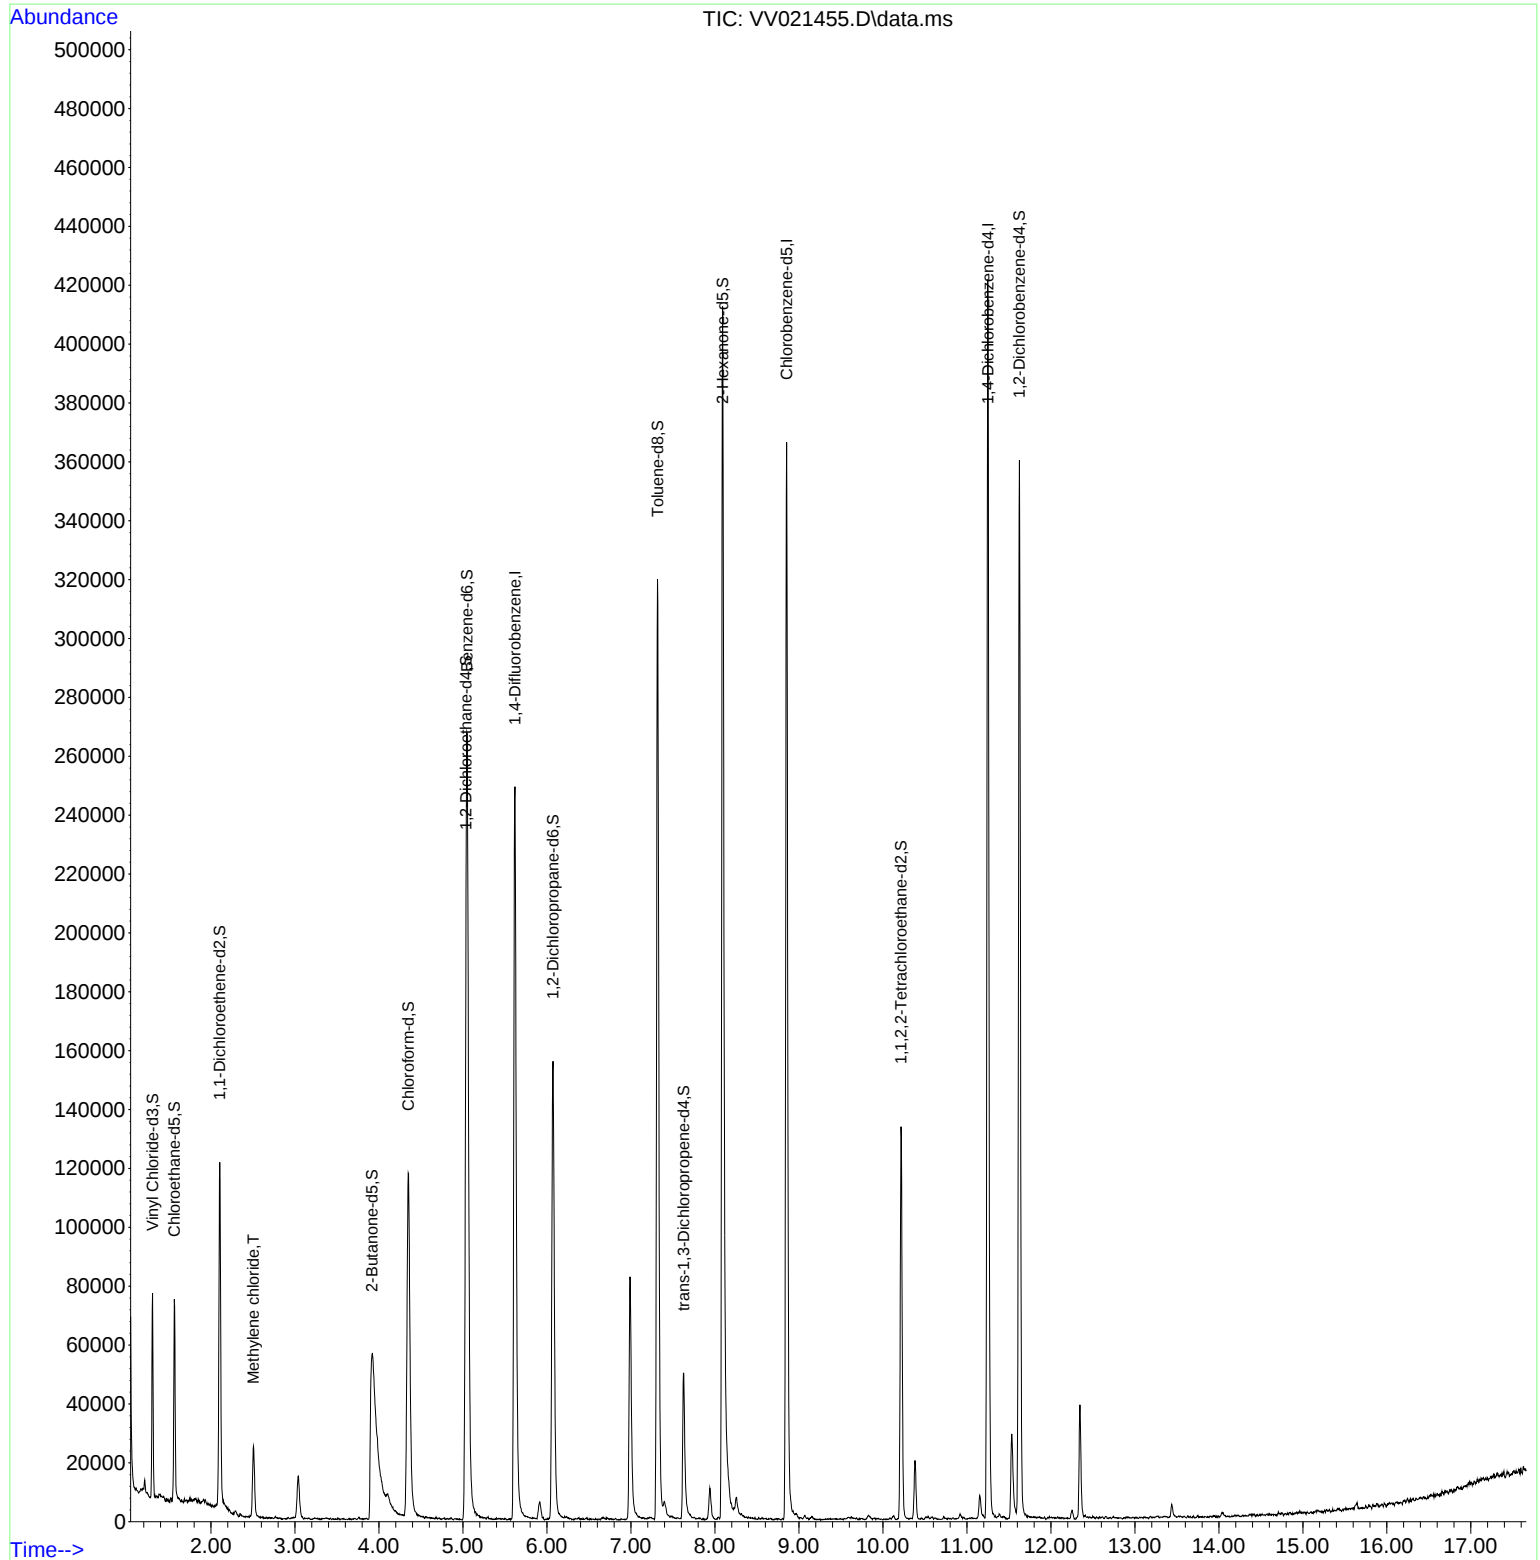

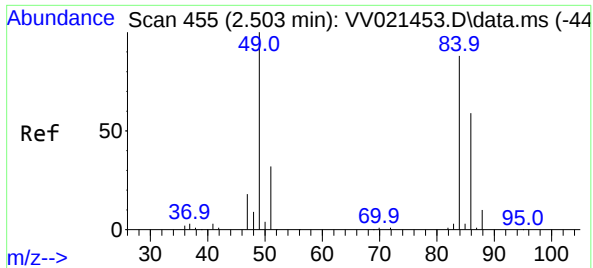

#16
Methylene chloride
Concen: 0.571 ug/L
RT: 2.506 min Scan# 456
Delta R.T. 0.003 min
Lab File: VV021455.D
Acq: 01 Jun 2021 13:14

Instrument :
MSVOA_V
ClientSampleId :
C0GP1

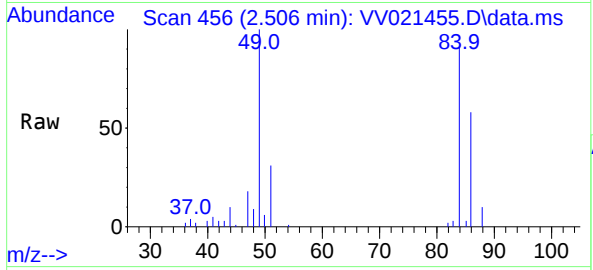

Tgt Ion: 84 Resp: 11071

Ion	Ratio	Lower	Upper
84	100		
86	63.3	44.7	82.9
49	109.6	82.7	153.5

