

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060121\
 Data File : VV021458.D
 Acq On : 01 Jun 2021 14:24
 Operator : SY/MD
 Sample : M2568-04DL 50X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GM9DL

Quant Time: Jun 02 00:50:30 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 02 00:49:39 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	229965	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	212307	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	120893	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	38629	3.970	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	79.400%
7) Chloroethane-d5	1.565	69	42319	4.558	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.200%
11) 1,1-Dichloroethene-d2	2.102	63	57424	3.114	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	62.200%
20) 2-Butanone-d5	3.931	46	188720	53.960	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	107.920%
24) Chloroform-d	4.352	84	130552	4.838	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.800%
26) 1,2-Dichloroethane-d4	5.037	65	64496	5.199	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.000%
32) Benzene-d6	5.050	84	250372	4.902	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.000%
36) 1,2-Dichloropropane-d6	6.072	67	82154	4.960	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.200%
41) Toluene-d8	7.320	98	225232	4.809	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.200%
43) trans-1,3-Dichloroprop...	7.629	79	32124	4.659	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	93.200%
46) 2-Hexanone-d5	8.095	63	170501	52.518	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	105.040%
56) 1,1,2,2-Tetrachloroeth...	10.220	84	69524	5.207	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.200%
66) 1,2-Dichlorobenzene-d4	11.625	152	104514	5.016	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.400%
Target Compounds						Qvalue
16) Methylene chloride	2.507	84	14798	0.789	ug/L	94
34) Trichloroethene	5.921	95	22594	1.485	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060121\
Data File : VV021458.D
Acq On : 01 Jun 2021 14:24
Operator : SY/MD
Sample : M2568-04DL 50X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GM9DL


Quant Time: Jun 02 00:50:30 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 02 00:49:39 2021
Response via : Initial Calibration

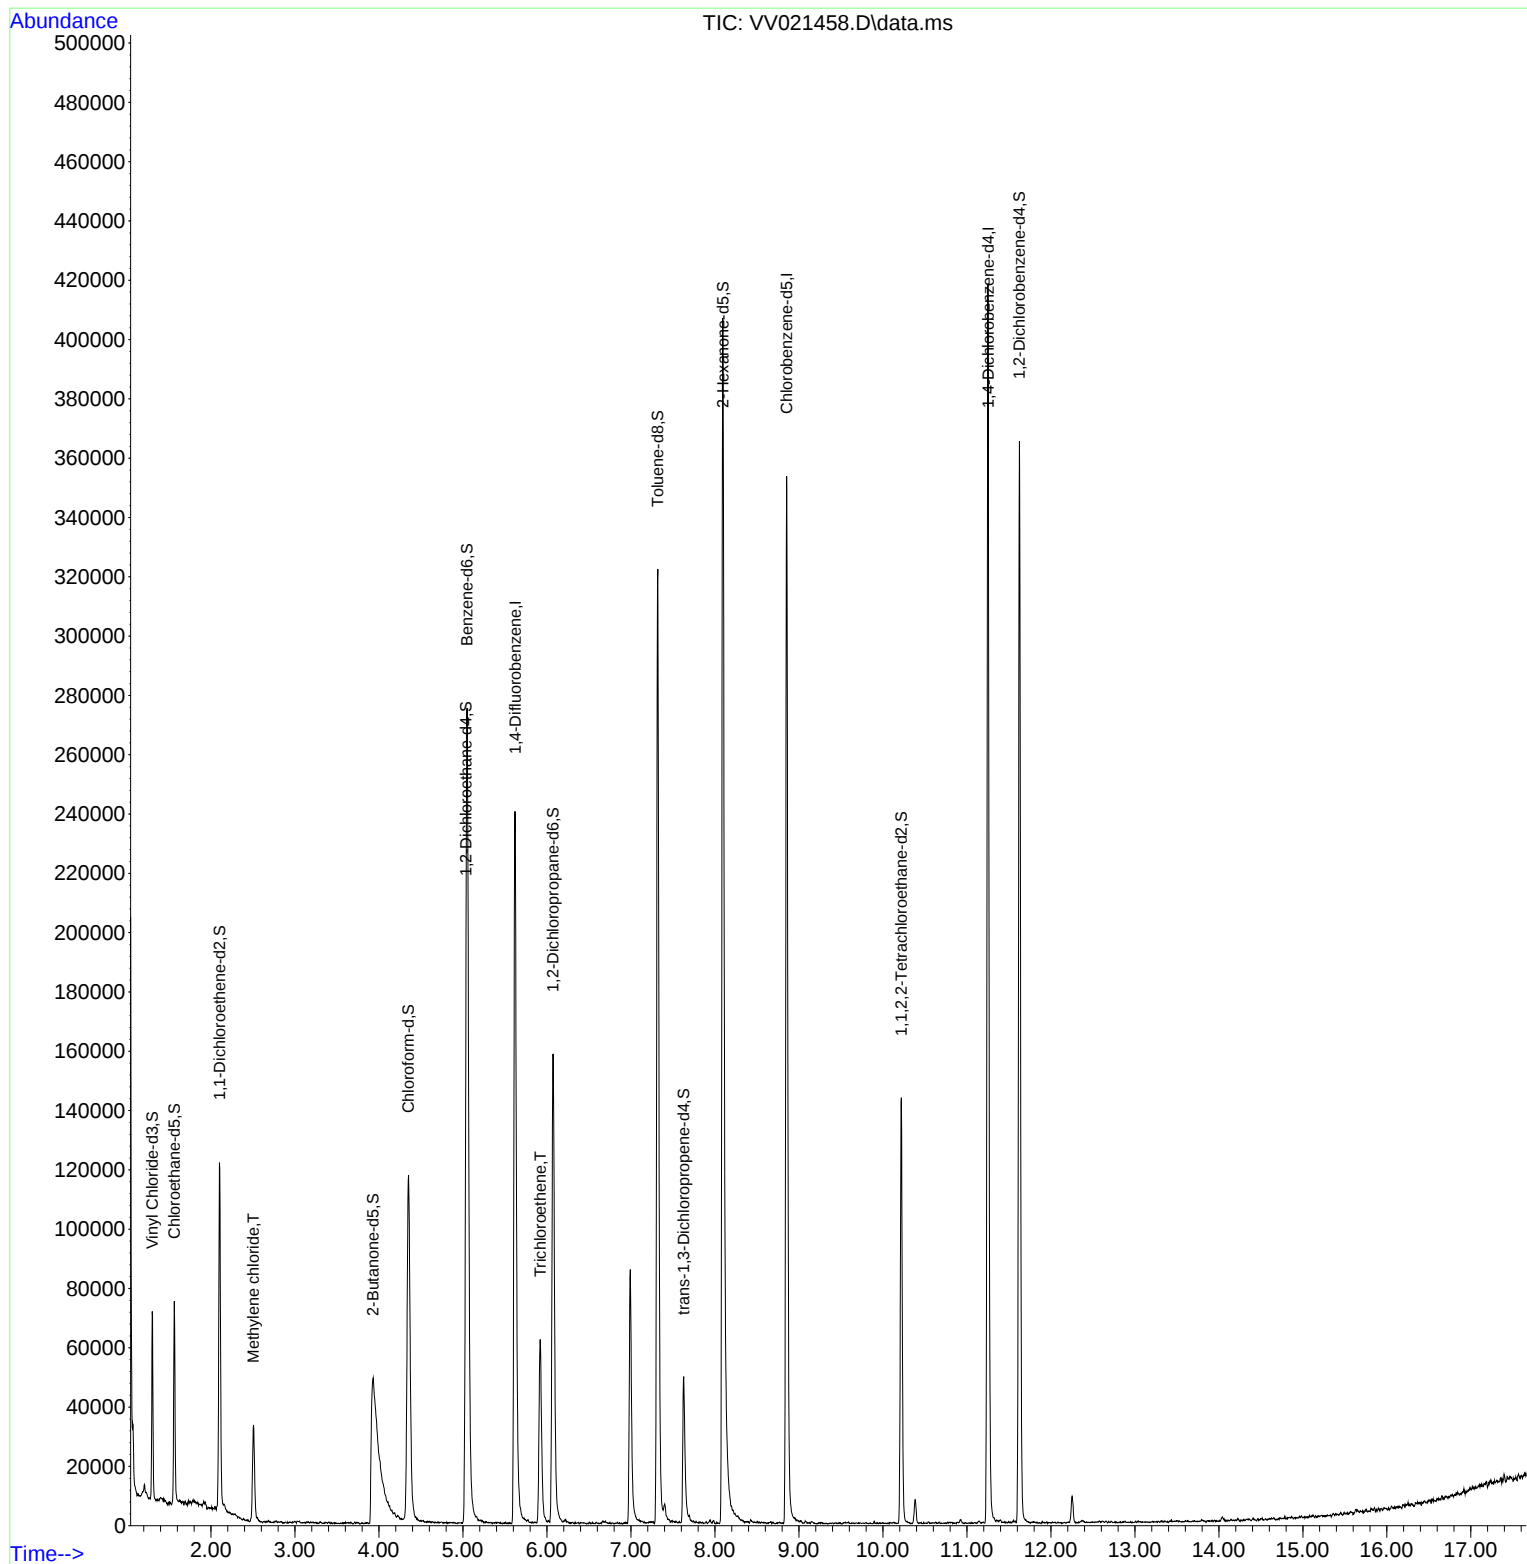



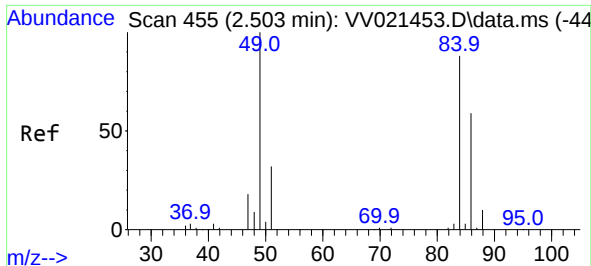


#16
Methylene chloride
Concen: 0.789 ug/L
RT: 2.507 min Scan# 456
Delta R.T. 0.003 min
Lab File: VV021458.D
Acq: 01 Jun 2021 14:24

Instrument :
MSVOA_V
ClientSampleId :
C0GM9DL

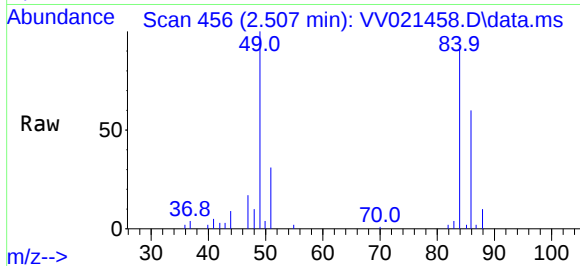

Tgt Ion: 84 Resp: 14798
Ion Ratio Lower Upper
84 100
86 65.8 44.7 82.9
49 109.1 82.7 153.5

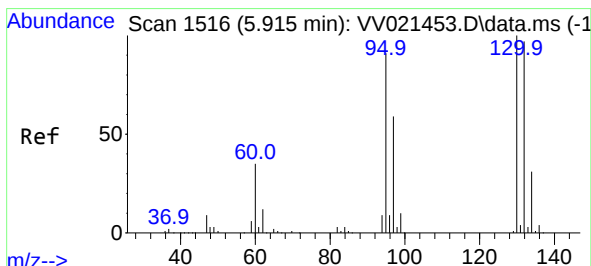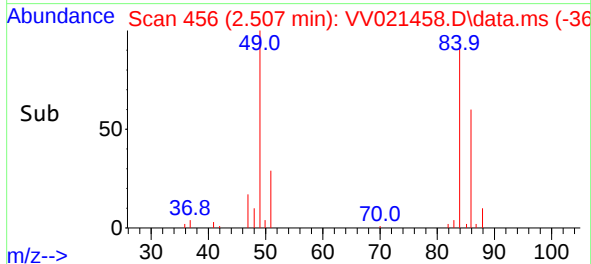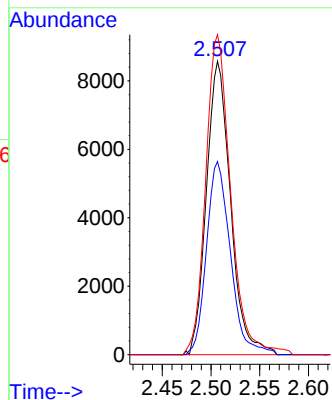

#34
Trichloroethene
Concen: 1.485 ug/L
RT: 5.921 min Scan# 1518
Delta R.T. 0.006 min
Lab File: VV021458.D
Acq: 01 Jun 2021 14:24

Tgt Ion: 95 Resp: 22594
Ion Ratio Lower Upper
95 100
97 62.2 45.4 84.4
132 106.3 74.5 138.3
130 112.0 77.7 144.3

