

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060121\
 Data File : VV021459.D
 Acq On : 01 Jun 2021 14:46
 Operator : SY/MD
 Sample : M2568-05 50X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GN1

Quant Time: Jun 02 00:50:36 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Jun 02 00:49:39 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	243796	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	226428	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	127902	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	36856	3.573	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	71.400%	
7) Chloroethane-d5	1.565	69	39560	4.019	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	80.400%	
11) 1,1-Dichloroethene-d2	2.105	63	53167	2.719	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	54.400%#	
20) 2-Butanone-d5	3.934	46	180188	48.598	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	97.200%	
24) Chloroform-d	4.355	84	123888	4.331	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	86.600%	
26) 1,2-Dichloroethane-d4	5.040	65	60089	4.569	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	91.400%	
32) Benzene-d6	5.053	84	233379	4.284	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	85.600%	
36) 1,2-Dichloropropane-d6	6.076	67	79644	4.508	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	90.200%	
41) Toluene-d8	7.320	98	212394	4.252	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	85.000%	
43) trans-1,3-Dichloroprop...	7.629	79	31425	4.273	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	85.400%	
46) 2-Hexanone-d5	8.095	63	167234	48.299	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	96.600%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	65524	4.602	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	92.000%	
66) 1,2-Dichlorobenzene-d4	11.625	152	99012	4.491	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	89.800%	
Target Compounds						Qvalue
16) Methylene chloride	2.507	84	8519	0.429	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060121\
Data File : VV021459.D
Acq On : 01 Jun 2021 14:46
Operator : SY/MD
Sample : M2568-05 50X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GN1


Quant Time: Jun 02 00:50:36 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Jun 02 00:49:39 2021
Response via : Initial Calibration

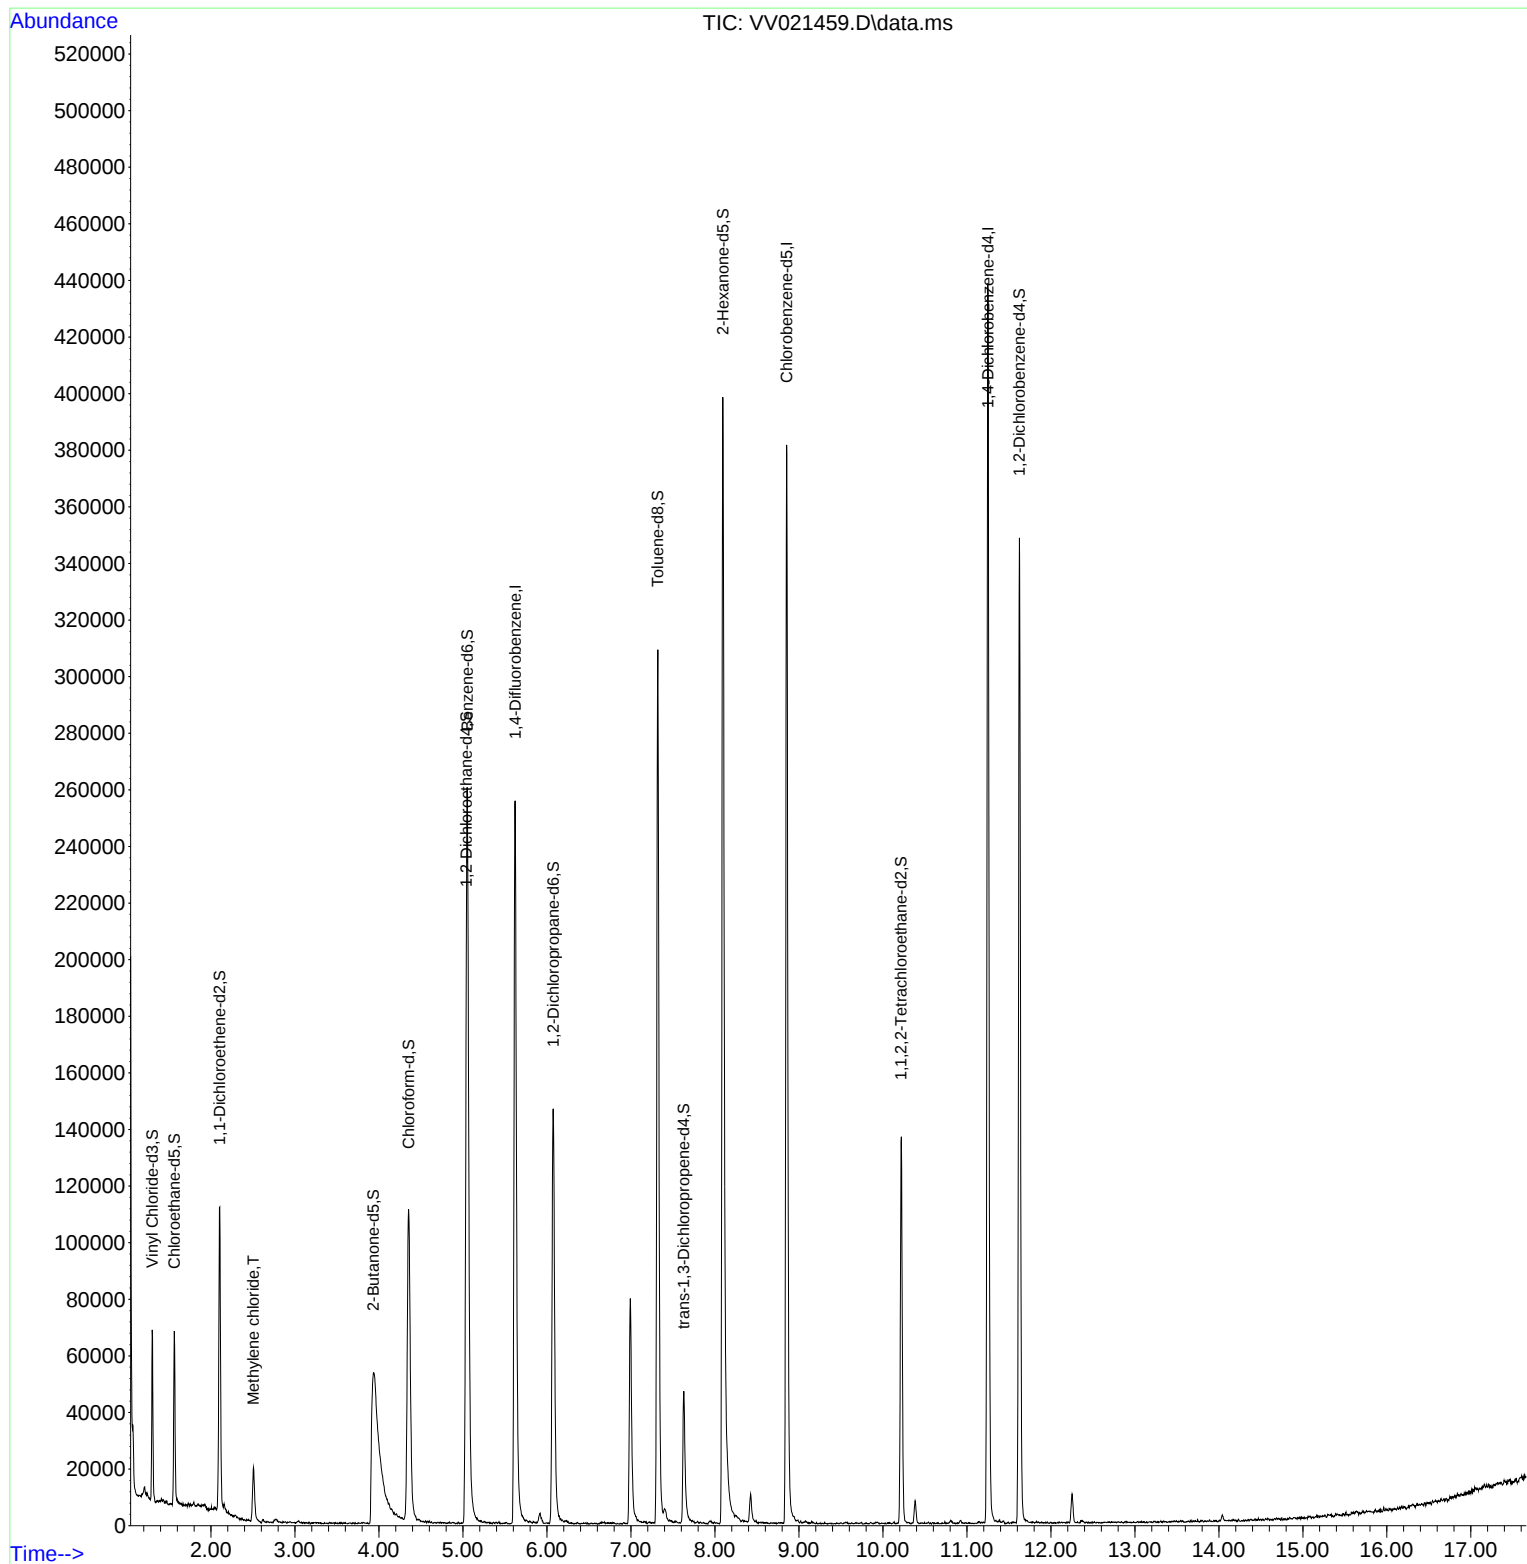

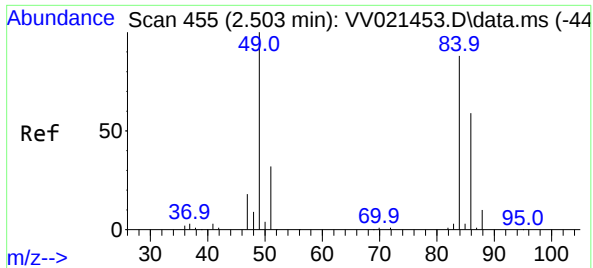

#16
Methylene chloride
Concen: 0.429 ug/L
RT: 2.507 min Scan# 456
Delta R.T. 0.003 min
Lab File: VV021459.D
Acq: 01 Jun 2021 14:46

Instrument :
MSVOA_V
ClientSampleId :
C0GN1

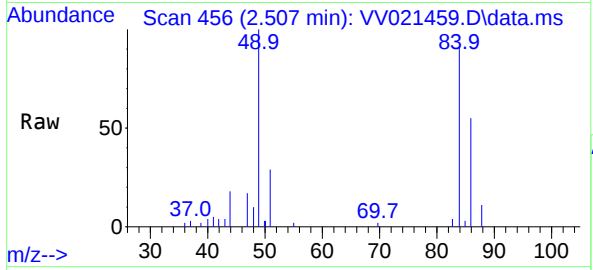

Tgt Ion: 84 Resp: 8519

Ion	Ratio	Lower	Upper
84	100		
86	60.4	44.7	82.9
49	109.8	82.7	153.5

