

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060121\
 Data File : VV021455.D
 Acq On : 01 Jun 2021 13:14
 Operator : SY/MD
 Sample : M2568-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GP1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV021455.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	90	rBV	69285	69137	8.67%	1.080%
2	1.564	154	163	177	rBV	68799	83045	10.41%	1.297%
3	2.105	321	331	344	rBV	116345	171408	21.50%	2.677%
4	2.506	446	456	470	rBV2	23729	39706	4.98%	0.620%
5	3.040	611	622	636	rBV	13980	27753	3.48%	0.433%
6	3.921	880	896	943	rBV	56398	312796	39.23%	4.885%
7	4.349	1011	1029	1060	rBV	116400	295311	37.04%	4.612%
8	5.047	1230	1246	1276	rBV2	267533	674800	84.63%	10.539%
9	5.619	1412	1424	1452	rBV	248618	512349	64.26%	8.002%
10	5.915	1506	1516	1527	rBV5	5744	12016	1.51%	0.188%
11	6.072	1548	1565	1586	rBV	155648	326431	40.94%	5.098%
12	6.989	1835	1850	1873	rBV	82532	160243	20.10%	2.503%
13	7.317	1941	1952	1971	rBV	319265	566724	71.07%	8.851%
14	7.400	1973	1978	1996	rVB3	5310	11572	1.45%	0.181%
15	7.625	2039	2048	2072	rBV	49364	93740	11.76%	1.464%
16	7.940	2137	2146	2159	rBV2	10241	17667	2.22%	0.276%
17	8.091	2182	2193	2223	rBV	411764	797366	100.00%	12.453%
18	8.255	2238	2244	2255	rVB6	5410	9150	1.15%	0.143%
19	8.854	2418	2430	2453	rBV	365942	608979	76.37%	9.511%
20	10.217	2843	2854	2875	rBV	133192	210417	26.39%	3.286%
21	10.381	2895	2905	2918	rBV	19875	32168	4.03%	0.502%
22	11.152	3135	3145	3156	rBV7	7740	13821	1.73%	0.216%
23	11.249	3164	3175	3193	rBV	420747	664152	83.29%	10.373%
24	11.535	3254	3264	3280	rBV2	28683	55666	6.98%	0.869%
25	11.625	3280	3292	3313	rVB	358545	577861	72.47%	9.025%
26	12.345	3504	3516	3530	rBV2	38418	58543	7.34%	0.914%




Sum of corrected areas: 6402821

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060121\
Data File : VV021455.D
Acq On : 01 Jun 2021 13:14
Operator : SY/MD
Sample : M2568-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
C0GP1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

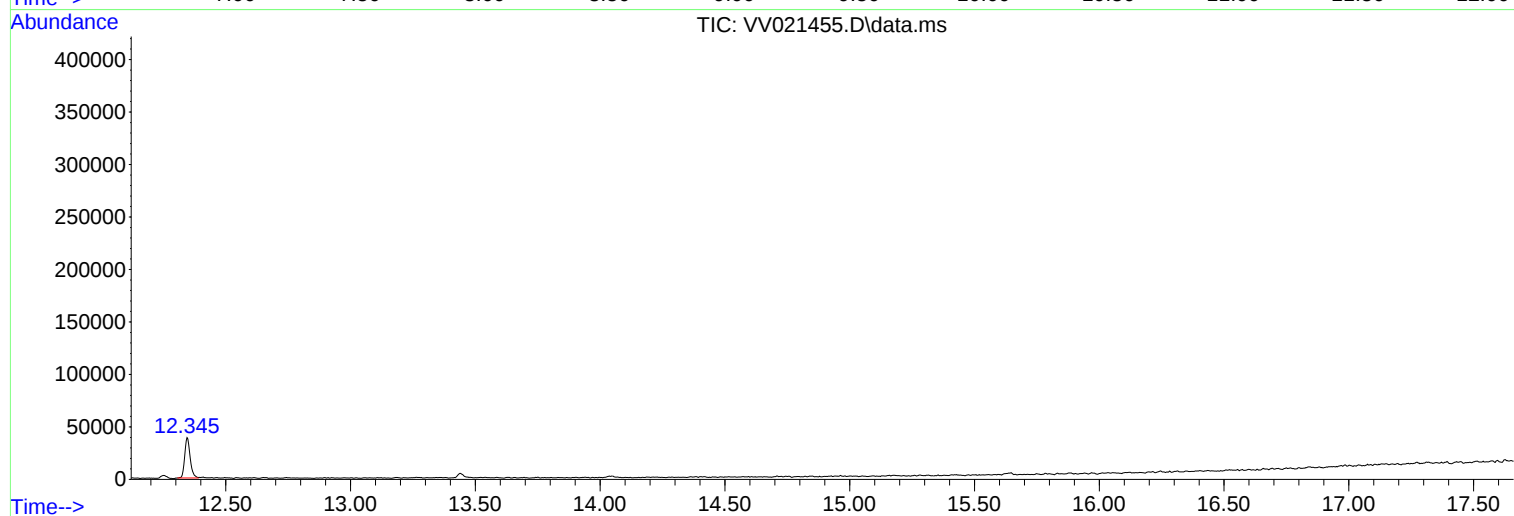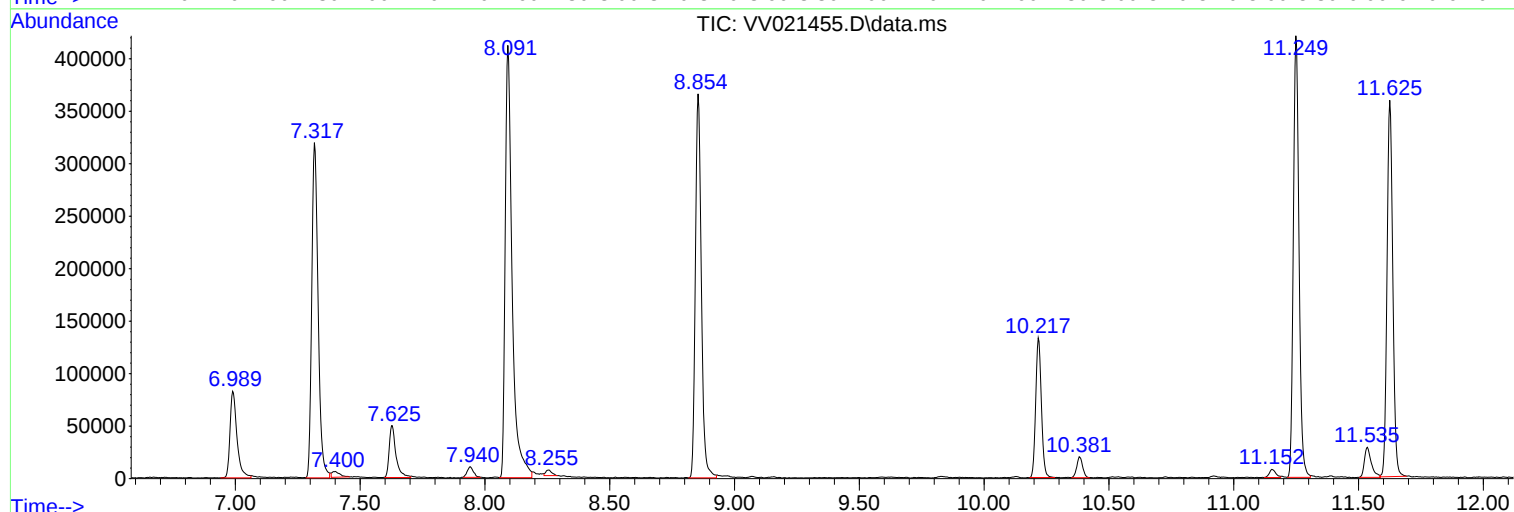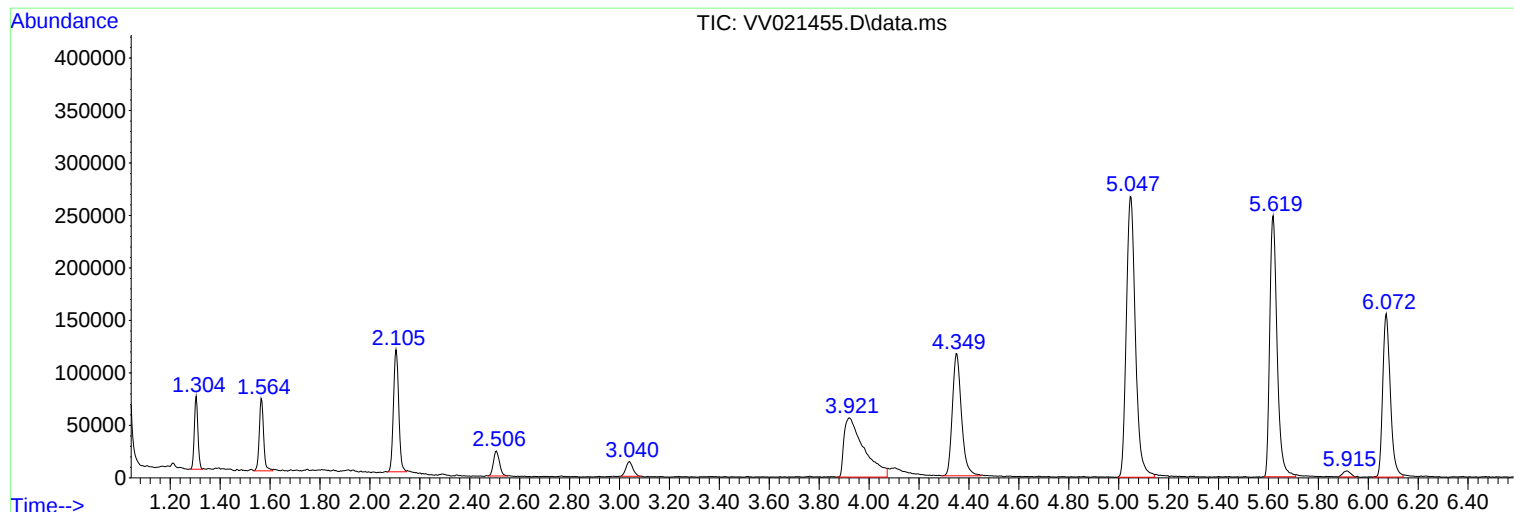

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060121\
Data File : VV021455.D
Acq On : 01 Jun 2021 13:14
Operator : SY/MD
Sample : M2568-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GP1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060121\
Data File : VV021455.D
Acq On : 01 Jun 2021 13:14
Operator : SY/MD
Sample : M2568-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GP1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
