

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060121\
 Data File : VV021459.D
 Acq On : 01 Jun 2021 14:46
 Operator : SY/MD
 Sample : M2568-05 50X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GN1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV021459.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	92	rVB	60872	61143	7.69%	0.996%
2	1.565	155	163	172	rBV	61435	71607	9.00%	1.166%
3	2.105	321	331	344	rBV	106362	151921	19.10%	2.474%
4	2.507	446	456	476	rBV	19108	33584	4.22%	0.547%
5	3.937	883	901	955	rBV3	53451	346474	43.56%	5.642%
6	4.352	1013	1030	1060	rVB	109809	283165	35.60%	4.611%
7	5.050	1230	1247	1280	rBV2	260075	641272	80.62%	10.443%
8	5.622	1409	1425	1451	rBV	255437	525209	66.03%	8.553%
9	6.076	1551	1566	1586	rBV	146630	313968	39.47%	5.113%
10	6.992	1840	1851	1871	rBV	79614	152929	19.23%	2.490%
11	7.320	1942	1953	1973	rBV	308628	537036	67.51%	8.745%
12	7.629	2036	2049	2071	rBV	46698	89845	11.29%	1.463%
13	8.095	2181	2194	2237	rBV	398074	795456	100.00%	12.954%
14	8.426	2285	2297	2313	rBV3	9971	17473	2.20%	0.285%
15	8.854	2419	2430	2455	rBV	380957	626440	78.75%	10.201%
16	10.220	2843	2855	2869	rBV	136519	214431	26.96%	3.492%
17	10.384	2898	2906	2915	rBV	7826	12016	1.51%	0.196%
18	11.249	3163	3175	3202	rBV	437873	695137	87.39%	11.320%
19	11.625	3281	3292	3311	rBV	347906	554991	69.77%	9.038%
20	12.252	3477	3487	3499	rBV2	10341	16624	2.09%	0.271%




Sum of corrected areas: 6140721

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060121\
Data File : VV021459.D
Acq On : 01 Jun 2021 14:46
Operator : SY/MD
Sample : M2568-05 50X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GN1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

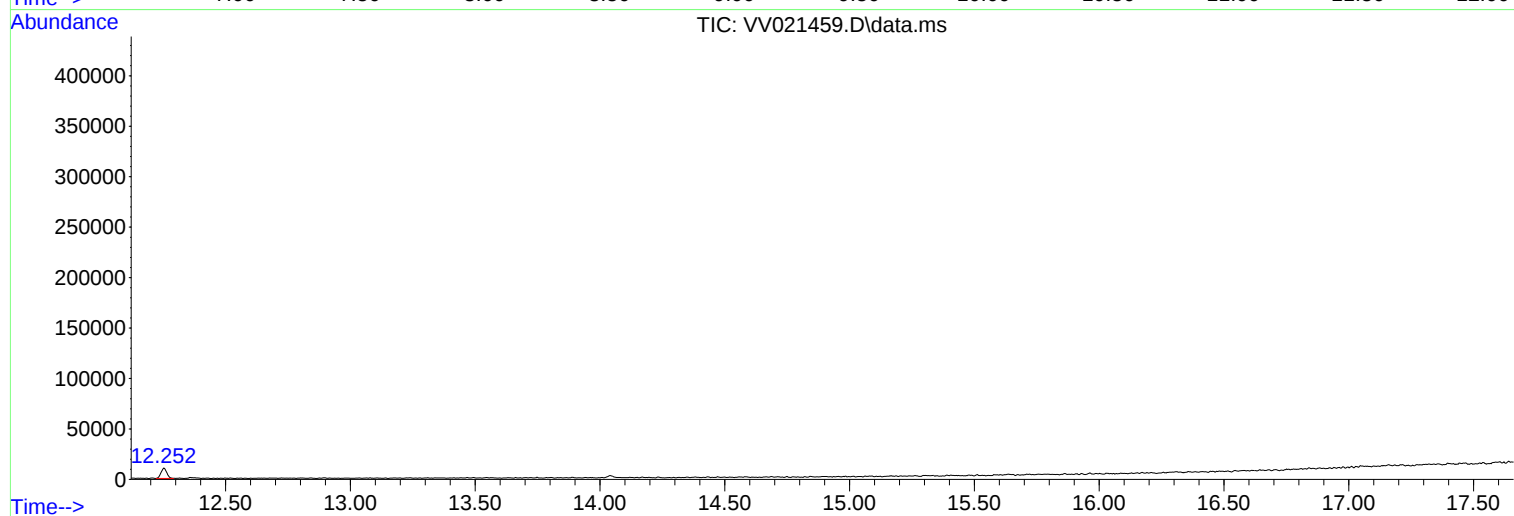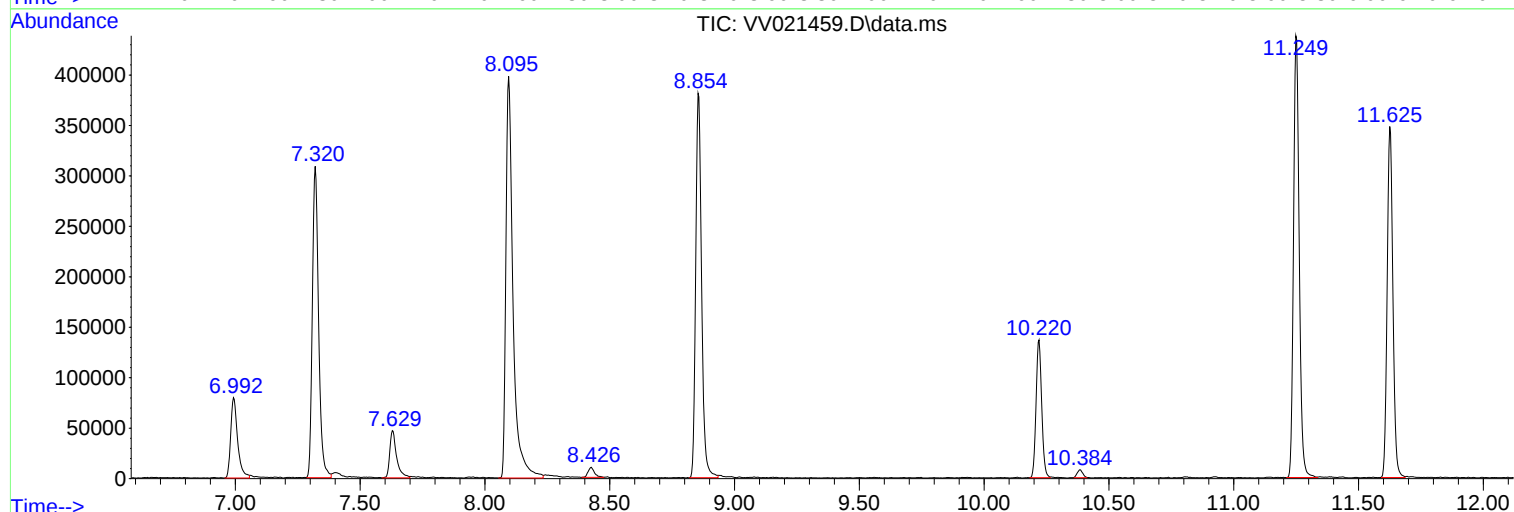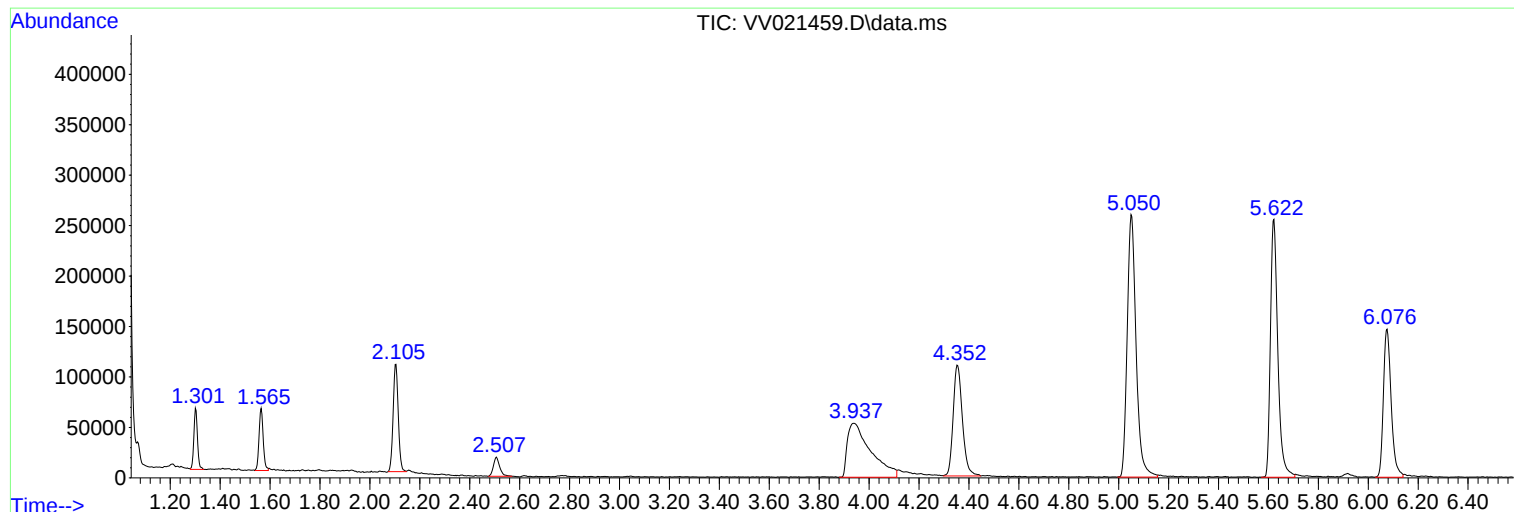

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060121\
Data File : VV021459.D
Acq On : 01 Jun 2021 14:46
Operator : SY/MD
Sample : M2568-05 50X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GN1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060121\
Data File : VV021459.D
Acq On : 01 Jun 2021 14:46
Operator : SY/MD
Sample : M2568-05 50X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GN1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
