
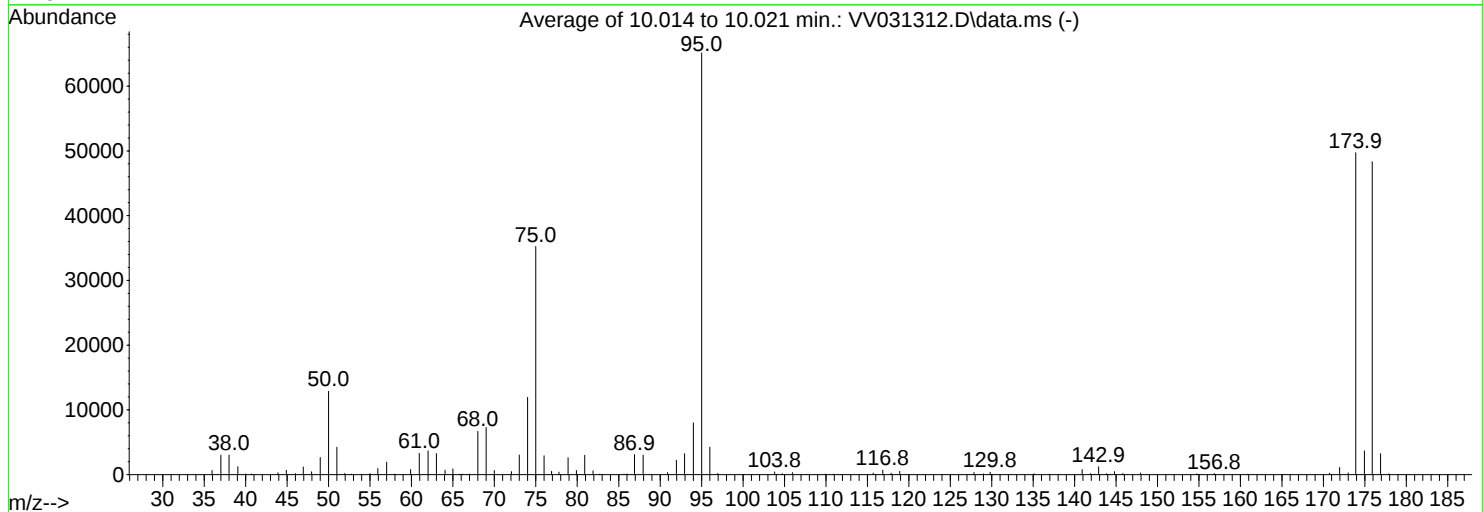


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060123\
 Data File : VV031312.D
 Acq On : 01 Jun 2023 09:37
 Operator : SY/MD
 Sample : BFB268
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB268

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Jun 02 02:28:48 2023

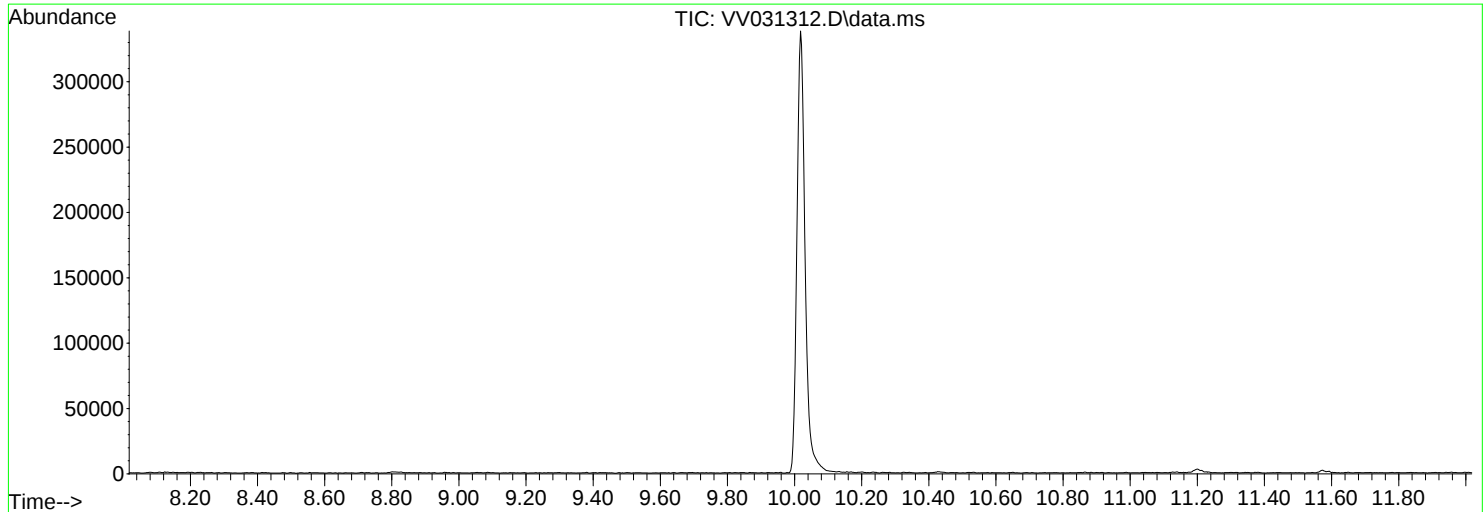

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	12886	PASS
75	95	30	80	54.1	35237	PASS
95	95	100	100	100.0	65139	PASS
96	95	5	9	6.5	4244	PASS
173	174	0.00	2	0.6	277	PASS
174	95	50	120	76.3	49725	PASS
175	174	5	9	7.4	3658	PASS
176	174	95	105	97.2	48328	PASS
177	176	5	10	6.7	3228	PASS

m/z	Abundance
40.00	316.0
42.80	146.0
43.90	390.0
44.90	106.0

Instrument :
MSVOA_V
ClientSampleId :
BFB268

m/z	Abundance
36.00	677.0
37.00	2865.0
38.00	2939.0
39.10	1181.0
40.00	377.0
40.70	161.0
44.00	618.0
44.90	761.0
46.00	184.0
47.00	1239.0
48.00	464.0
49.00	2562.0
50.00	12740.0
51.00	4185.0
51.90	147.0
55.10	186.0
55.90	893.0
57.00	1917.0
59.90	785.0
61.00	3374.0
62.00	3539.0
63.00	3100.0
64.10	686.0
65.00	777.0
65.90	124.0
66.20	122.0
66.80	185.0
68.00	6466.0
69.00	6825.0
70.00	602.0
72.00	432.0
73.00	2888.0
74.00	11475.0
75.00	34632.0
76.00	2848.0
76.90	501.0
77.80	415.0
78.90	2646.0
79.90	660.0
80.90	2799.0
81.90	514.0
82.70	123.0
85.60	122.0
86.00	133.0
86.90	2948.0
88.00	2899.0
90.90	285.0
92.00	2148.0
93.00	3061.0
94.00	7932.0
95.00	63856.0
96.00	4306.0
96.90	221.0
103.80	421.0
104.80	159.0
105.90	328.0
109.90	110.0
115.70	204.0
116.00	158.0
116.90	738.0
117.90	227.0
118.90	521.0
127.90	282.0
128.70	114.0
129.00	114.0
129.80	354.0
135.10	153.0
140.90	870.0
141.90	141.0
142.90	1193.0
143.80	130.0
144.70	446.0
145.80	181.0
147.90	191.0
154.80	103.0
156.80	123.0
161.00	102.0
170.80	143.0
172.00	1034.0
173.00	830.0
173.90	47080.0
174.90	3492.0
175.90	45416.0
176.90	3036.0
177.90	155.0

Instrument :
MSVOA_V
ClientSampleId :
BFB268

m/z	Abundance
35.90	674.0
37.00	3102.0
38.00	3148.0
39.10	1251.0
40.00	407.0
40.70	133.0
44.00	685.0
44.90	795.0
46.00	199.0
47.00	1228.0
47.90	436.0
49.00	2723.0
50.00	13319.0
51.00	4393.0
51.90	191.0
52.70	127.0
55.00	177.0
55.90	945.0
57.00	2020.0
58.00	148.0
59.90	844.0
60.90	3357.0
62.00	3873.0
63.00	3459.0
64.00	731.0
65.00	933.0
65.80	103.0
66.20	106.0
67.00	160.0
68.00	6904.0
69.00	7534.0
70.00	649.0
72.10	490.0
73.00	3169.0
74.00	12346.0
75.00	36392.0
76.00	3000.0
76.90	540.0
77.80	399.0
78.90	2666.0
79.90	649.0
80.90	3106.0
81.90	596.0
82.70	127.0
85.70	133.0
86.00	152.0
86.90	3215.0
87.90	3178.0
90.90	321.0
92.00	2376.0
92.90	3321.0
94.00	8203.0
95.00	67088.0
96.00	4318.0
97.00	182.0
103.80	432.0
104.80	152.0
105.90	333.0
110.00	118.0
110.90	102.0
115.70	269.0
116.90	731.0
117.90	222.0
118.90	527.0
127.80	380.0
129.00	146.0
129.80	390.0
135.10	156.0
136.90	106.0
140.90	802.0
141.90	146.0
142.90	1266.0
143.80	171.0
144.80	476.0
145.80	179.0
148.00	239.0
154.80	126.0
156.90	175.0
170.70	180.0
170.90	180.0
172.00	1137.0
173.90	51704.0
174.90	3703.0
175.90	50032.0
176.90	3341.0
177.90	159.0

Instrument :
MSVOA_V
ClientSampleId :
BFB268

m/z	Abundance
35.90	575.0
37.00	3071.0
38.00	3044.0
39.00	1269.0
40.10	510.0
43.90	749.0
44.90	752.0
46.00	171.0
46.90	1095.0
47.90	417.0
49.00	2631.0
50.00	12598.0
51.00	4131.0
52.00	259.0
52.80	128.0
53.90	137.0
54.90	196.0
56.00	946.0
57.00	1854.0
58.00	173.0
59.90	721.0
60.90	3141.0
62.00	3631.0
63.00	3244.0
64.00	645.0
65.00	993.0
67.00	163.0
68.00	6650.0
69.00	7546.0
70.00	648.0
72.10	501.0
73.00	3097.0
74.00	11973.0
75.00	34688.0
76.00	2914.0
76.90	549.0
77.80	356.0
78.90	2529.0
79.90	635.0
80.90	3060.0
81.90	655.0
82.90	134.0
86.00	116.0
86.90	3104.0
87.90	2951.0
90.90	340.0
91.90	2182.0
92.90	3324.0
94.00	7919.0
95.00	64472.0
96.00	4108.0
96.90	191.0
103.80	395.0
104.70	132.0
106.00	314.0
107.70	134.0
110.00	100.0
110.90	146.0
111.80	100.0
115.70	281.0
116.80	630.0
117.80	234.0
118.90	503.0
127.80	366.0
129.00	132.0
129.80	336.0
135.10	135.0
136.90	115.0
140.90	695.0
141.90	154.0
142.90	1147.0
143.90	185.0
144.90	470.0
145.80	163.0
148.00	281.0
154.70	158.0
156.90	197.0
160.80	117.0
170.70	184.0
171.90	1150.0
173.90	50392.0
175.00	3780.0
175.90	49536.0
176.90	3306.0
177.90	134.0

Instrument :
MSVOA_V
ClientSampleId :
BFB268