


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV060220\
 Data File : VV016422.D
 Acq On : 02 Jun 2020 10:14
 Operator : SY/MD
 Sample : BFB38
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB38

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR053020WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue Jun 02 18:21:27 2020

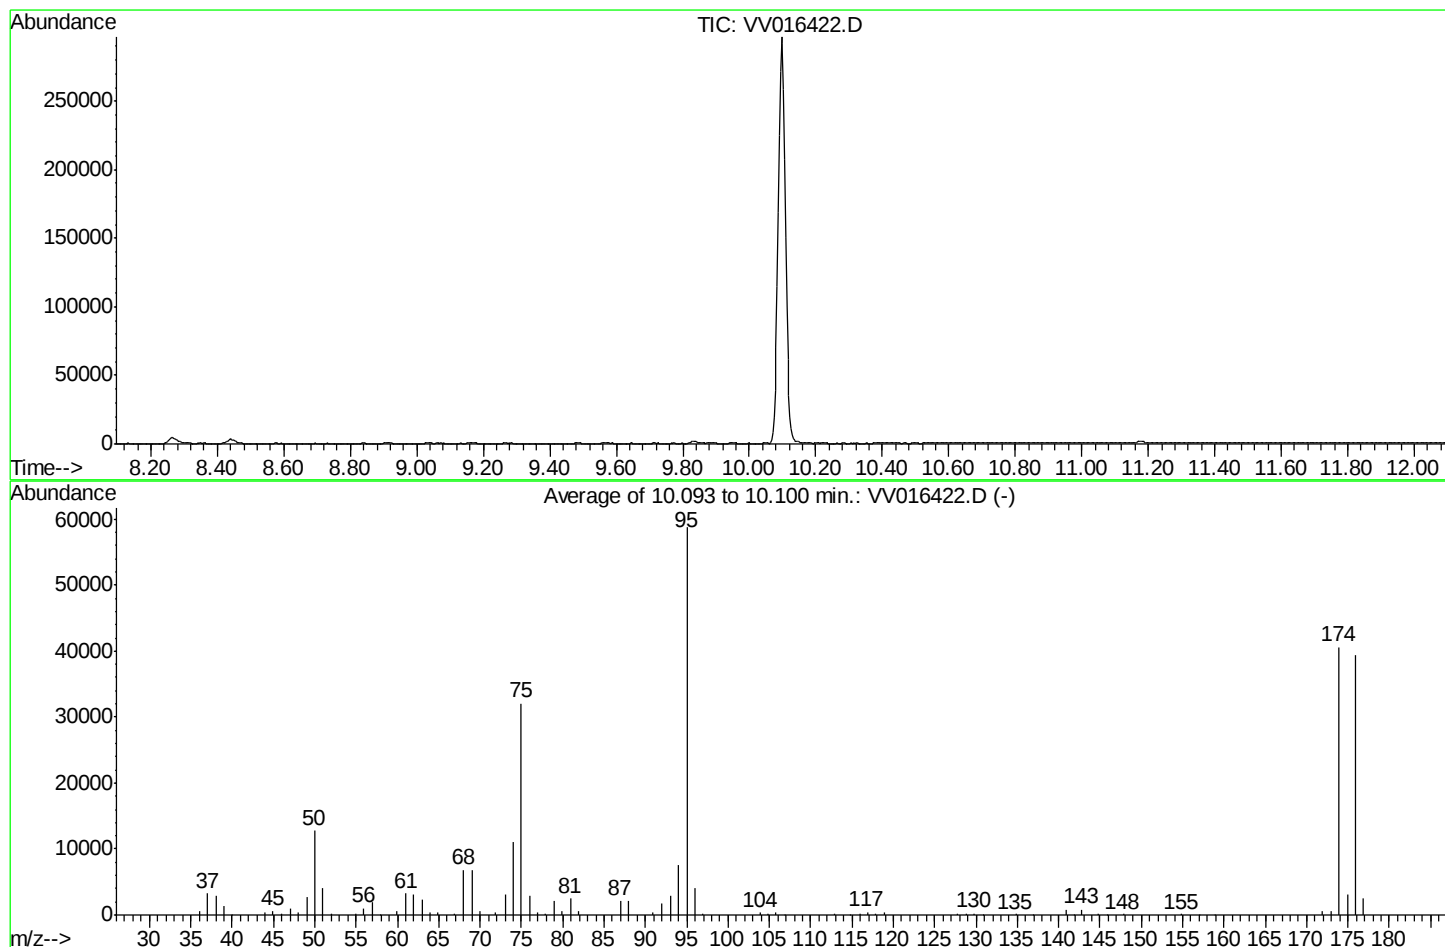

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	12792	PASS
75	95	30	80	54.5	32040	PASS
95	95	100	100	100.0	58762	PASS
96	95	5	9	6.8	3999	PASS
173	174	0.00	2	1.5	606	PASS
174	95	50	120	69.1	40605	PASS
175	174	5	9	7.9	3192	PASS
176	174	95	101	96.9	39352	PASS
177	176	5	9	6.5	2541	PASS

m/z	Abundance
36.00	674.0
37.00	3256.0
38.00	2829.0
39.00	1457.0
39.90	220.0
43.90	631.0
44.90	608.0
46.00	106.0
47.00	931.0
48.00	473.0
49.00	2694.0
50.00	12435.0
51.00	3809.0
52.00	249.0
55.00	219.0
55.90	1024.0
57.00	1893.0
57.90	125.0
59.90	567.0
61.00	3097.0
62.00	2852.0
63.00	2336.0
64.00	315.0
64.90	503.0
66.90	169.0
68.00	6594.0
69.00	6517.0
69.90	549.0
71.90	416.0
73.00	2895.0
74.00	10760.0
75.00	30752.0
76.00	2825.0
77.00	404.0
77.80	207.0
78.90	2119.0
79.90	576.0
80.90	2330.0
81.80	467.0
86.90	1973.0
87.90	1998.0
90.90	293.0
92.00	1716.0
93.00	2793.0
94.00	7186.0
95.00	56248.0
96.00	3906.0
97.00	175.0
103.90	291.0
104.80	151.0
105.80	292.0
112.80	114.0
115.90	263.0
116.90	361.0
117.80	289.0
118.90	407.0
127.80	174.0
128.80	106.0
129.80	260.0
130.90	113.0
134.80	150.0
140.90	616.0
142.80	740.0
144.80	163.0
147.90	125.0
154.80	167.0
157.00	115.0
171.80	468.0
173.00	546.0
173.90	37104.0
174.90	3020.0
175.90	36136.0
176.90	2468.0

Instrument :
MSVOA_V
ClientSampleId :
BFB38

m/z	Abundance
36.00	688.0
37.00	3329.0
38.00	3069.0
39.00	1469.0
39.90	215.0
44.00	648.0
44.90	647.0
46.00	123.0
47.00	950.0
47.90	507.0
49.00	2874.0
50.00	13242.0
51.00	4335.0
51.90	281.0
54.90	251.0
55.90	1072.0
57.00	1977.0
57.90	117.0
59.90	613.0
61.00	3322.0
62.00	3166.0
63.00	2459.0
64.00	305.0
64.90	487.0
66.90	204.0
68.00	7121.0
69.00	7012.0
69.90	581.0
71.90	386.0
73.00	3134.0
74.00	11507.0
75.00	33248.0
76.00	3012.0
77.00	424.0
77.90	212.0
78.90	2194.0
79.90	687.0
80.90	2541.0
81.90	523.0
87.00	2237.0
87.90	2212.0
90.90	351.0
92.00	1891.0
93.00	3016.0
94.00	7774.0
95.00	60800.0
96.00	4120.0
96.90	180.0
103.90	319.0
104.80	169.0
105.80	315.0
106.80	104.0
112.80	107.0
115.90	287.0
116.90	448.0
117.80	264.0
118.90	416.0
127.80	212.0
128.80	126.0
129.80	256.0
130.90	113.0
134.80	146.0
140.90	732.0
141.90	105.0
142.80	811.0
144.80	146.0
145.80	120.0
147.90	169.0
154.80	181.0
171.90	527.0
173.00	613.0
173.90	42080.0
174.90	3289.0
175.90	40696.0
176.90	2580.0

Instrument :
MSVOA_V
ClientSampleId :
BFB38

m/z	Abundance
36.00	618.0
37.00	3185.0
38.00	2986.0
39.00	1343.0
39.90	194.0
44.00	638.0
44.90	643.0
46.00	119.0
47.00	881.0
47.90	444.0
49.00	2704.0
50.00	12700.0
51.00	4301.0
51.90	269.0
54.90	238.0
56.00	1039.0
57.00	1953.0
60.00	567.0
61.00	3256.0
62.00	3216.0
63.00	2464.0
64.00	313.0
64.90	415.0
66.90	222.0
68.00	6802.0
69.00	6852.0
69.90	552.0
71.90	333.0
73.00	3188.0
74.00	11089.0
75.00	32120.0
76.00	2808.0
77.00	405.0
78.00	209.0
78.90	2109.0
79.90	731.0
80.90	2510.0
81.90	505.0
87.00	2311.0
87.90	2159.0
90.90	333.0
92.00	1925.0
93.00	2894.0
94.00	7645.0
95.00	59240.0
96.00	3972.0
96.90	160.0
103.90	353.0
104.80	142.0
105.80	323.0
112.80	107.0
114.80	102.0
115.90	273.0
116.80	486.0
117.80	233.0
118.90	334.0
127.70	223.0
128.80	142.0
129.80	194.0
134.80	118.0
136.90	102.0
140.80	777.0
141.90	115.0
142.80	828.0
144.80	145.0
145.80	133.0
147.80	191.0
154.90	177.0
158.80	112.0
171.90	568.0
172.90	660.0
173.90	42632.0
174.90	3267.0
175.90	41224.0
176.90	2577.0

Instrument :
MSVOA_V
ClientSampleId :
BFB38

Scan 2788 (10.055 min): VV016422.D
BFB38

m/z	Abundance
39.90	200.0
43.90	313.0

Instrument :
MSVOA_V
ClientSampleId :
BFB38