

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060221\
 Data File : VV021471.D
 Acq On : 02 Jun 2021 11:09
 Operator : SY/MD
 Sample : M2568-06DL 2000X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GN3DL

Quant Time: Jun 03 02:16:15 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jun 03 02:14:36 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	233563	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	219877	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	121805	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	55331	5.599	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	112.000%
7) Chloroethane-d5	1.564	69	45451	4.820	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.400%
11) 1,1-Dichloroethene-d2	2.101	63	74940	4.001	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	80.000%
20) 2-Butanone-d5	3.928	46	120449	33.909	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	67.820%
24) Chloroform-d	4.346	84	113261	4.133	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.600%
26) 1,2-Dichloroethane-d4	5.034	65	52815	4.192	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.800%
32) Benzene-d6	5.050	84	240143	4.540	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.800%
36) 1,2-Dichloropropane-d6	6.069	67	71931	4.193	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	83.800%
41) Toluene-d8	7.317	98	230027	4.742	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.800%
43) trans-1,3-Dichloroprop...	7.625	79	28526	3.995	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.800%
46) 2-Hexanone-d5	8.092	63	109889	32.683	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	65.360%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	51133	3.698	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	74.000%
66) 1,2-Dichlorobenzene-d4	11.625	152	95760	4.561	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	91.200%
Target Compounds						Qvalue
34) Trichloroethene	5.912	95	135997	8.629	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060221\
Data File : VV021471.D
Acq On : 02 Jun 2021 11:09
Operator : SY/MD
Sample : M2568-06DL 2000X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GN3DL

Quant Time: Jun 03 02:16:15 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jun 03 02:14:36 2021
Response via : Initial Calibration

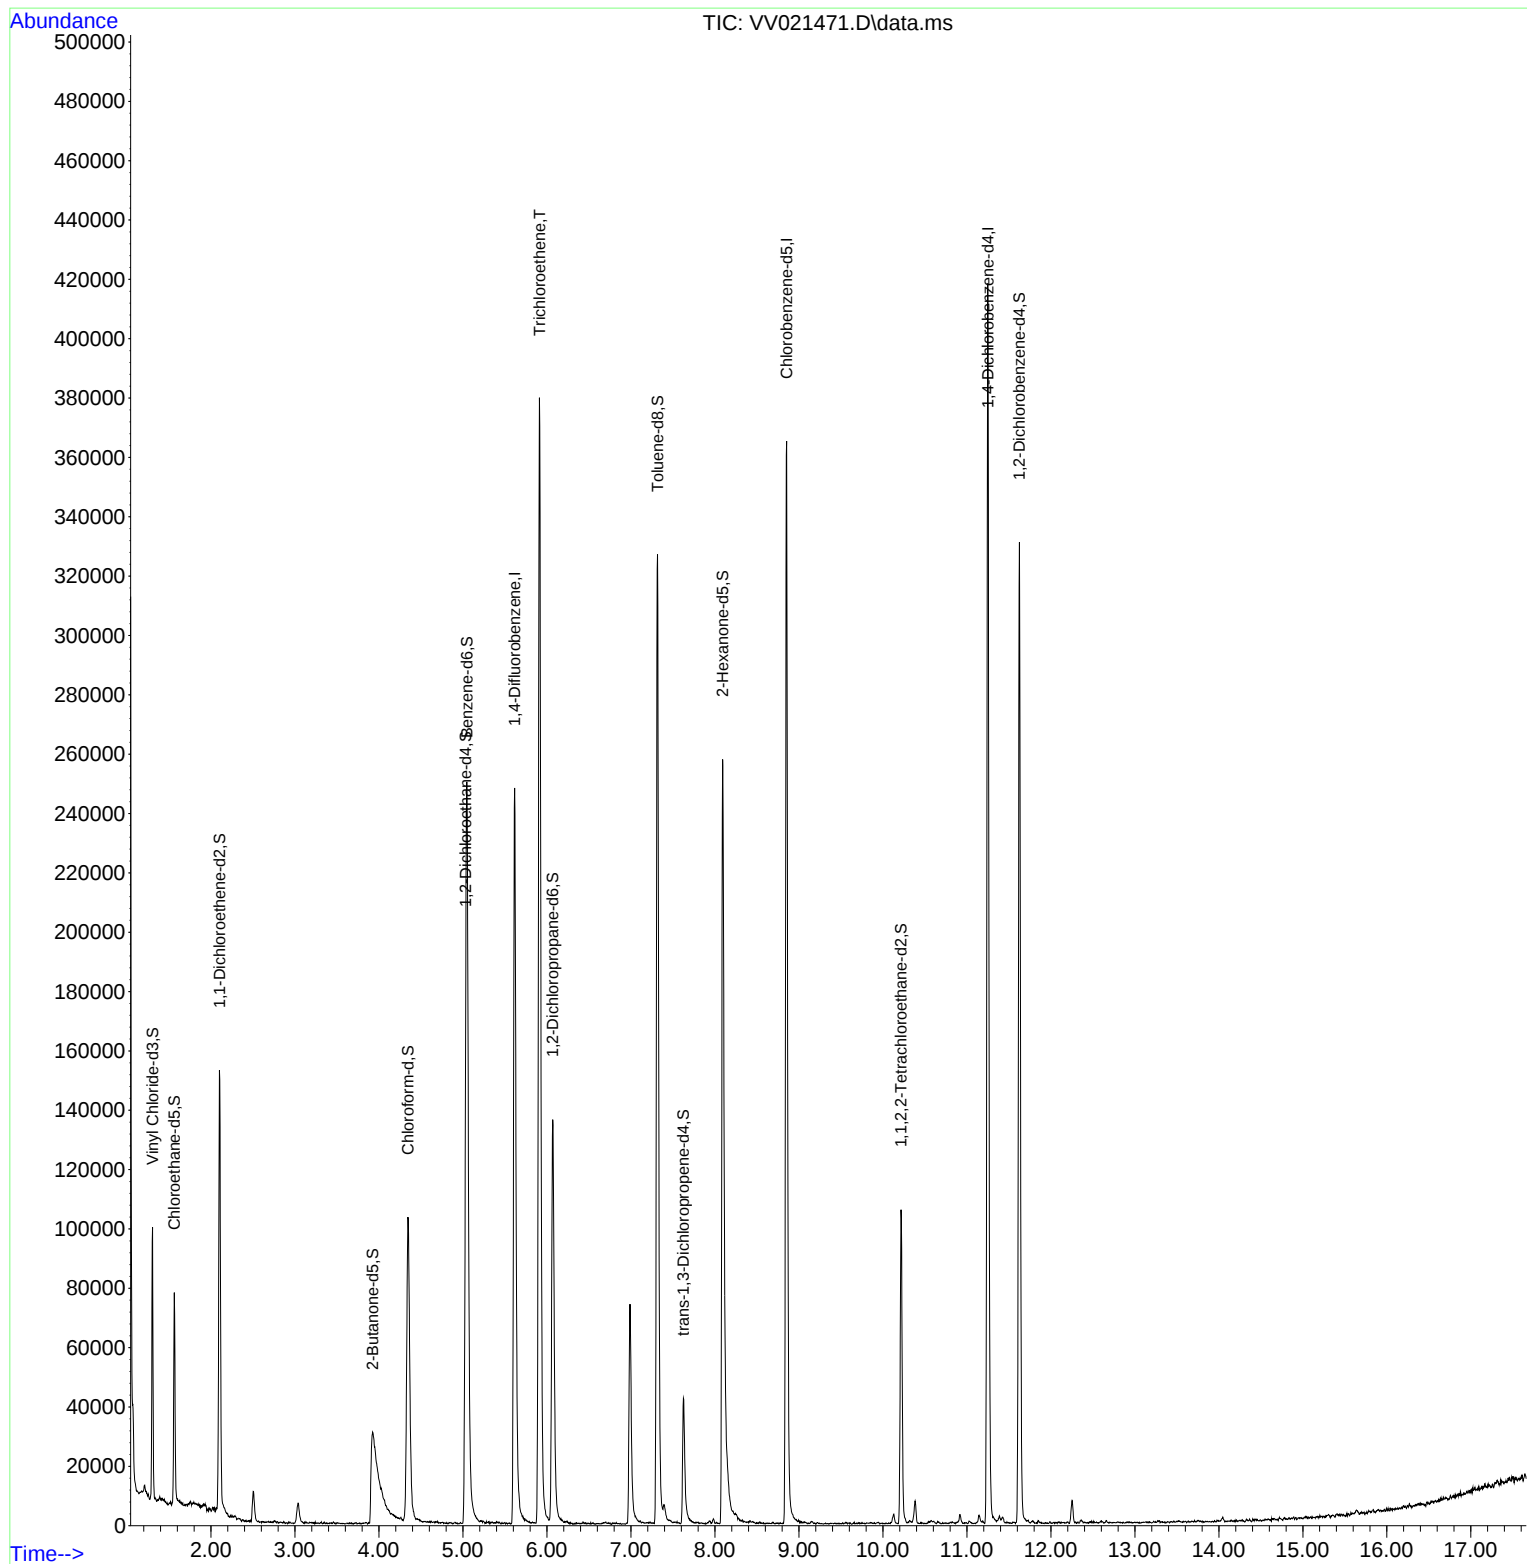

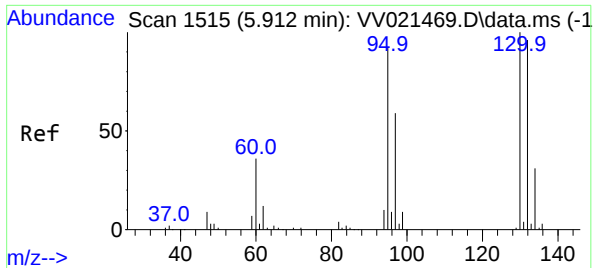

#34
 Trichloroethene
 Concen: 8.629 ug/L
 RT: 5.912 min Scan# 1515
 Delta R.T. -0.000 min
 Lab File: VV021471.D
 Acq: 02 Jun 2021 11:09

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GN3DL

Tgt Ion: 95 Resp: 135997

Ion	Ratio	Lower	Upper
95	100		
97	65.3	45.4	84.4
132	107.5	74.5	138.3
130	113.5	77.7	144.3

