

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060221\
 Data File : VV021472.D
 Acq On : 02 Jun 2021 11:32
 Operator : SY/MD
 Sample : M2568-07DL 2000X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GN4DL

Quant Time: Jun 03 02:16:23 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jun 03 02:14:36 2021
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	235980	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	217241	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	124700	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	58299	5.839	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	116.800%	
7) Chloroethane-d5	1.564	69	47744	5.011	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	100.200%	
11) 1,1-Dichloroethene-d2	2.105	63	76213	4.027	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	80.600%	
20) 2-Butanone-d5	3.924	46	119253	33.229	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	66.460%	
24) Chloroform-d	4.352	84	119511	4.316	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	86.400%	
26) 1,2-Dichloroethane-d4	5.037	65	56499	4.438	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	88.800%	
32) Benzene-d6	5.053	84	251853	4.819	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	96.400%	
36) 1,2-Dichloropropane-d6	6.072	67	74467	4.393	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	87.800%	
41) Toluene-d8	7.320	98	240293	5.014	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	100.200%	
43) trans-1,3-Dichloroprop...	7.628	79	30555	4.331	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	86.600%	
46) 2-Hexanone-d5	8.095	63	118194	35.579	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	71.160%	
56) 1,1,2,2-Tetrachloroeth...	10.220	84	55444	4.058	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	81.200%	
66) 1,2-Dichlorobenzene-d4	11.625	152	100606	4.681	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	93.600%	
Target Compounds						
34) Trichloroethene	5.915	95	147069	9.445	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060221\
Data File : VV021472.D
Acq On : 02 Jun 2021 11:32
Operator : SY/MD
Sample : M2568-07DL 2000X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GN4DL


Quant Time: Jun 03 02:16:23 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jun 03 02:14:36 2021
Response via : Initial Calibration

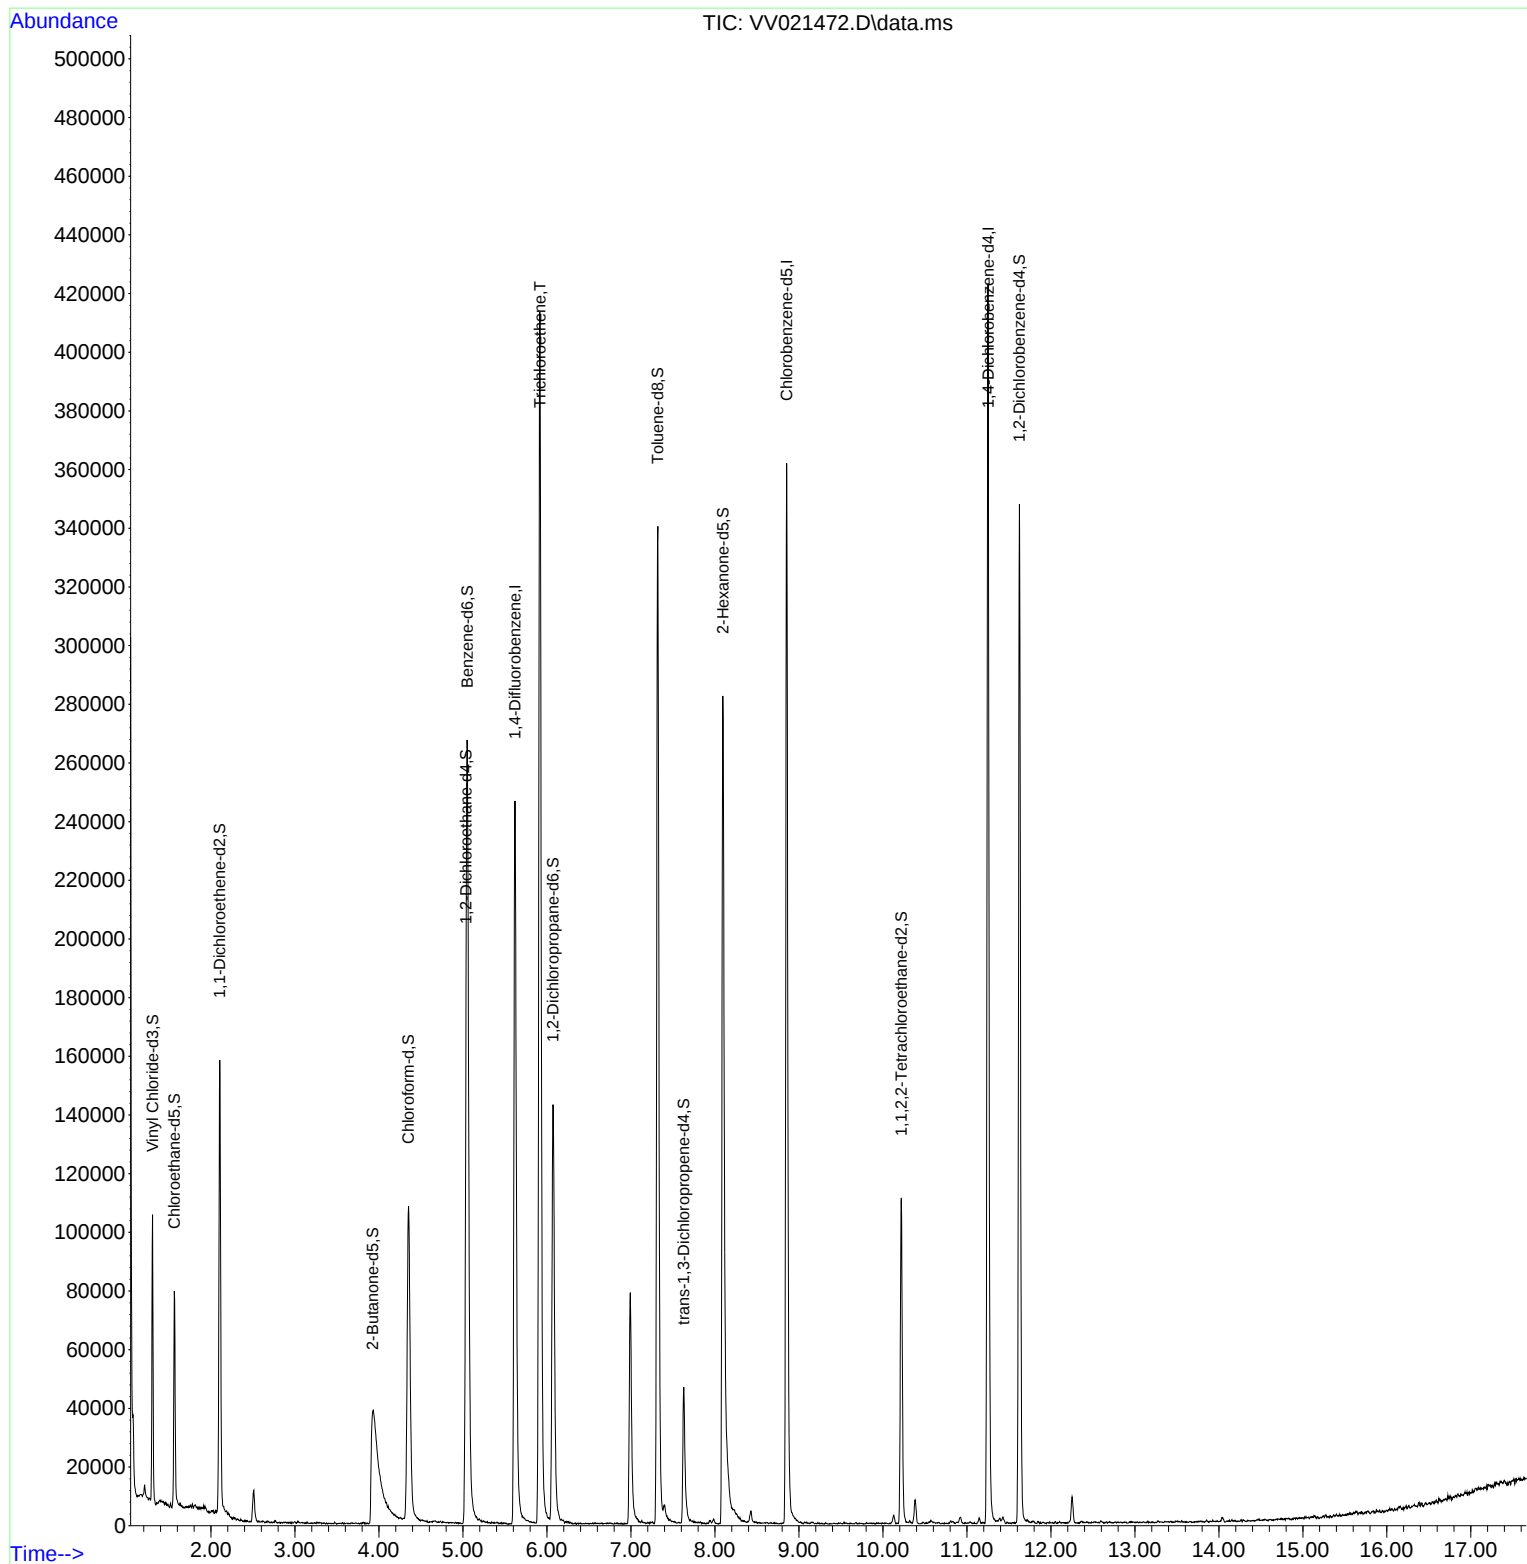

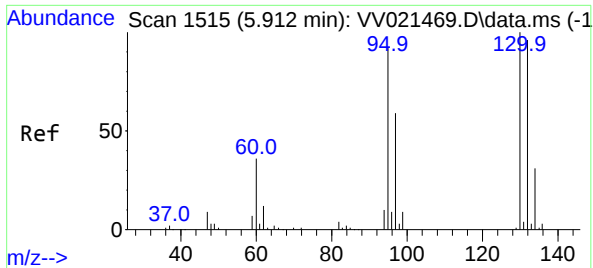

#34
 Trichloroethene
 Concen: 9.445 ug/L
 RT: 5.915 min Scan# 1516
 Delta R.T. 0.003 min
 Lab File: VV021472.D
 Acq: 02 Jun 2021 11:32

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GN4DL

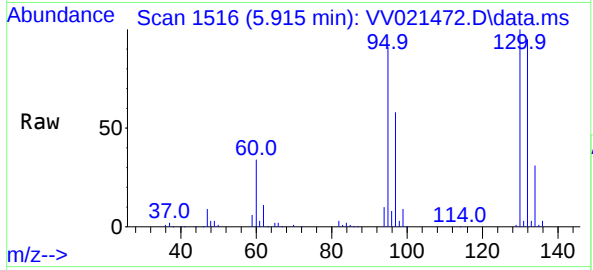

Tgt Ion: 95 Resp: 147069

Ion	Ratio	Lower	Upper
95	100		
97	63.2	45.4	84.4
132	104.8	74.5	138.3
130	109.8	77.7	144.3

