

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060221\
 Data File : VV021477.D
 Acq On : 02 Jun 2021 13:35
 Operator : SY/MD
 Sample : M2568-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Jun 03 02:17:00 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Jun 03 02:14:36 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	224885	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	209962	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	119643	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	53335	5.606	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	112.200%	
7) Chloroethane-d5	1.564	69	43534	4.795	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	95.800%	
11) 1,1-Dichloroethene-d2	2.101	63	69260	3.840	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	76.800%	
20) 2-Butanone-d5	3.934	46	125882	36.806	ug/L	0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	=	73.620%	
24) Chloroform-d	4.349	84	111277	4.217	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	84.400%	
26) 1,2-Dichloroethane-d4	5.037	65	52250	4.307	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	86.200%	
32) Benzene-d6	5.050	84	232197	4.597	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	92.000%	
36) 1,2-Dichloropropane-d6	6.072	67	69780	4.260	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	85.200%	
41) Toluene-d8	7.317	98	223059	4.815	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	96.400%	
43) trans-1,3-Dichloroprop...	7.628	79	26002	3.813	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	76.200%	
46) 2-Hexanone-d5	8.095	63	107971	33.629	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	67.260%	
56) 1,1,2,2-Tetrachloroeth...	10.220	84	49760	3.769	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	75.400%	
66) 1,2-Dichlorobenzene-d4	11.625	152	92315	4.477	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	89.600%	
Target Compounds						Qvalue
16) Methylene chloride	2.506	84	10284	0.561	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060221\
Data File : VV021477.D
Acq On : 02 Jun 2021 13:35
Operator : SY/MD
Sample : M2568-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Jun 03 02:17:00 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Jun 03 02:14:36 2021
Response via : Initial Calibration

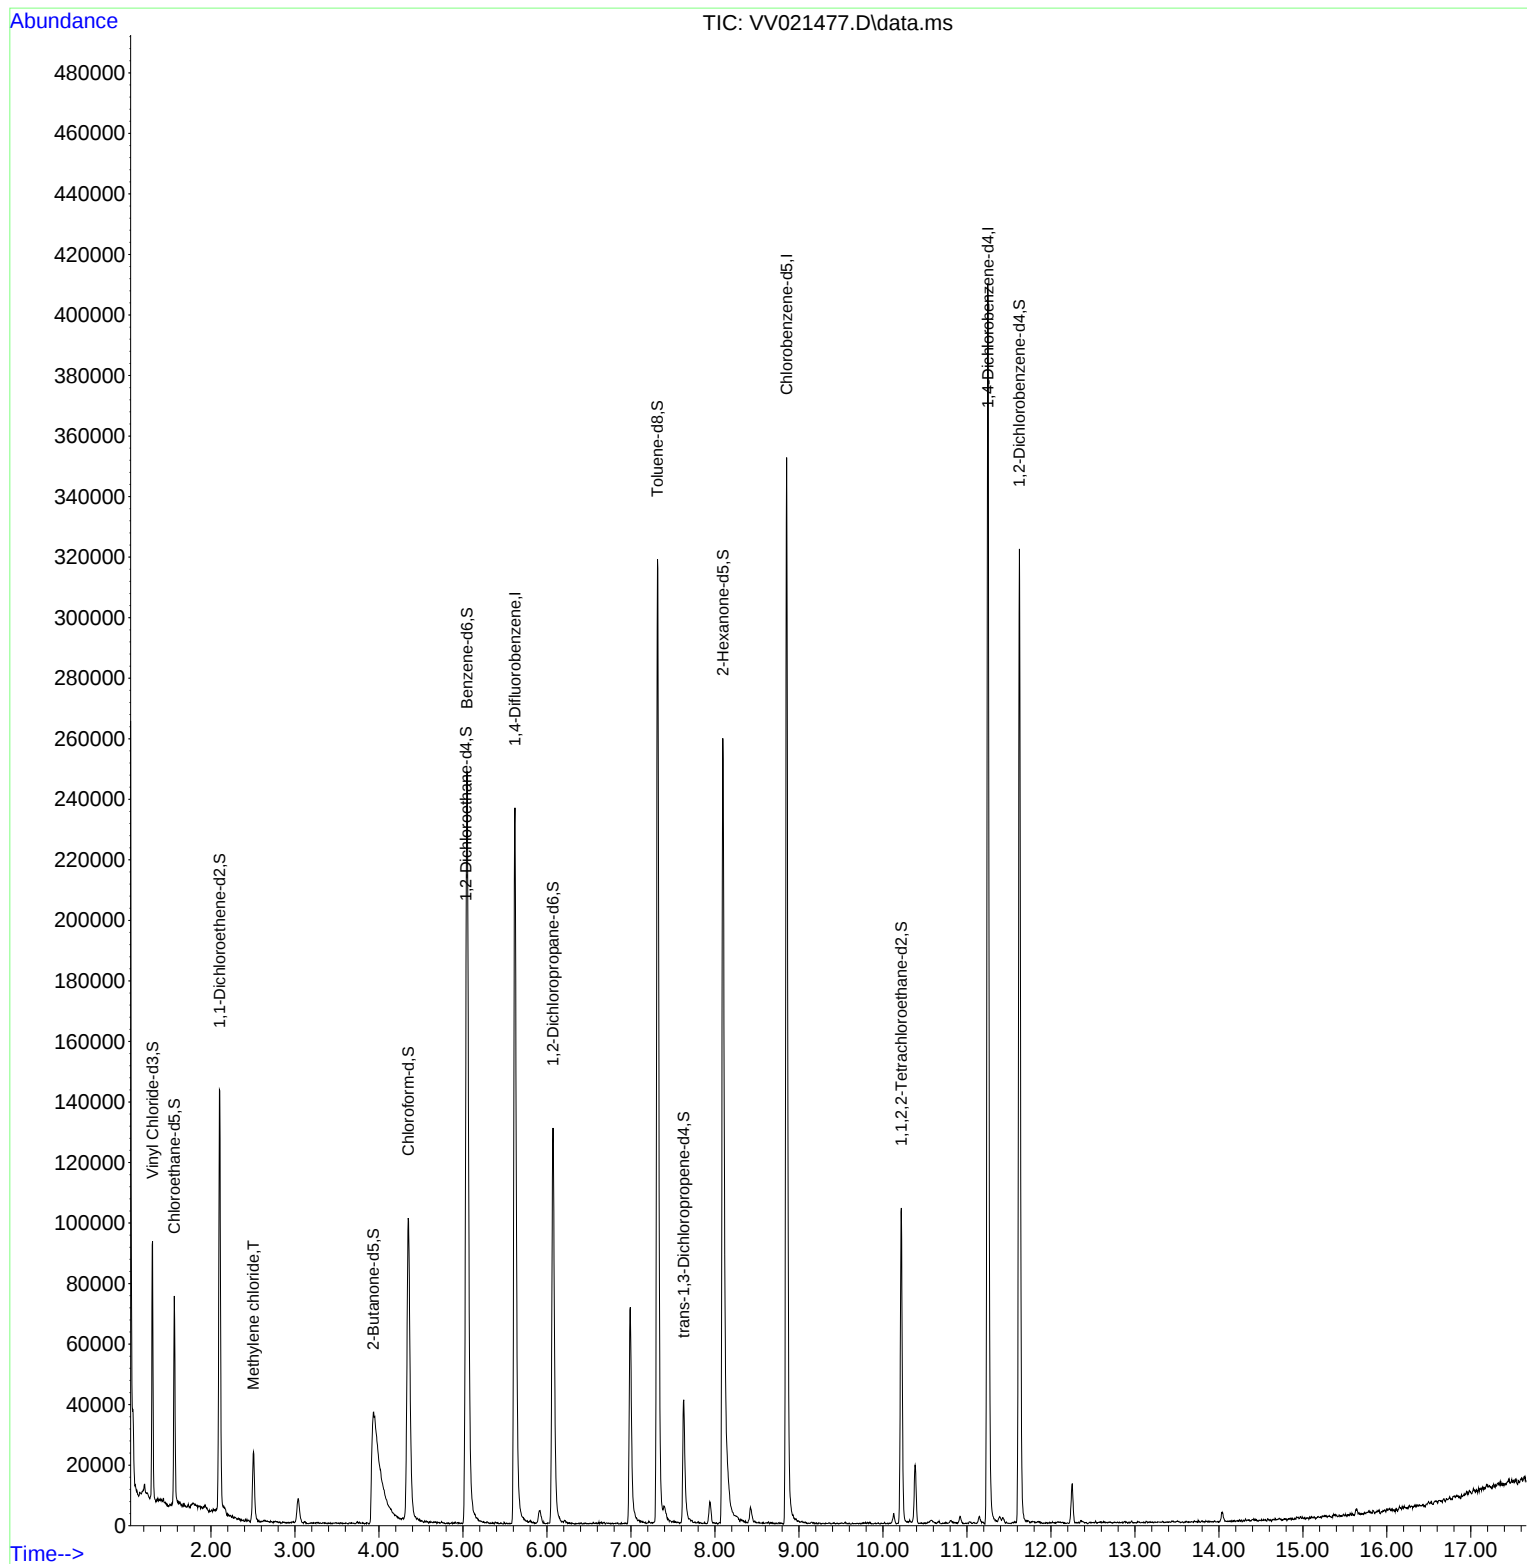

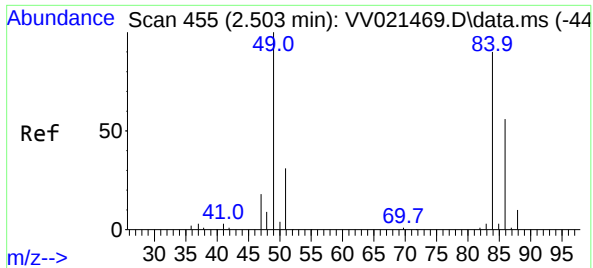

#16
Methylene chloride
Concen: 0.561 ug/L
RT: 2.506 min Scan# 456
Delta R.T. 0.003 min
Lab File: VV021477.D
Acq: 02 Jun 2021 13:35

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Tgt Ion:	84	Resp:	10284
Ion	Ratio	Lower	Upper
84	100		
86	71.3	44.7	82.9
49	113.6	82.7	153.5

