

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060221\
 Data File : VV021470.D
 Acq On : 02 Jun 2021 10:32
 Operator : SY/MD
 Sample : VV0602WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK183

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV021470.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	94	rVB	95393	95976	14.63%	1.705%
2	1.564	156	163	176	rBV	73774	84548	12.89%	1.502%
3	2.104	320	331	346	rBV	148720	215400	32.83%	3.826%
4	2.506	447	456	467	rBV	11569	19525	2.98%	0.347%
5	3.937	887	901	904	rBV2	35002	72355	11.03%	1.285%
6	4.352	1015	1030	1058	rVB2	106241	267404	40.76%	4.750%
7	5.050	1230	1247	1291	rBV2	262508	656034	100.00%	11.653%
8	5.619	1405	1424	1454	rBV	242310	497612	75.85%	8.839%
9	5.915	1505	1516	1531	rVB10	4613	10567	1.61%	0.188%
10	6.072	1552	1565	1597	rBV	139137	298353	45.48%	5.299%
11	6.992	1840	1851	1871	rBV	77168	149041	22.72%	2.647%
12	7.316	1939	1952	1972	rBV	335929	600677	91.56%	10.670%
13	7.628	2038	2049	2073	rBV	44560	86718	13.22%	1.540%
14	8.095	2184	2194	2238	rBV	275558	593307	90.44%	10.539%
15	8.853	2417	2430	2450	rBV	348647	583156	88.89%	10.358%
16	10.220	2843	2855	2871	rBV	109988	177589	27.07%	3.154%
17	10.381	2895	2905	2914	rVB	7335	12204	1.86%	0.217%
18	11.249	3165	3175	3193	rBV	411030	647820	98.75%	11.507%
19	11.625	3280	3292	3313	rBV	343425	546814	83.35%	9.713%
20	12.252	3478	3487	3499	rVB4	9124	14745	2.25%	0.262%




Sum of corrected areas: 5629845

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060221\
Data File : VV021470.D
Acq On : 02 Jun 2021 10:32
Operator : SY/MD
Sample : VV0602WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK183

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

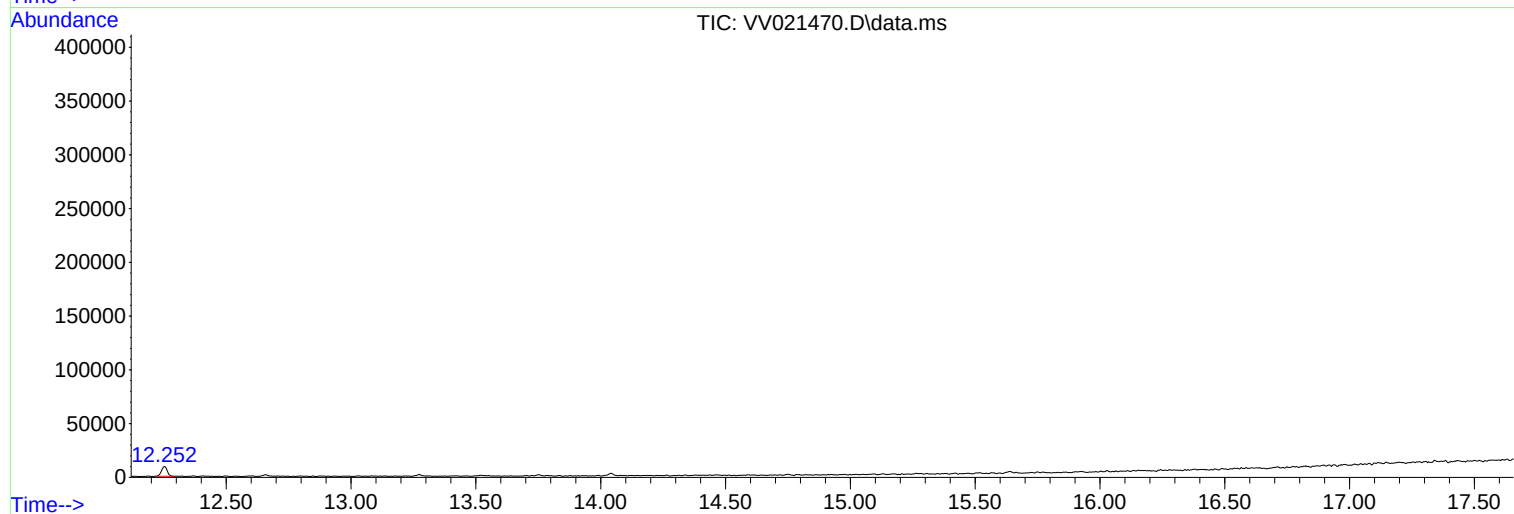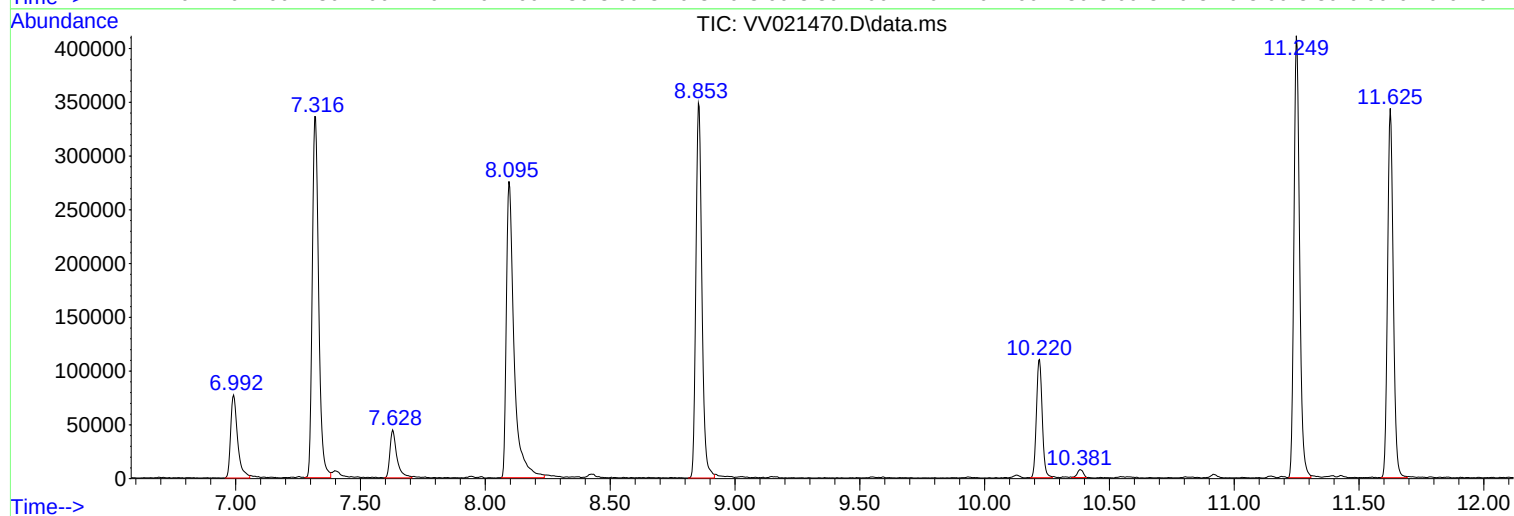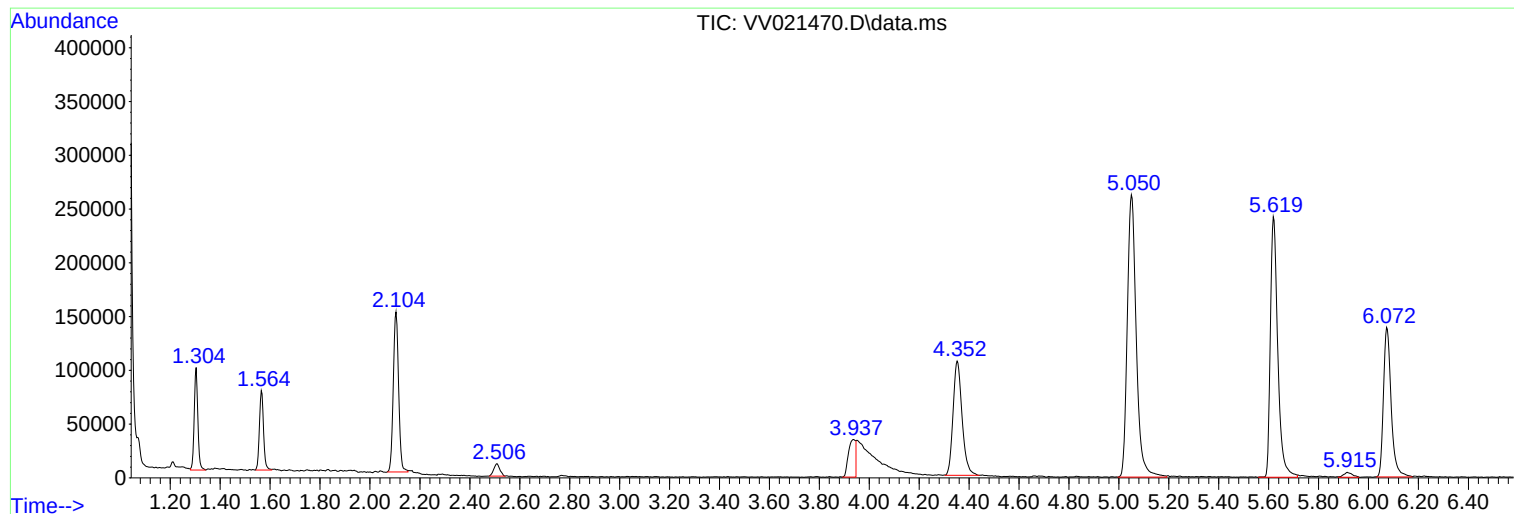

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060221\
Data File : VV021470.D
Acq On : 02 Jun 2021 10:32
Operator : SY/MD
Sample : VV0602WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK183

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060221\
Data File : VV021470.D
Acq On : 02 Jun 2021 10:32
Operator : SY/MD
Sample : VV0602WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK183

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
