

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060221\
 Data File : VV021472.D
 Acq On : 02 Jun 2021 11:32
 Operator : SY/MD
 Sample : M2568-07DL 2000X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GN4DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV021472.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	94	rVB	98970	97666	11.80%	1.461%
2	1.564	154	163	179	rBV	73933	89948	10.87%	1.346%
3	2.105	321	331	344	rBV	153850	220168	26.61%	3.294%
4	2.510	447	457	470	rBV2	10755	18606	2.25%	0.278%
5	3.931	882	899	941	rBV3	38770	230120	27.81%	3.443%
6	4.352	1015	1030	1063	rBV	106419	267954	32.38%	4.009%
7	5.050	1228	1247	1288	rBV2	267159	664540	80.31%	9.943%
8	5.619	1410	1424	1451	rBV	246543	505517	61.09%	7.563%
9	5.915	1502	1516	1540	rBV	412843	827453	100.00%	12.380%
10	6.072	1553	1565	1593	rVB	141624	296399	35.82%	4.435%
11	6.992	1838	1851	1871	rBV	78895	151582	18.32%	2.268%
12	7.320	1941	1953	1972	rBV	339936	609860	73.70%	9.124%
13	7.628	2038	2049	2071	rBV	46325	86236	10.42%	1.290%
14	8.095	2183	2194	2227	rBV	282144	586012	70.82%	8.768%
15	8.853	2419	2430	2460	rBV	361185	598232	72.30%	8.950%
16	10.220	2843	2855	2875	rBV	110994	182167	22.02%	2.725%
17	10.384	2896	2906	2915	rBV3	7991	13062	1.58%	0.195%
18	11.252	3165	3176	3198	rBV	422498	669422	80.90%	10.016%
19	11.625	3280	3292	3315	rBV	347133	555466	67.13%	8.311%
20	12.252	3479	3487	3497	rVB	8845	13408	1.62%	0.201%




Sum of corrected areas: 6683818

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060221\
Data File : VV021472.D
Acq On : 02 Jun 2021 11:32
Operator : SY/MD
Sample : M2568-07DL 2000X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GN4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

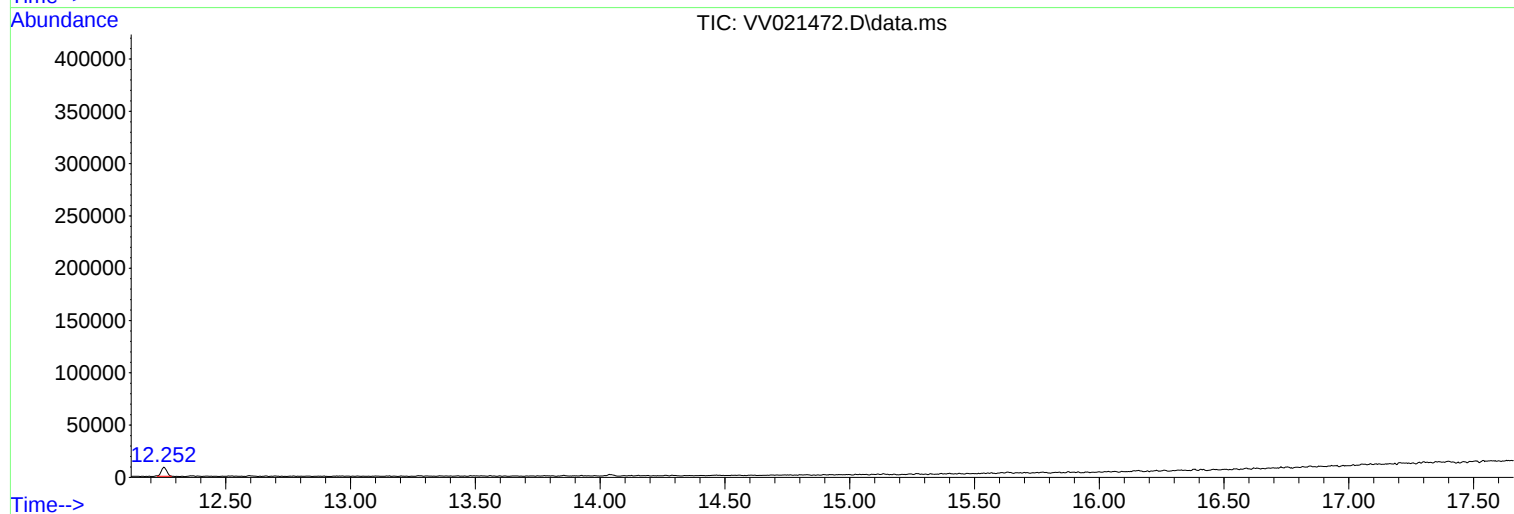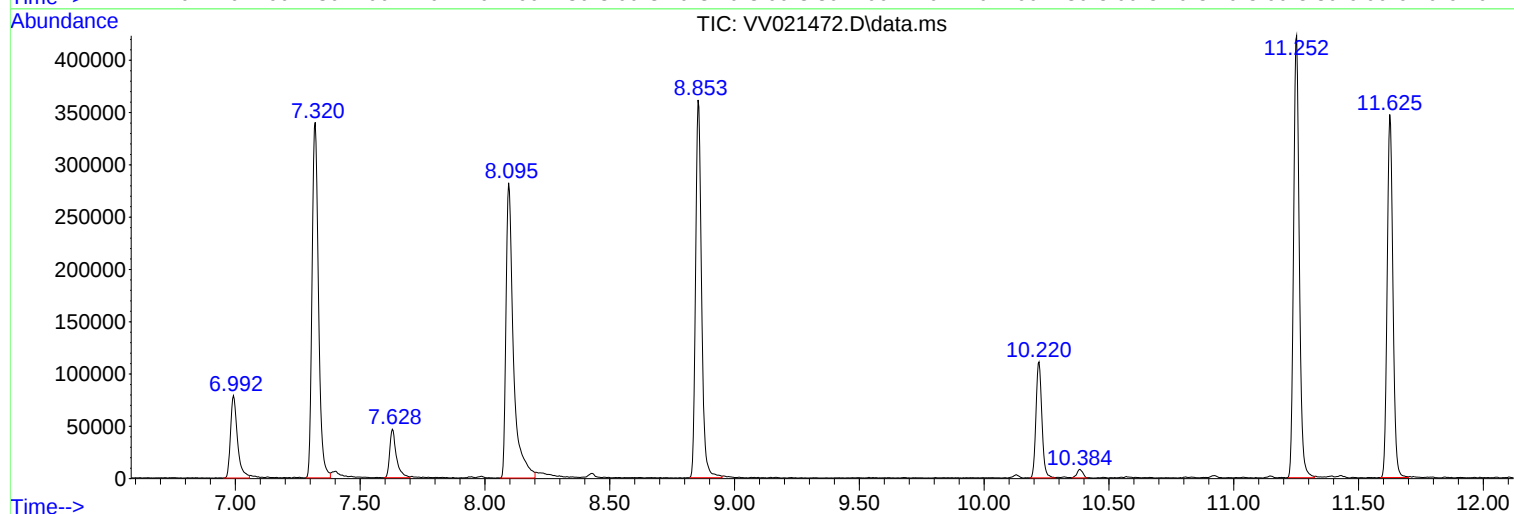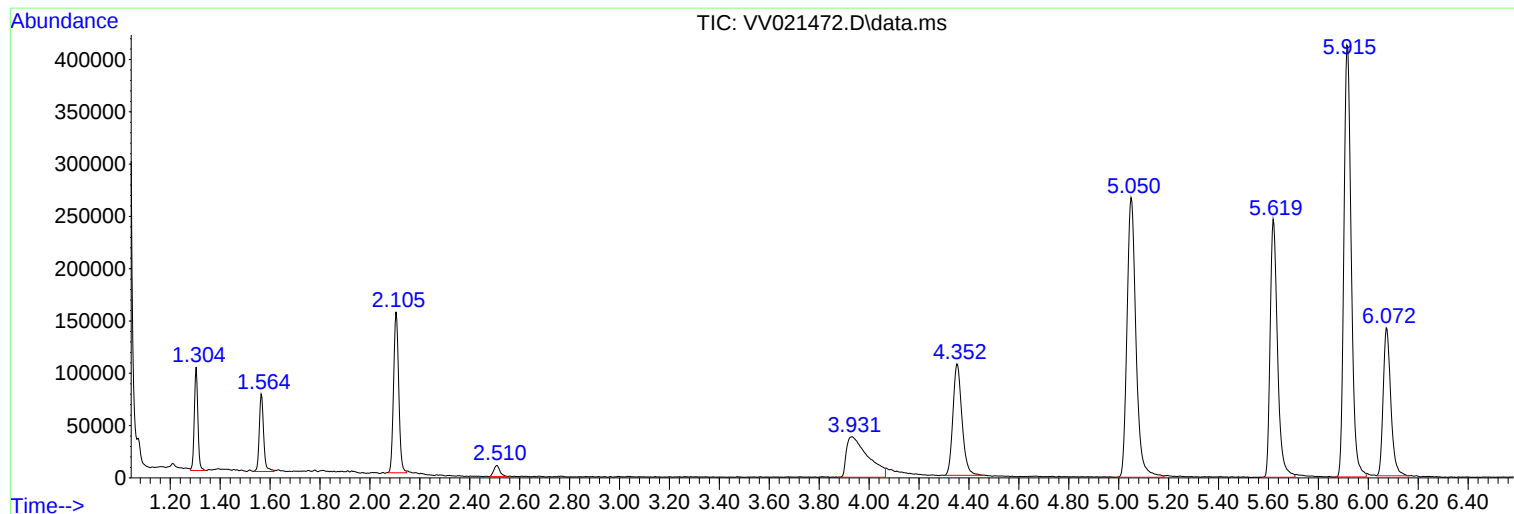

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060221\
Data File : VV021472.D
Acq On : 02 Jun 2021 11:32
Operator : SY/MD
Sample : M2568-07DL 2000X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GN4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060221\
Data File : VV021472.D
Acq On : 02 Jun 2021 11:32
Operator : SY/MD
Sample : M2568-07DL 2000X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GN4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
