

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060221\
 Data File : VV021473.D
 Acq On : 02 Jun 2021 11:56
 Operator : SY/MD
 Sample : M2568-01DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0GN0DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV021473.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	92	rVB	91799	90624	13.77%	1.437%
2	1.565	155	163	178	rBV	72399	84481	12.84%	1.340%
3	2.105	320	331	347	rBV	144577	208892	31.74%	3.313%
4	2.507	447	456	466	rBV2	10886	18251	2.77%	0.289%
5	3.934	886	900	944	rBV2	38706	236705	35.96%	3.755%
6	4.352	1014	1030	1055	rBV	103406	260546	39.58%	4.133%
7	5.050	1230	1247	1281	rBV2	257152	637251	96.82%	10.108%
8	5.619	1412	1424	1448	rBV	234311	482971	73.38%	7.661%
9	5.918	1504	1517	1548	rBV	324708	658208	100.00%	10.441%
10	6.072	1553	1565	1587	rVV	134037	283365	43.05%	4.495%
11	6.992	1840	1851	1877	rBV	74094	148202	22.52%	2.351%
12	7.320	1941	1953	1973	rBV	331261	588633	89.43%	9.337%
13	7.400	1973	1978	1990	rVB6	4853	8774	1.33%	0.139%
14	7.629	2040	2049	2070	rBV	42711	80600	12.25%	1.278%
15	8.095	2184	2194	2234	rBV	265237	573294	87.10%	9.094%
16	8.854	2418	2430	2453	rBV	345509	578119	87.83%	9.170%
17	10.220	2844	2855	2877	rBV	108350	174213	26.47%	2.763%
18	10.381	2896	2905	2918	rVB2	5627	8523	1.29%	0.135%
19	11.249	3164	3175	3194	rBV	403682	637256	96.82%	10.108%
20	11.625	3280	3292	3311	rBV	334522	534264	81.17%	8.475%
21	12.252	3478	3487	3499	rVB2	6742	11176	1.70%	0.177%


Sum of corrected areas: 6304348

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060221\
Data File : VV021473.D
Acq On : 02 Jun 2021 11:56
Operator : SY/MD
Sample : M2568-01DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GN0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

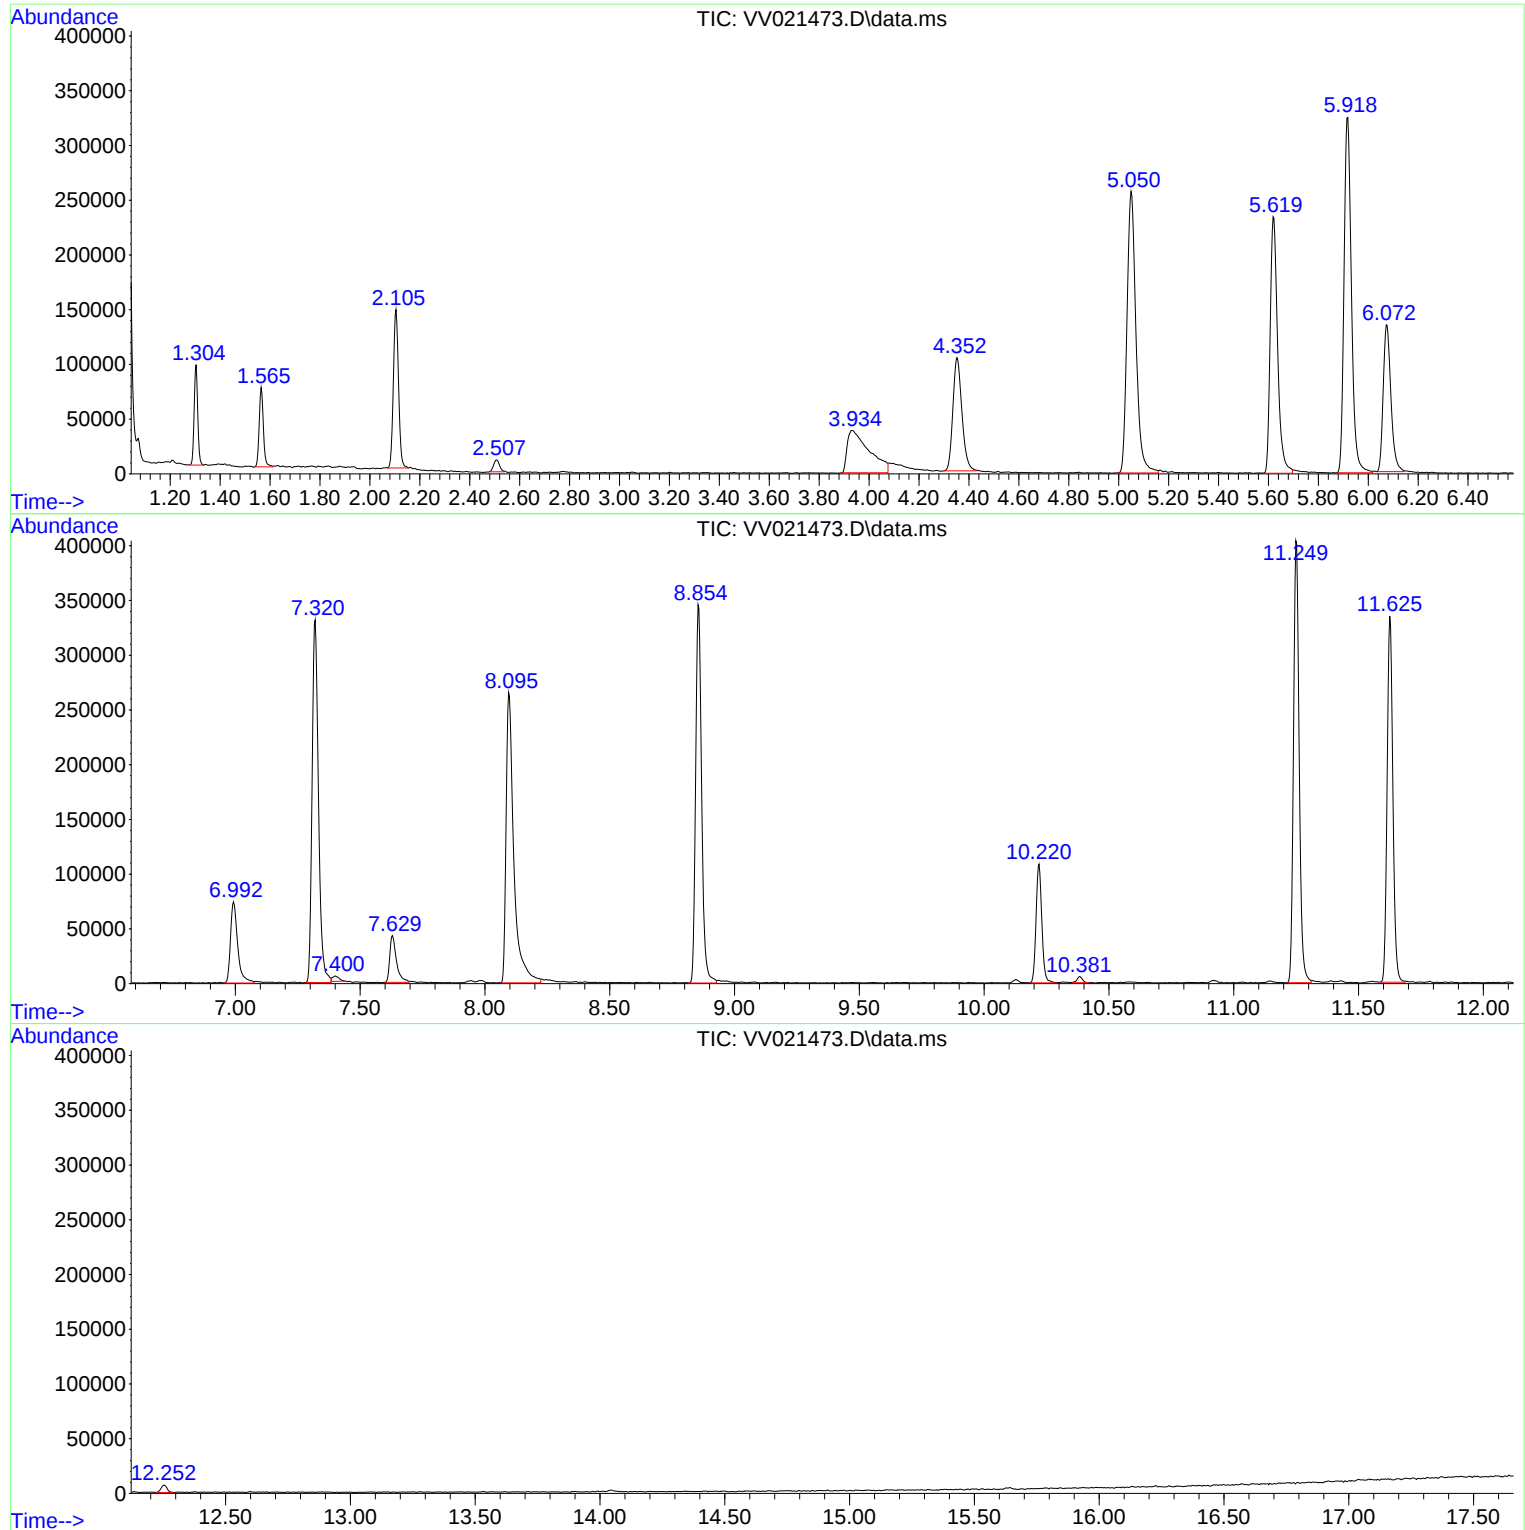

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060221\
Data File : VV021473.D
Acq On : 02 Jun 2021 11:56
Operator : SY/MD
Sample : M2568-01DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GN0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060221\
Data File : VV021473.D
Acq On : 02 Jun 2021 11:56
Operator : SY/MD
Sample : M2568-01DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0GN0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
