

m/z	Abundance
38.90	105.0
40.00	226.0
41.10	106.0
43.90	517.0
207.10	104.0

Instrument :
MSVOA_V
ClientSampleId :
BFB65

m/z	Abundance
36.00	879.0
37.00	4731.0
38.00	4089.0
39.10	1771.0
39.90	244.0
42.90	153.0
43.90	1037.0
45.00	916.0
46.00	144.0
46.90	1672.0
47.90	795.0
49.00	4507.0
50.00	20728.0
51.00	6652.0
51.90	323.0
55.00	405.0
56.00	1695.0
57.00	3063.0
58.00	192.0
59.90	1156.0
61.00	5223.0
62.00	5454.0
63.00	3714.0
63.90	400.0
64.90	140.0
67.10	356.0
68.00	12379.0
69.00	12676.0
70.00	1026.0
72.00	742.0
73.00	5911.0
74.00	20648.0
75.00	62344.0
76.00	5505.0
77.00	758.0
77.90	542.0
78.90	3471.0
79.90	1130.0
80.90	3550.0
81.90	745.0
82.90	139.0
86.00	129.0
86.90	5322.0
87.90	5571.0
90.90	460.0
92.00	3876.0
93.00	5361.0
94.00	15368.0
95.00	136896.0
96.00	8949.0
96.90	241.0
103.90	526.0
104.90	249.0
105.80	605.0
106.90	179.0
111.00	170.0
111.80	133.0
112.80	129.0
114.80	135.0
115.80	513.0
116.90	854.0
117.80	587.0
118.80	659.0
127.90	607.0
128.90	275.0
129.90	695.0
130.90	194.0
134.80	325.0
136.80	279.0
139.80	126.0
140.90	1511.0
142.00	204.0
142.90	1668.0
143.90	108.0
144.90	142.0
145.80	251.0
147.80	296.0
148.80	114.0
149.90	182.0
152.80	112.0
153.90	130.0
154.90	311.0
156.80	293.0
158.90	179.0
160.90	160.0
171.90	349.0
173.00	1165.0
173.90	135936.0
175.00	9556.0
175.90	133696.0
176.90	9093.0
177.90	273.0

Instrument :
MSVOA_V
ClientSampleId :
BFB65

m/z	Abundance
36.00	996.0
37.00	4922.0
38.00	4340.0
39.10	1958.0
39.90	247.0
40.80	106.0
42.90	153.0
43.90	980.0
45.00	934.0
46.00	151.0
46.90	1745.0
47.90	841.0
49.00	4732.0
50.00	21936.0
51.00	7116.0
51.90	330.0
55.00	399.0
56.00	1826.0
57.00	3314.0
58.00	212.0
59.90	1290.0
61.00	5482.0
62.00	5898.0
63.00	4155.0
63.90	442.0
64.90	148.0
66.80	366.0
68.00	13357.0
69.00	13195.0
70.00	1054.0
72.00	728.0
73.00	6136.0
74.00	22456.0
75.00	65296.0
76.00	5857.0
77.00	785.0
77.90	590.0
78.90	3570.0
79.90	1150.0
80.90	3629.0
81.90	788.0
83.00	142.0
85.60	101.0
86.00	134.0
86.90	5677.0
87.90	5865.0
90.90	433.0
92.00	3998.0
93.00	5653.0
94.00	16374.0
95.00	142592.0
96.00	9606.0
96.90	278.0
103.90	523.0
104.90	282.0
105.80	577.0
106.80	179.0
111.00	159.0
111.80	104.0
112.80	120.0
114.90	134.0
115.80	494.0
116.90	920.0
117.80	612.0
118.80	647.0
123.80	118.0
127.90	658.0
128.90	274.0
129.90	660.0
130.80	213.0
134.70	338.0
136.90	268.0
139.80	121.0
140.90	1526.0
142.00	212.0
142.90	1704.0
143.90	124.0
144.80	114.0
145.80	329.0
146.90	114.0
147.80	357.0
148.90	124.0
150.00	214.0
152.90	110.0
153.90	122.0
155.00	289.0
156.80	365.0
158.90	195.0
160.80	175.0
171.90	369.0
173.00	1176.0
173.90	138048.0

Instrument :
MSVOA_V
ClientSampleId :
BFB65

175.00	10061.0
175.90	136128.0
176.90	9485.0
177.90	282.0

Instrument :
MSVOA_V
ClientSampleId :
BFB65

m/z	Abundance
36.00	958.0
37.00	4821.0
38.00	4224.0
39.00	1867.0
39.80	254.0
40.90	113.0
41.10	113.0
43.00	137.0
44.00	888.0
45.00	886.0
46.00	129.0
46.90	1574.0
48.00	769.0
49.00	4552.0
50.00	20792.0
51.00	6806.0
51.90	263.0
55.00	358.0
56.00	1744.0
57.00	3042.0
58.00	186.0
60.00	1296.0
61.00	5362.0
62.00	5601.0
63.00	4171.0
63.90	401.0
64.90	143.0
66.80	350.0
68.00	12672.0
69.00	12430.0
70.00	932.0
72.00	646.0
73.00	5542.0
74.00	21664.0
75.00	62760.0
76.00	5655.0
77.00	731.0
77.90	612.0
78.90	3397.0
79.90	1074.0
80.90	3433.0
81.90	778.0
83.00	116.0
86.00	130.0
86.90	5620.0
87.90	5643.0
90.90	389.0
92.00	3846.0
93.00	5412.0
94.00	15490.0
95.00	134208.0
96.00	9216.0
96.90	278.0
103.90	478.0
104.90	242.0
105.80	519.0
106.80	152.0
109.70	114.0
111.00	144.0
112.80	125.0
114.90	112.0
115.80	418.0
116.90	933.0
117.80	589.0
118.80	635.0
123.80	120.0
127.90	608.0
128.90	244.0
130.00	539.0
130.90	213.0
134.70	307.0
136.90	237.0
139.90	127.0
140.90	1385.0
142.00	175.0
142.90	1500.0
143.90	123.0
145.80	316.0
146.90	118.0
147.90	365.0
148.90	137.0
149.90	206.0
152.90	119.0
154.00	103.0
154.80	281.0
156.80	359.0
158.80	199.0
160.80	184.0
171.90	331.0
173.00	1116.0
173.90	127104.0
174.90	9496.0

Instrument :
MSVOA_V
ClientSampleId :
BFB65

175.90	123992.0
176.90	8673.0
177.90	263.0



Instrument :
MSVOA_V
ClientSampleId :
BFB65

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060221\
 Data File : VV021468.D
 Acq On : 02 Jun 2021 09:04
 Operator : SY/MD
 Sample : BFB65
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB65

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR052521WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Jun 03 02:14:36 2021

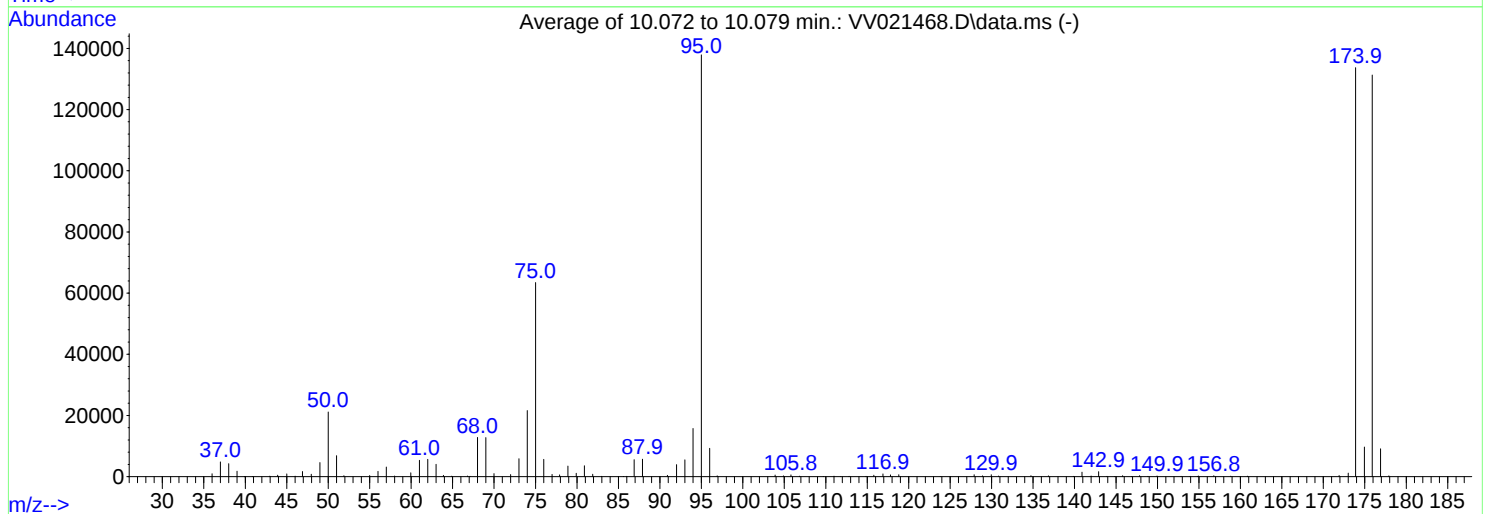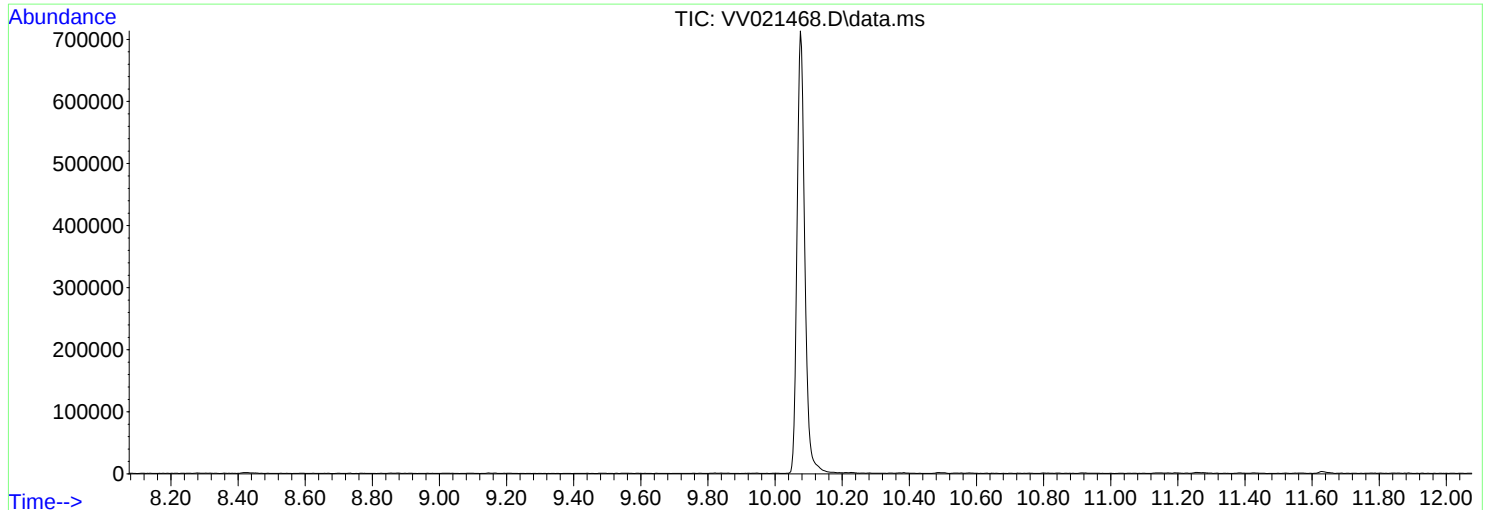

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.3	21152	PASS
75	95	30	80	46.0	63467	PASS
95	95	100	100	100.0	137899	PASS
96	95	5	9	6.7	9257	PASS
173	174	0.00	2	0.9	1152	PASS
174	95	50	120	97.0	133696	PASS
175	174	5	9	7.3	9704	PASS
176	174	95	105	98.2	131272	PASS
177	176	5	10	6.9	9084	PASS