
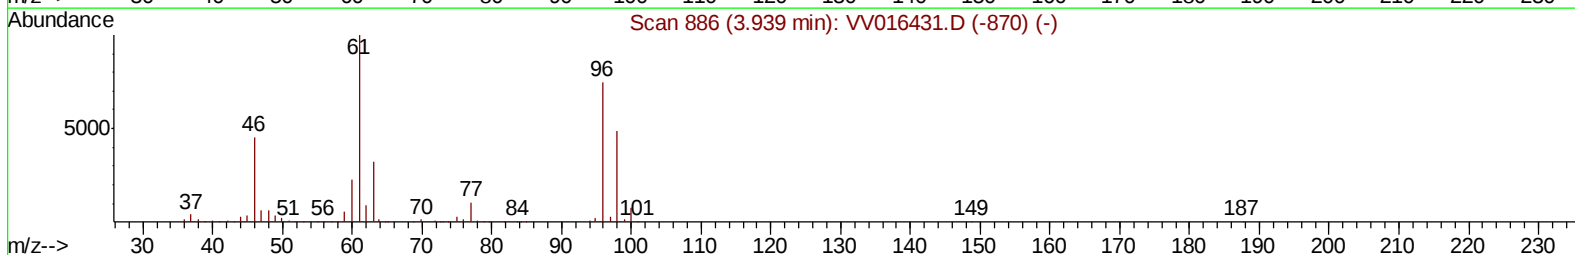
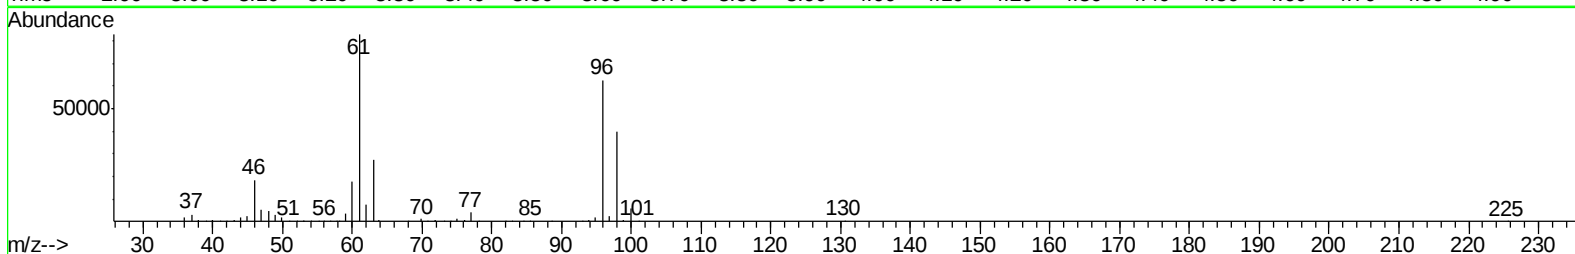


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
Data File : VV016450.D
Acq On : 03 Jun 2020 10:10
Operator : SY/MD
Sample : VSTDCCC050
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 26 Sample Multiplier: 1

Quant Time: Jun 04 01:00:48 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 03 01:20:33 2020
Response via : Initial Calibration

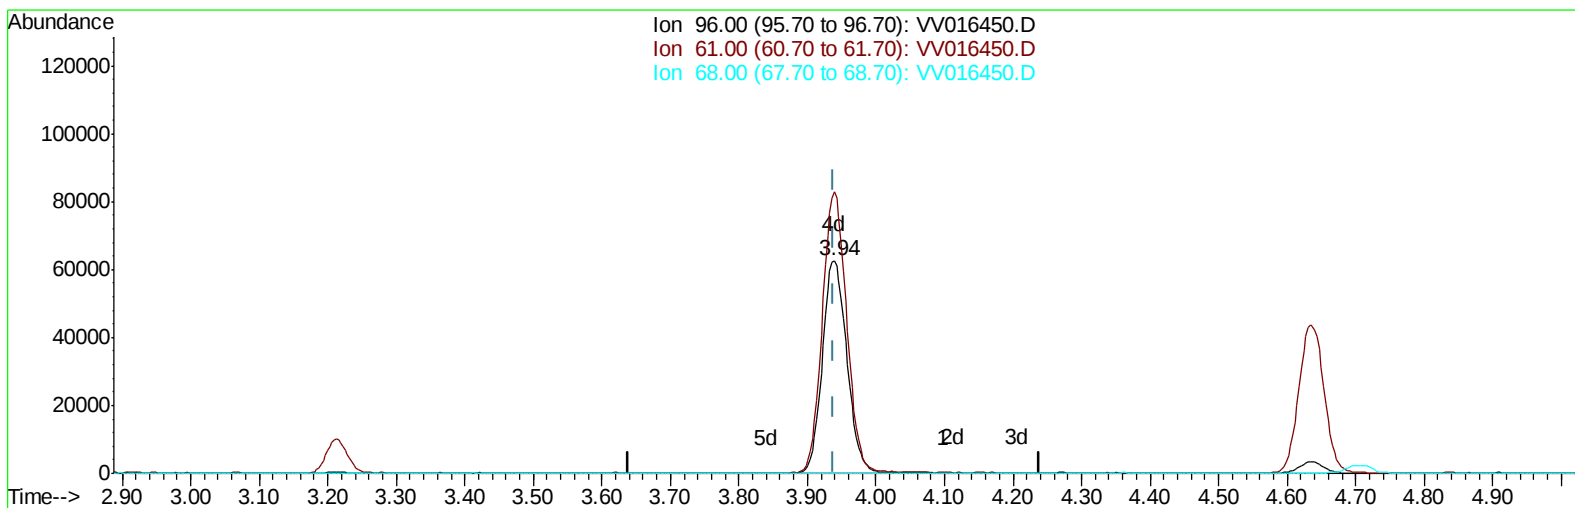

TIC: VV016450.D

(20) cis-1,2-Dichloroethene (T)

3.939min (+0.000) 51.97ug/L m

response 155026

Ion	Exp%	Act%
96.00	100	100
61.00	133.40	132.19
68.00	0.00	0.22#
0.00	0.00	0.00