
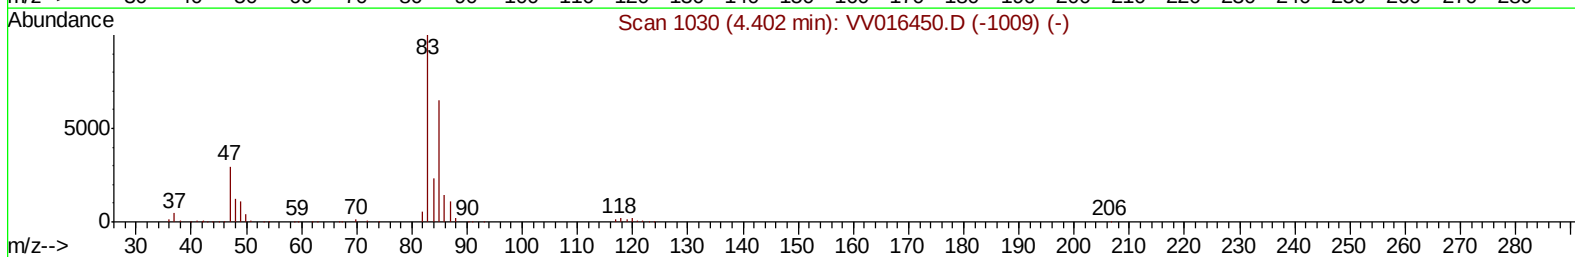
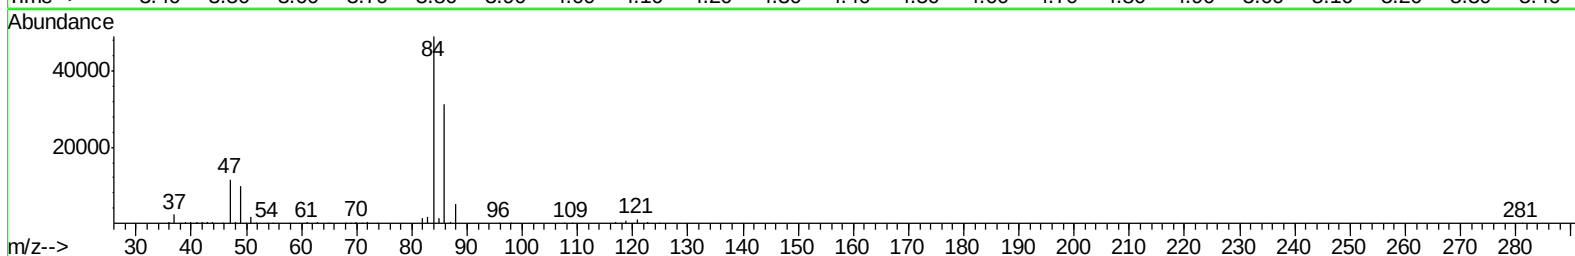


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060320\
Data File : VV016454.D
Acq On : 03 Jun 2020 14:09
Operator : SY/MD
Sample : L2843-09
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 31 Sample Multiplier: 1

Quant Time: Jun 04 02:03:38 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jun 04 01:16:39 2020
Response via : Initial Calibration

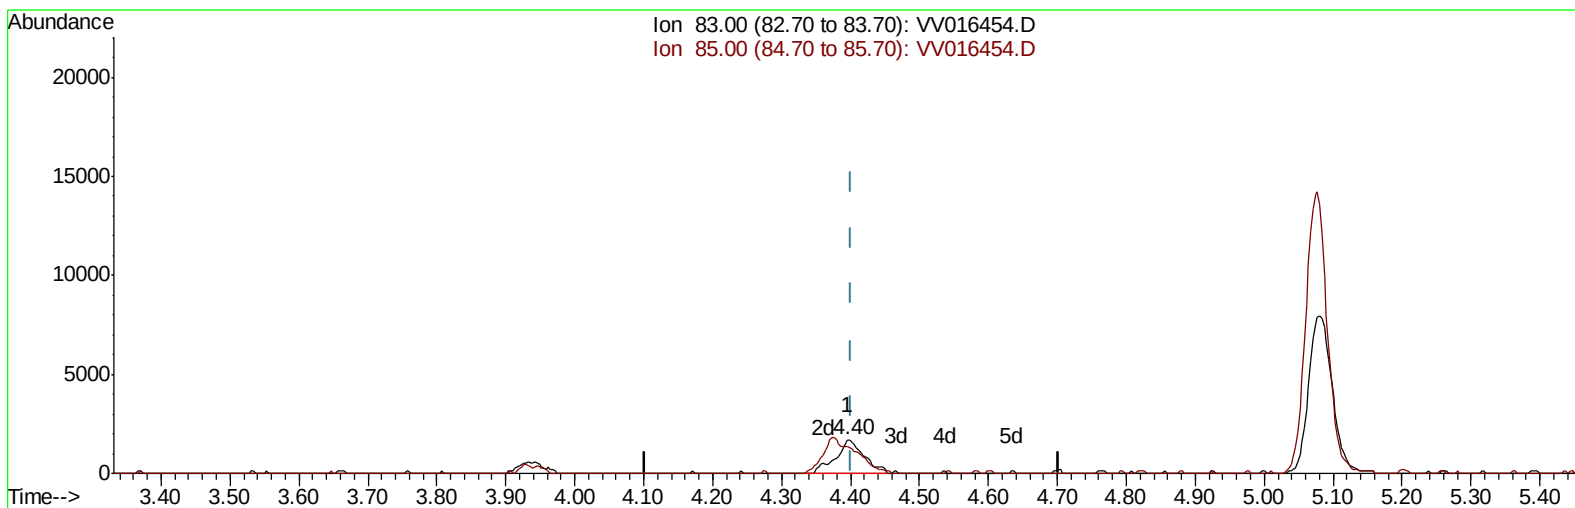

TIC: VV016454.D

(25) Chloroform (T)

4.396min (-0.007) 0.94ug/L m

response 4859

Ion	Exp%	Act%
83.00	100	100
85.00	65.90	80.57
0.00	0.00	0.00
0.00	0.00	0.00