
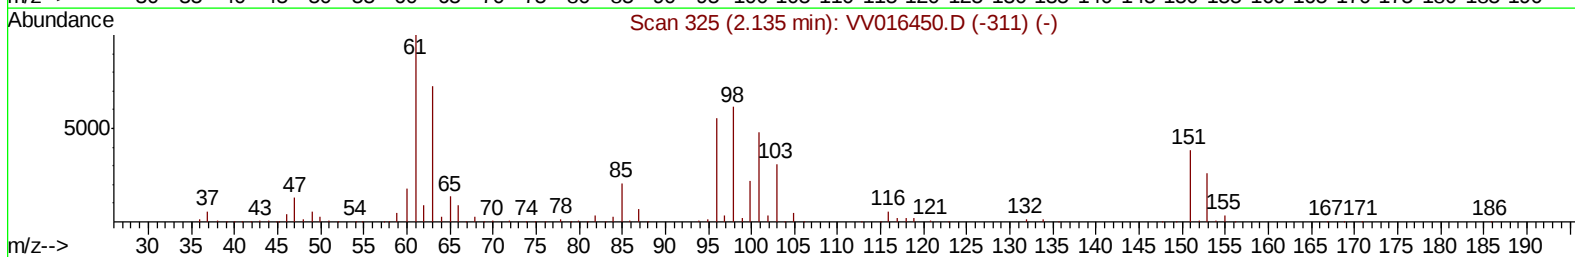
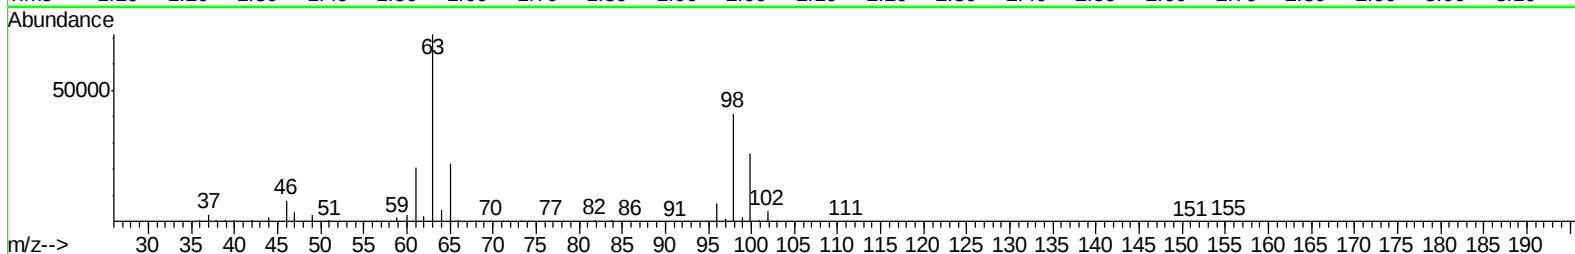


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016456.D
 Acq On : 03 Jun 2020 14:56
 Operator : SY/MD
 Sample : L2843-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Quant Time: Jun 04 01:19:25 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jun 04 01:16:39 2020
 Response via : Initial Calibration

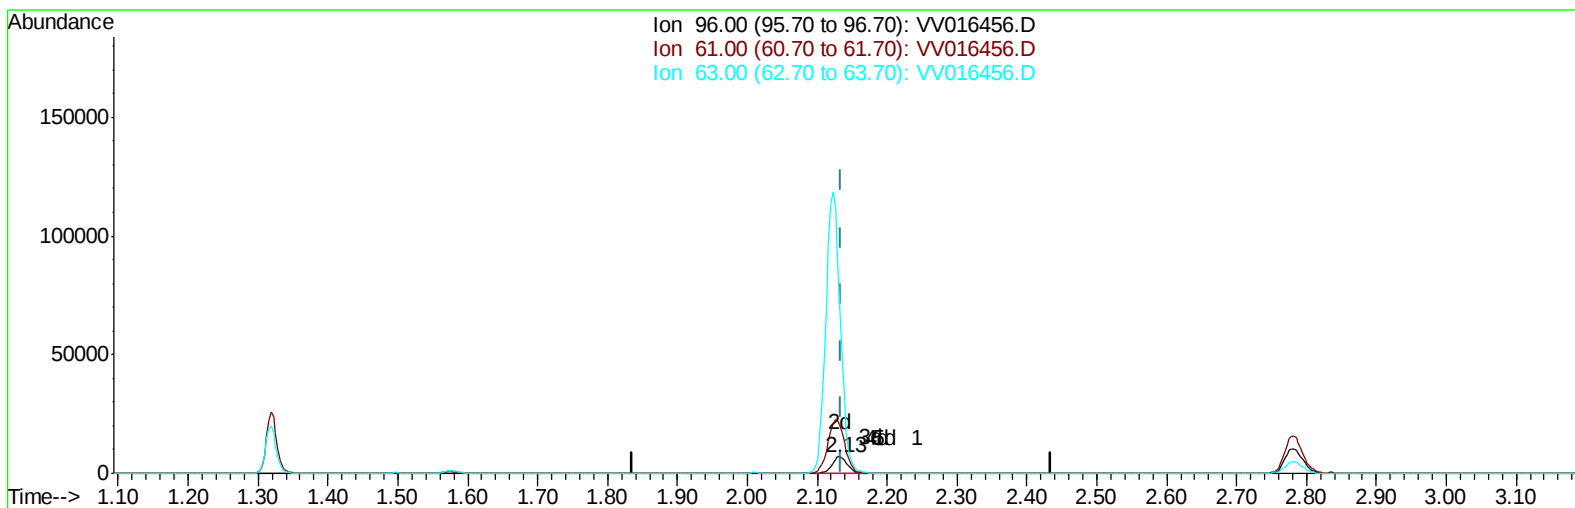

TIC: VV016456.D

(12) 1,1-Dichloroethene (T)

2.132min (-0.003) 5.17ug/L m

response 10837

Ion	Exp%	Act%
96.00	100	100
61.00	179.30	302.46#
63.00	148.50	1044.38#
0.00	0.00	0.00