

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016469.D
 Acq On : 03 Jun 2020 20:08
 Operator : SY/MD
 Sample : L2844-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AF4

Quant Time: Jun 04 04:55:45 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jun 04 01:16:39 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	366117	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	344328	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	160289	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	110894	42.76	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	85.52%
7) Chloroethane-d5	1.57	69	84596	45.19	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	90.38%
11) 1,1-Dichloroethene-d2	2.12	63	156636	34.07	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	68.14%
21) 2-Butanone-d5	3.89	46	174674	105.35	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	105.35%
24) Chloroform-d	4.37	84	231293	47.53	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.06%
26) 1,2-Dichloroethane-d4	5.06	65	159687	49.00	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.00%
32) Benzene-d6	5.07	84	457035	49.55	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.10%
36) 1,2-Dichloropropane-d6	6.09	67	146048	50.82	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	101.64%
41) Toluene-d8	7.34	98	408250	48.74	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	97.48%
43) trans-1,3-Dichloropropene-	7.64	79	65452	46.73	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.46%
47) 2-Hexanone-d5	8.11	63	136042	110.53	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	110.53%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	195198	50.08	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	100.16%
64) 1,2-Dichlorobenzene-d4	11.65	152	164913	54.75	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	109.50%


Target Compounds					Ovalue
13) Acetone	2.17	43	5893	3.803 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060320\
Data File : VV016469.D
Acq On : 03 Jun 2020 20:08
Operator : SY/MD
Sample : L2844-07
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF4

Quant Time: Jun 04 04:55:45 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jun 04 01:16:39 2020
Response via : Initial Calibration

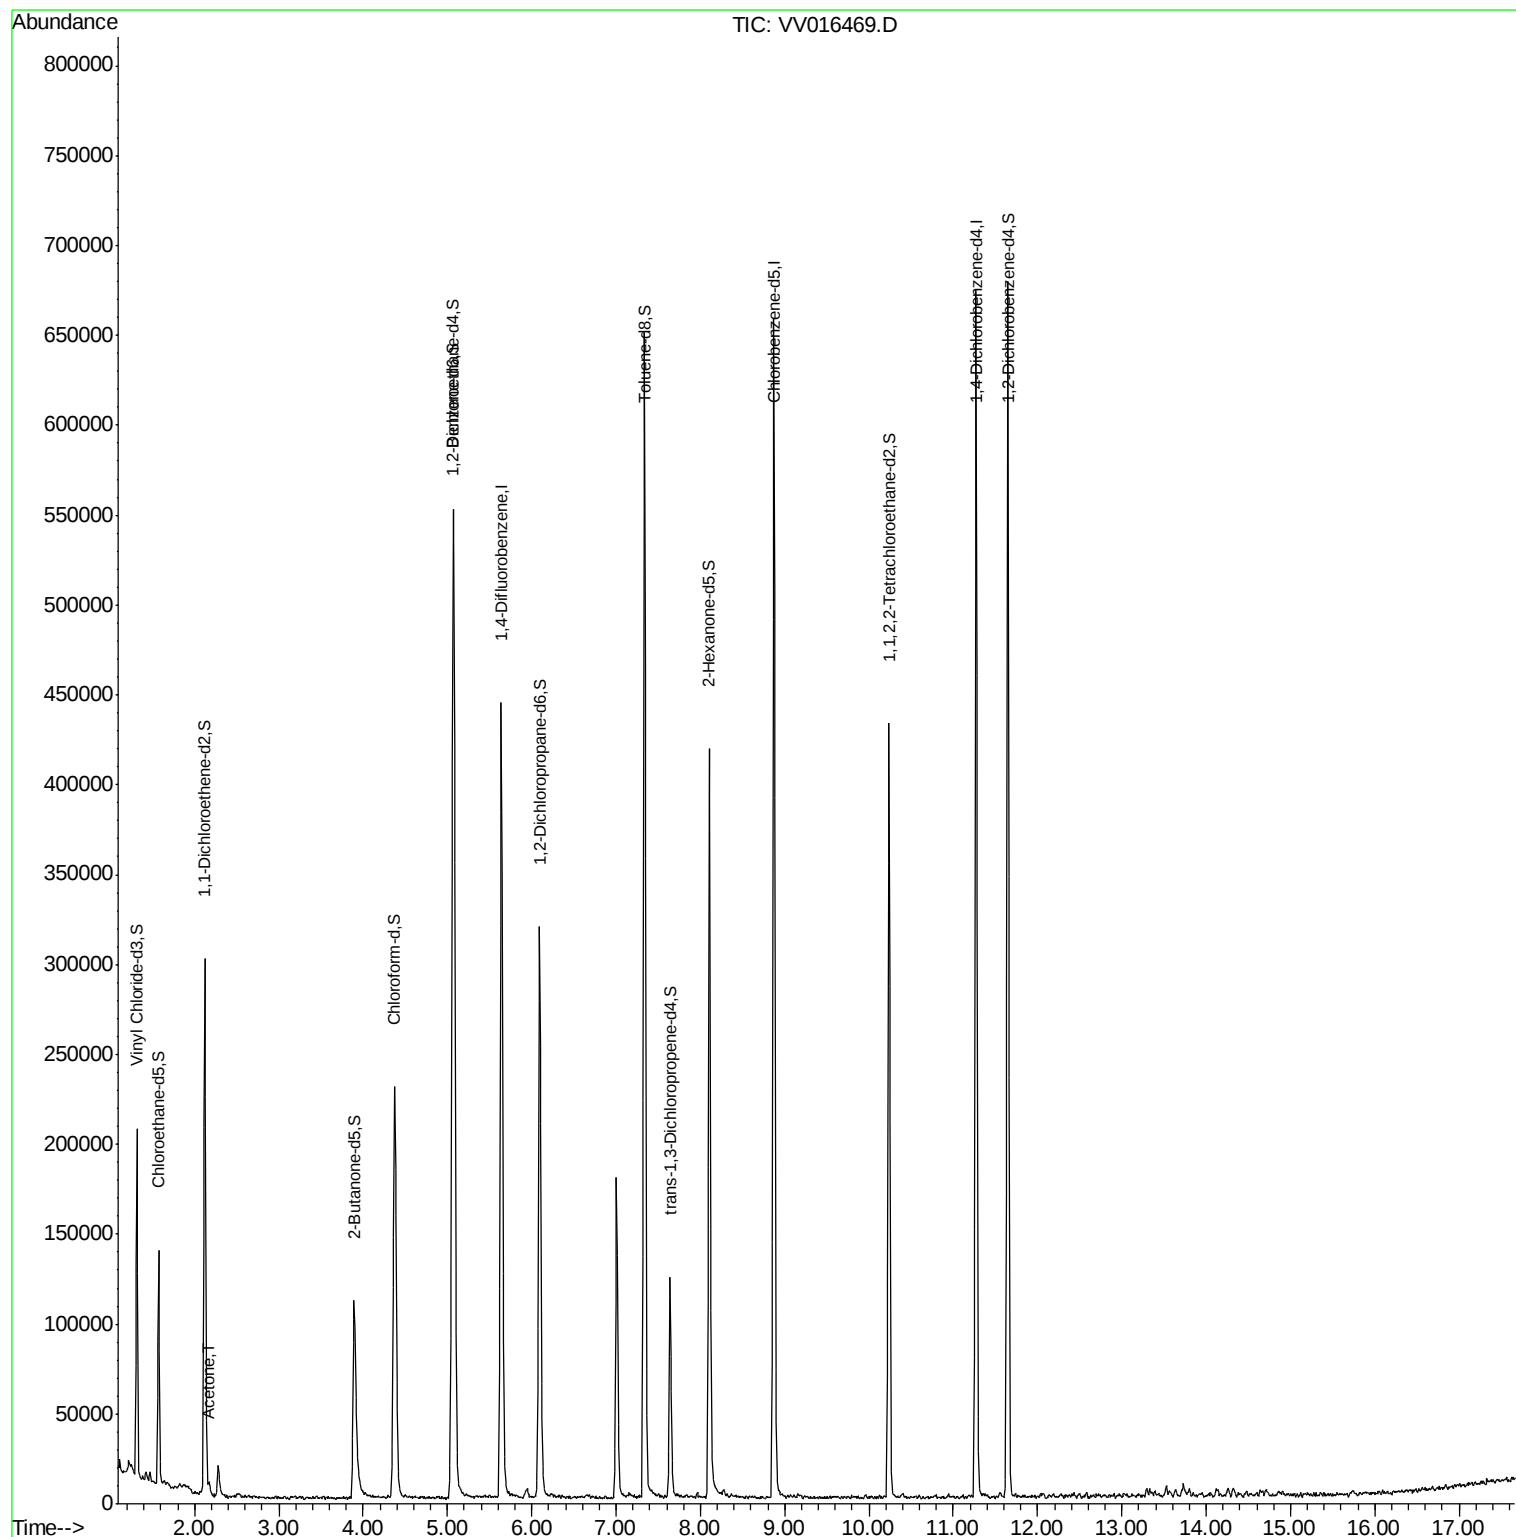

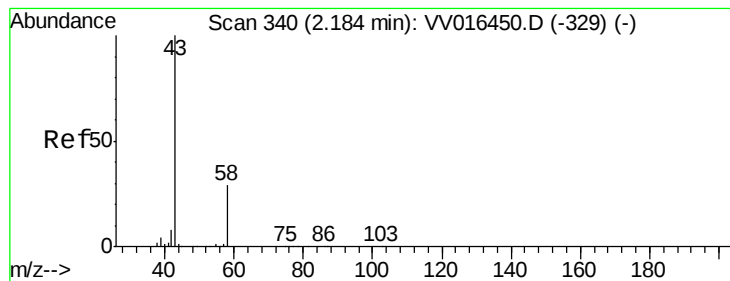

#13
 Acetone
 Concen: 3.803 ug/L
 RT: 2.17 min Scan# 336
 Delta R.T. -0.01 min
 Lab File: VV016469.D
 Acq: 03 Jun 2020 20:08

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AF4

Tot Ion: 43 Resp: 5893
 Ion Ratio Lower Upper
 43 100
 58 25.8 0.0 57.2

