

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016439.D
 Acq On : 02 Jun 2020 20:27
 Operator : SY/MD
 Sample : L2836-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFXC5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	64	71	86	rVB	205983	219362	15.02%	1.918%
2	1.579	146	152	164	rVB	148036	171519	11.75%	1.499%
3	2.126	313	322	349	rVB	325793	499347	34.20%	4.365%
4	2.820	534	538	539	rBV4	997	607	0.04%	0.005%
5	2.852	546	548	550	rVB3	1594	769	0.05%	0.007%
6	2.920	566	569	573	rBV3	1455	1422	0.10%	0.012%
7	3.036	601	605	606	rBV4	1226	780	0.05%	0.007%
8	3.045	606	608	611	rVB3	1345	667	0.05%	0.006%
9	3.064	611	614	615	rBV3	1198	577	0.04%	0.005%
10	3.145	636	639	644	rBV6	1488	1448	0.10%	0.013%
11	3.325	689	695	698	rBV6	959	1035	0.07%	0.009%
12	3.367	706	708	710	rBV3	1039	465	0.03%	0.004%
13	3.415	720	723	725	rBV4	2138	1048	0.07%	0.009%
14	3.470	737	740	743	rBV4	1939	1443	0.10%	0.013%
15	3.527	755	758	761	rBV6	748	590	0.04%	0.005%
16	3.582	771	775	776	rVB4	1159	653	0.04%	0.006%
17	3.637	790	792	793	rBV2	1312	625	0.04%	0.005%
18	3.675	801	804	806	rBV4	1312	767	0.05%	0.007%
19	3.711	813	815	820	rVB5	875	541	0.04%	0.005%
20	3.836	851	854	857	rVB4	1300	875	0.06%	0.008%
21	3.855	857	860	864	rBV4	1278	1061	0.07%	0.009%
22	3.910	866	877	905	rBV3	108804	342101	23.43%	2.991%
23	4.376	1008	1022	1048	rVB	229406	574546	39.35%	5.023%
24	4.566	1077	1081	1082	rBV3	1824	1209	0.08%	0.011%
25	4.798	1150	1153	1158	rVB7	909	954	0.07%	0.008%
26	4.933	1192	1195	1198	rBV3	675	569	0.04%	0.005%
27	5.074	1222	1239	1259	rBV2	569842	1460193	100.00%	12.765%
28	5.447	1348	1355	1360	rBV10	2235	2945	0.20%	0.026%
29	5.576	1392	1395	1396	rBV4	791	494	0.03%	0.004%
30	5.643	1402	1416	1435	rBV	479864	947497	64.89%	8.283%
31	5.910	1495	1499	1501	rBV3	2337	1694	0.12%	0.015%
32	6.096	1543	1557	1578	rBV	327349	664808	45.53%	5.812%
33	6.466	1669	1672	1676	rBV6	1417	1267	0.09%	0.011%
34	6.588	1708	1710	1713	rBV4	1007	573	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016439.D
 Acq On : 02 Jun 2020 20:27
 Operator : SY/MD
 Sample : L2836-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFXC5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.633	1716	1724	1728	rBV9	1885	3079	0.21%	0.027%
36	6.749	1758	1760	1764	rVB3	1457	696	0.05%	0.006%
37	6.778	1767	1769	1770	rBV2	1240	579	0.04%	0.005%
38	6.810	1775	1779	1782	rBV4	1385	1165	0.08%	0.010%
39	6.830	1782	1785	1788	rBV5	1610	1250	0.09%	0.011%
40	6.900	1806	1807	1810	rVB3	1221	561	0.04%	0.005%
41	6.955	1822	1824	1827	rVB4	1125	468	0.03%	0.004%
42	7.006	1827	1840	1860	rBV	181123	327820	22.45%	2.866%
43	7.248	1913	1915	1917	rBV3	1355	598	0.04%	0.005%
44	7.338	1928	1943	1961	rBV	684693	1180326	80.83%	10.319%
45	7.643	2028	2038	2052	rBV	128932	214583	14.70%	1.876%
46	7.775	2076	2079	2082	rBV5	1814	1425	0.10%	0.012%
47	7.958	2130	2136	2140	rBV8	1897	2525	0.17%	0.022%
48	8.109	2172	2183	2204	rBV	393818	693944	47.52%	6.067%
49	8.434	2280	2284	2285	rBV3	1529	1141	0.08%	0.010%
50	8.482	2295	2299	2301	rBV3	1475	1098	0.08%	0.010%
51	8.508	2305	2307	2309	rBV2	1537	724	0.05%	0.006%
52	8.675	2357	2359	2361	rBV3	1415	511	0.03%	0.004%
53	8.730	2373	2376	2378	rBV4	1425	897	0.06%	0.008%
54	8.765	2382	2387	2391	rBV7	1255	1621	0.11%	0.014%
55	8.875	2408	2421	2441	rBV	727567	1163946	79.71%	10.176%
56	9.067	2479	2481	2482	rBV2	1127	488	0.03%	0.004%
57	9.453	2599	2601	2604	rBV4	1571	1110	0.08%	0.010%
58	9.473	2605	2607	2610	rBV4	1060	807	0.06%	0.007%
59	9.556	2629	2633	2634	rBV3	1417	986	0.07%	0.009%
60	9.685	2669	2673	2676	rBV5	1226	1062	0.07%	0.009%
61	9.768	2697	2699	2701	rBV3	1199	726	0.05%	0.006%
62	9.807	2709	2711	2714	rVB2	1326	705	0.05%	0.006%
63	9.836	2716	2720	2721	rBV4	1019	693	0.05%	0.006%
64	9.881	2733	2734	2738	rVB4	1393	631	0.04%	0.006%
65	10.061	2787	2790	2791	rBV3	1178	733	0.05%	0.006%
66	10.090	2797	2799	2803	rVB5	1437	767	0.05%	0.007%
67	10.112	2804	2806	2810	rVB4	1083	536	0.04%	0.005%
68	10.161	2819	2821	2823	rBV3	1288	593	0.04%	0.005%
69	10.238	2833	2845	2860	rBV	438439	679000	46.50%	5.936%
70	10.373	2886	2887	2889	rVB2	1676	528	0.04%	0.005%
71	10.415	2899	2900	2905	rVB4	1433	678	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016439.D
 Acq On : 02 Jun 2020 20:27
 Operator : SY/MD
 Sample : L2836-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFXC5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	10.456	2911	2913	2915	rBV2	1287	764	0.05%	0.007%
73	10.508	2925	2929	2932	rBV4	1361	923	0.06%	0.008%
74	10.559	2939	2945	2946	rBV4	1524	1333	0.09%	0.012%
75	10.698	2983	2988	2991	rBV5	1544	1519	0.10%	0.013%
76	10.772	3008	3011	3014	rVB4	1175	682	0.05%	0.006%
77	10.797	3014	3019	3020	rBV4	1376	957	0.07%	0.008%
78	11.032	3087	3092	3094	rBV6	1624	1333	0.09%	0.012%
79	11.090	3104	3110	3112	rBV5	1466	865	0.06%	0.008%
80	11.103	3112	3114	3116	rBV3	1011	623	0.04%	0.005%
81	11.173	3127	3136	3137	rBV7	2374	2562	0.18%	0.022%
82	11.270	3154	3166	3181	rBV	733524	1125553	77.08%	9.840%
83	11.579	3260	3262	3265	rBV3	1101	714	0.05%	0.006%
84	11.646	3270	3283	3300	rBV	698407	1074298	73.57%	9.392%
85	11.907	3363	3364	3368	rBV3	1518	885	0.06%	0.008%
86	12.096	3421	3423	3425	rBV3	1231	632	0.04%	0.006%
87	12.218	3459	3461	3462	rBV2	1147	486	0.03%	0.004%
88	12.318	3490	3492	3496	rVB5	1242	757	0.05%	0.007%
89	12.334	3496	3497	3501	rBV5	948	658	0.05%	0.006%
90	12.530	3554	3558	3560	rBV3	1366	1090	0.07%	0.010%
91	12.653	3590	3596	3597	rBV6	1704	1502	0.10%	0.013%
92	12.929	3679	3682	3685	rBV4	2090	1406	0.10%	0.012%
93	13.286	3788	3793	3798	rBV7	3627	4792	0.33%	0.042%
94	13.443	3838	3842	3846	rBV4	1929	1980	0.14%	0.017%
95	13.527	3859	3868	3881	rBV	8257	14411	0.99%	0.126%
96	13.951	3999	4000	4005	rBV5	1208	647	0.04%	0.006%
97	14.074	4036	4038	4040	rBV3	1310	752	0.05%	0.007%
98	14.112	4048	4050	4052	rBV3	1382	843	0.06%	0.007%
99	14.595	4195	4200	4203	rBV7	1699	1737	0.12%	0.015%
100	14.646	4214	4216	4218	rBV3	1130	505	0.03%	0.004%


Sum of corrected areas: 11438660

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060320\
Data File : VV016439.D
Acq On : 02 Jun 2020 20:27
Operator : SY/MD
Sample : L2836-01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXC5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

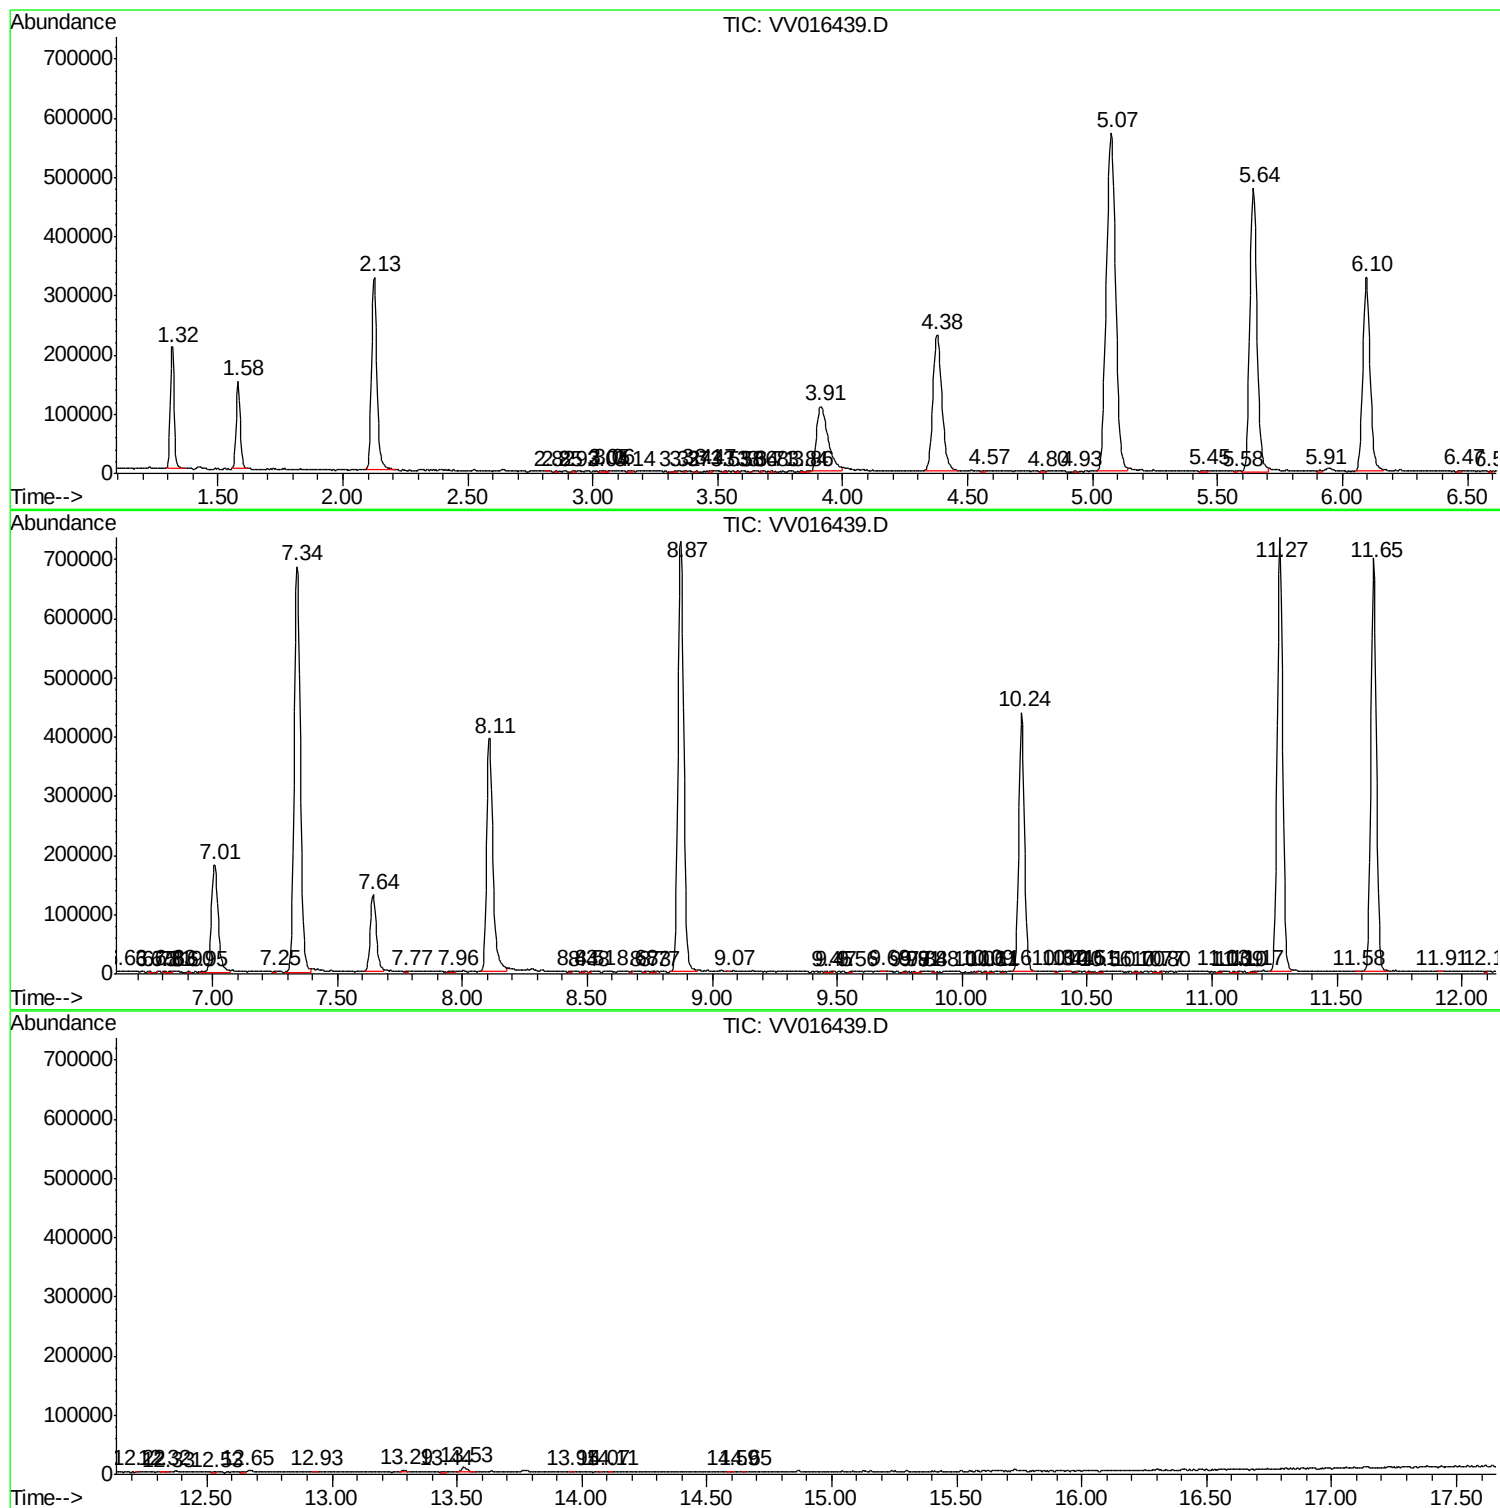

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV060320\
Data File : VV016439.D
Acq On : 02 Jun 2020 20:27
Operator : SY/MD
Sample : L2836-01
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BFXC5

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060320\
Data File : VV016439.D
Acq On : 02 Jun 2020 20:27
Operator : SY/MD
Sample : L2836-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXC5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc