

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016441.D
 Acq On : 02 Jun 2020 21:12
 Operator : SY/MD
 Sample : L2836-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFXC7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	83	rVB	214294	225235	14.91%	1.950%
2	1.579	145	152	162	rBV	148996	172151	11.40%	1.491%
3	2.126	312	322	340	rBV	331987	501281	33.19%	4.340%
4	2.312	375	380	385	rBV9	2690	3342	0.22%	0.029%
5	2.714	501	505	506	rBV4	1532	969	0.06%	0.008%
6	2.740	506	513	514	rBV4	1247	1164	0.08%	0.010%
7	2.923	568	570	573	rBV4	1953	898	0.06%	0.008%
8	3.048	605	609	612	rBV5	1153	1039	0.07%	0.009%
9	3.100	621	625	627	rBV5	2370	1507	0.10%	0.013%
10	3.196	652	655	657	rBV3	1495	875	0.06%	0.008%
11	3.251	670	672	675	rBV3	1418	743	0.05%	0.006%
12	3.309	687	690	691	rBV3	1107	636	0.04%	0.006%
13	3.344	698	701	704	rBV4	1681	1118	0.07%	0.010%
14	3.463	734	738	740	rBV4	985	714	0.05%	0.006%
15	3.518	752	755	757	rBV4	1230	865	0.06%	0.007%
16	3.598	776	780	782	rVV4	1062	922	0.06%	0.008%
17	3.621	783	787	793	rVB7	1521	1337	0.09%	0.012%
18	3.662	796	800	802	rVB4	1315	939	0.06%	0.008%
19	3.711	811	815	817	rVB4	1060	611	0.04%	0.005%
20	3.727	817	820	821	rBV3	914	590	0.04%	0.005%
21	3.788	835	839	841	rVB4	2142	1159	0.08%	0.010%
22	3.836	851	854	858	rVB5	1619	900	0.06%	0.008%
23	3.859	858	861	864	rBV4	1317	928	0.06%	0.008%
24	3.910	866	877	903	rBV2	116013	361277	23.92%	3.128%
25	4.379	1008	1023	1047	rBV	234952	586371	38.82%	5.077%
26	4.531	1068	1070	1073	rBV4	1613	1141	0.08%	0.010%
27	4.640	1101	1104	1107	rBV5	1439	1004	0.07%	0.009%
28	4.904	1182	1186	1187	rBV3	1133	827	0.05%	0.007%
29	5.074	1221	1239	1266	rVV2	584416	1510481	100.00%	13.079%
30	5.447	1353	1355	1363	rVB7	2669	2336	0.15%	0.020%
31	5.482	1363	1366	1372	rBV5	1668	1678	0.11%	0.015%
32	5.643	1403	1416	1437	rBV	467555	925122	61.25%	8.010%
33	5.817	1467	1470	1471	rBV2	1050	637	0.04%	0.006%
34	5.871	1485	1487	1490	rVB3	1718	744	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016441.D
 Acq On : 02 Jun 2020 21:12
 Operator : SY/MD
 Sample : L2836-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFXC7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	5.894	1490	1494	1496	rBV3	1483	1221	0.08%	0.011%
36	5.945	1501	1510	1511	rBV7	8809	11555	0.76%	0.100%
37	6.016	1529	1532	1534	rBV4	1428	877	0.06%	0.008%
38	6.093	1542	1556	1582	rBV	331629	677799	44.87%	5.869%
39	6.367	1639	1641	1645	rVB4	1092	726	0.05%	0.006%
40	6.460	1666	1670	1671	rBV4	1636	1007	0.07%	0.009%
41	6.524	1687	1690	1692	rBV4	1019	638	0.04%	0.006%
42	6.604	1710	1715	1718	rBV6	846	745	0.05%	0.006%
43	6.797	1771	1775	1778	rVB4	1787	1155	0.08%	0.010%
44	6.945	1818	1821	1824	rVB4	1435	1059	0.07%	0.009%
45	7.010	1829	1841	1859	rVV	182961	330684	21.89%	2.863%
46	7.183	1892	1895	1899	rBV5	1001	765	0.05%	0.007%
47	7.248	1912	1915	1917	rBV4	1086	940	0.06%	0.008%
48	7.280	1921	1925	1927	rBV5	1217	855	0.06%	0.007%
49	7.338	1931	1943	1962	rBV	696334	1198912	79.37%	10.381%
50	7.643	2026	2038	2059	rBV	131600	231215	15.31%	2.002%
51	7.868	2100	2108	2114	rBV9	2279	3058	0.20%	0.026%
52	7.900	2114	2118	2120	rVB5	2060	1208	0.08%	0.010%
53	7.923	2123	2125	2128	rVV3	1235	605	0.04%	0.005%
54	8.039	2159	2161	2164	rBV3	1236	768	0.05%	0.007%
55	8.106	2172	2182	2201	rBV	400616	700188	46.36%	6.063%
56	8.710	2366	2370	2372	rBV5	2149	1339	0.09%	0.012%
57	8.874	2409	2421	2436	rBV	706726	1142764	75.66%	9.895%
58	9.116	2494	2496	2499	rBV4	1480	827	0.05%	0.007%
59	9.154	2504	2508	2512	rBV6	2198	2690	0.18%	0.023%
60	9.183	2515	2517	2520	rVB3	1161	625	0.04%	0.005%
61	9.238	2531	2534	2538	rBV6	1512	1364	0.09%	0.012%
62	9.273	2541	2545	2547	rBV4	1363	912	0.06%	0.008%
63	9.299	2551	2553	2557	rVB4	952	608	0.04%	0.005%
64	9.318	2557	2559	2562	rBV4	943	780	0.05%	0.007%
65	9.566	2630	2636	2642	rBV4	2208	3117	0.21%	0.027%
66	9.865	2727	2729	2734	rVB6	1148	728	0.05%	0.006%
67	9.952	2752	2756	2758	rBV3	2033	1628	0.11%	0.014%
68	10.042	2780	2784	2788	rBV5	1799	1784	0.12%	0.015%
69	10.238	2833	2845	2865	rBV	441656	687565	45.52%	5.953%
70	10.341	2875	2877	2878	rBV2	1312	612	0.04%	0.005%
71	10.399	2893	2895	2897	rBV3	1477	767	0.05%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016441.D
 Acq On : 02 Jun 2020 21:12
 Operator : SY/MD
 Sample : L2836-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFXC7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	10.456	2908	2913	2914	rBV5	1172	918	0.06%	0.008%
73	10.511	2928	2930	2936	rVV6	959	919	0.06%	0.008%
74	10.810	3019	3023	3027	rBV6	1608	1622	0.11%	0.014%
75	10.907	3050	3053	3056	rVB5	1489	782	0.05%	0.007%
76	10.935	3056	3062	3064	rBV6	1840	1714	0.11%	0.015%
77	10.977	3073	3075	3081	rBV7	1432	845	0.06%	0.007%
78	11.058	3097	3100	3105	rVB5	1394	1120	0.07%	0.010%
79	11.083	3105	3108	3111	rBV6	1542	1030	0.07%	0.009%
80	11.173	3133	3136	3137	rBV2	1686	1032	0.07%	0.009%
81	11.270	3154	3166	3187	rBV	717195	1093534	72.40%	9.469%
82	11.495	3233	3236	3239	rBV4	1143	998	0.07%	0.009%
83	11.646	3272	3283	3301	rVB	702498	1089586	72.14%	9.434%
84	12.058	3408	3411	3414	rBV4	1486	1019	0.07%	0.009%
85	12.209	3452	3458	3460	rBV6	1206	1302	0.09%	0.011%
86	12.344	3497	3500	3503	rBV4	1448	1311	0.09%	0.011%
87	12.945	3684	3687	3689	rBV3	1349	682	0.05%	0.006%
88	13.112	3737	3739	3743	rBV5	972	718	0.05%	0.006%
89	13.151	3749	3751	3754	rVB4	1806	853	0.06%	0.007%
90	13.167	3754	3756	3759	rBV5	1085	934	0.06%	0.008%
91	13.386	3822	3824	3828	rVB4	1460	811	0.05%	0.007%
92	13.527	3858	3868	3878	rBV2	6866	12318	0.82%	0.107%
93	13.595	3887	3889	3892	rBV3	1861	1072	0.07%	0.009%
94	13.878	3974	3977	3979	rBV3	1610	1083	0.07%	0.009%
95	14.035	4022	4026	4029	rBV5	1753	1220	0.08%	0.011%
96	14.636	4211	4213	4217	rVB5	1443	725	0.05%	0.006%
97	14.752	4247	4249	4253	rBV5	1317	884	0.06%	0.008%
98	15.176	4377	4381	4383	rBV4	1625	1231	0.08%	0.011%
99	15.337	4427	4431	4435	rBV4	2115	2215	0.15%	0.019%
100	15.459	4467	4469	4471	rBV3	1707	848	0.06%	0.007%


Sum of corrected areas: 11548957

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060320\
Data File : VV016441.D
Acq On : 02 Jun 2020 21:12
Operator : SY/MD
Sample : L2836-03
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXC7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

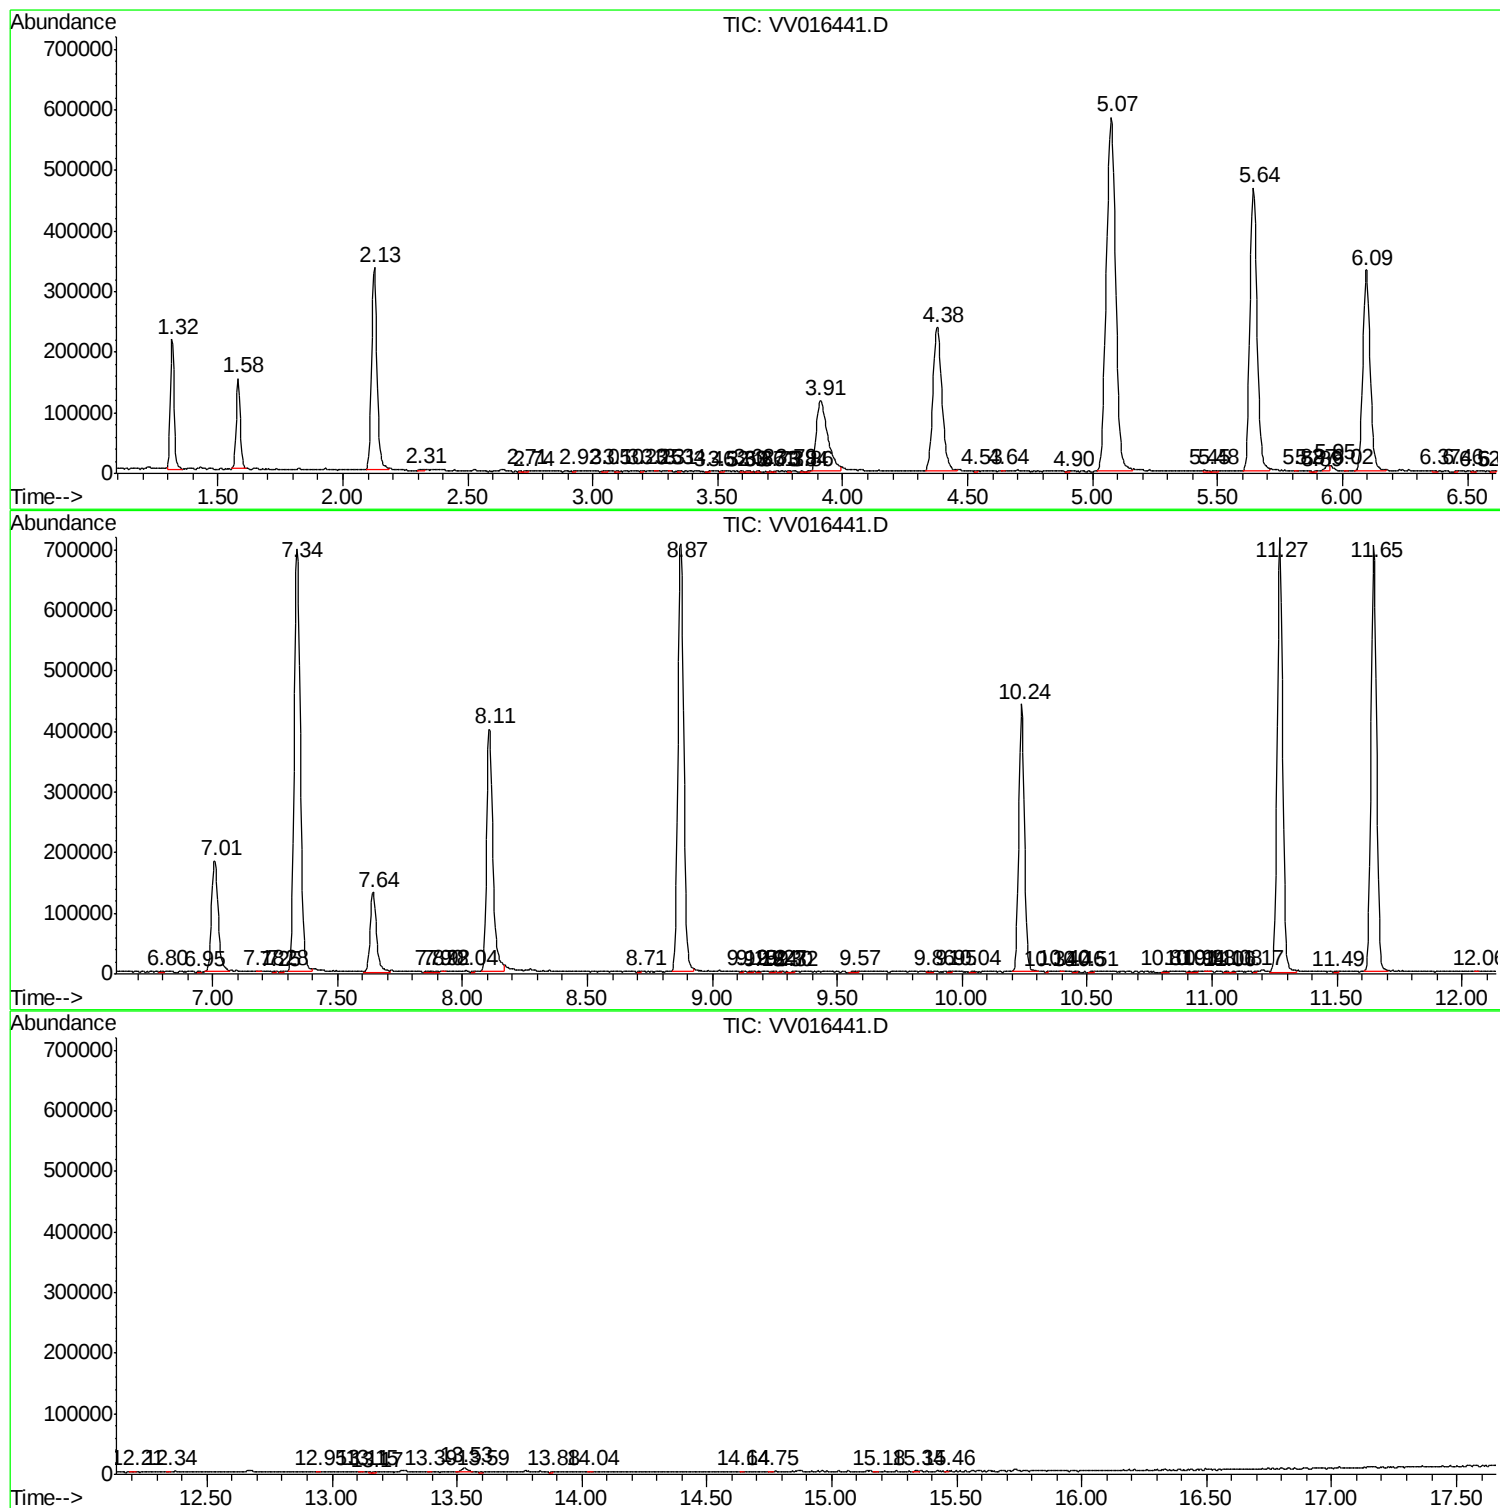

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060320\
Data File : VV016441.D
Acq On : 02 Jun 2020 21:12
Operator : SY/MD
Sample : L2836-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXC7

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060320\
Data File : VV016441.D
Acq On : 02 Jun 2020 21:12
Operator : SY/MD
Sample : L2836-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFXC7

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc