

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016445.D
 Acq On : 02 Jun 2020 22:44
 Operator : SY/MD
 Sample : L2843-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	64	71	84	rVB2	284238	306462	2.23%	0.880%
2	1.579	145	152	167	rVB	144443	178038	1.30%	0.511%
3	2.126	312	322	343	rBV2	345369	527196	3.84%	1.513%
4	2.299	372	376	378	rBV3	1969	1538	0.01%	0.004%
5	2.733	507	511	512	rBV4	1261	897	0.01%	0.003%
6	2.781	518	526	542	rVB2	32700	58447	0.43%	0.168%
7	2.900	560	563	567	rVB5	1212	784	0.01%	0.002%
8	2.920	567	569	572	rBV4	957	660	0.00%	0.002%
9	2.965	580	583	586	rBV3	2081	1657	0.01%	0.005%
10	3.007	591	596	598	rVB5	1779	1473	0.01%	0.004%
11	3.048	606	609	610	rBV3	1317	778	0.01%	0.002%
12	3.077	616	618	622	rVB4	2369	1150	0.01%	0.003%
13	3.154	639	642	643	rBV4	1647	822	0.01%	0.002%
14	3.209	657	659	660	rBV2	1310	563	0.00%	0.002%
15	3.296	684	686	690	rBV5	1762	1157	0.01%	0.003%
16	3.399	716	718	721	rVB5	1110	482	0.00%	0.001%
17	3.415	721	723	726	rBV4	923	658	0.00%	0.002%
18	3.515	750	754	758	rVB5	1184	976	0.01%	0.003%
19	3.534	758	760	761	rBV2	948	507	0.00%	0.001%
20	3.540	761	762	766	rVV2	1146	579	0.00%	0.002%
21	3.595	775	779	783	rBV7	1141	924	0.01%	0.003%
22	3.701	805	812	814	rBV6	1692	1806	0.01%	0.005%
23	3.939	865	886	927	rVV	4001302	9846350	71.67%	28.266%
24	4.380	1007	1023	1051	rBV	229754	605896	4.41%	1.739%
25	4.553	1075	1077	1082	rBV6	1281	829	0.01%	0.002%
26	4.752	1137	1139	1142	rBV4	1295	984	0.01%	0.003%
27	4.978	1206	1209	1210	rBV3	1101	479	0.00%	0.001%
28	5.074	1221	1239	1269	rBV2	579263	1501724	10.93%	4.311%
29	5.283	1300	1304	1308	rBV6	2401	2652	0.02%	0.008%
30	5.495	1365	1370	1371	rBV4	1180	863	0.01%	0.002%
31	5.582	1388	1397	1401	rBV4	2654	4588	0.03%	0.013%
32	5.643	1403	1416	1440	rVV	458399	912688	6.64%	2.620%
33	5.939	1490	1508	1540	rBV	7149079	13738772	100.00%	39.441%
34	6.096	1546	1557	1575	rVB	331841	656590	4.78%	1.885%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016445.D
 Acq On : 02 Jun 2020 22:44
 Operator : SY/MD
 Sample : L2843-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.476	1671	1675	1681	rBV8	1217	1455	0.01%	0.004%
36	6.502	1681	1683	1684	rBV2	1488	769	0.01%	0.002%
37	6.601	1712	1714	1718	rBV5	963	674	0.00%	0.002%
38	6.785	1766	1771	1775	rBV8	1829	1934	0.01%	0.006%
39	7.010	1829	1841	1856	rBV	182876	326241	2.37%	0.937%
40	7.338	1931	1943	1960	rBV	696261	1189071	8.65%	3.414%
41	7.576	2014	2017	2021	rBV4	1653	1548	0.01%	0.004%
42	7.640	2027	2037	2055	rVV	134830	235802	1.72%	0.677%
43	7.907	2118	2120	2123	rBV4	1240	647	0.00%	0.002%
44	7.987	2141	2145	2146	rBV4	2505	1785	0.01%	0.005%
45	8.109	2172	2183	2209	rBV	397824	692995	5.04%	1.989%
46	8.392	2269	2271	2272	rBV3	957	483	0.00%	0.001%
47	8.582	2325	2330	2332	rBV5	1721	1412	0.01%	0.004%
48	8.698	2364	2366	2368	rVB3	1381	526	0.00%	0.002%
49	8.714	2368	2371	2373	rBV4	924	661	0.00%	0.002%
50	8.723	2373	2374	2377	rVB4	1602	595	0.00%	0.002%
51	8.743	2377	2380	2382	rBV3	1069	781	0.01%	0.002%
52	8.874	2409	2421	2438	rBV	689356	1127287	8.21%	3.236%
53	9.032	2467	2470	2471	rBV3	1780	1050	0.01%	0.003%
54	9.119	2496	2497	2501	rBV4	1091	796	0.01%	0.002%
55	9.350	2564	2569	2576	rBV9	1681	2134	0.02%	0.006%
56	9.495	2611	2614	2615	rBV4	1094	596	0.00%	0.002%
57	9.569	2634	2637	2639	rBV3	2230	1178	0.01%	0.003%
58	9.627	2652	2655	2658	rBV5	1047	543	0.00%	0.002%
59	9.643	2658	2660	2662	rBV2	1397	722	0.01%	0.002%
60	9.698	2674	2677	2680	rVB4	1338	677	0.00%	0.002%
61	9.717	2680	2683	2690	rVB7	1081	848	0.01%	0.002%
62	9.752	2690	2694	2698	rBV6	1610	1356	0.01%	0.004%
63	9.775	2698	2701	2704	rVB5	1387	1008	0.01%	0.003%
64	9.797	2704	2708	2710	rBV5	1402	1154	0.01%	0.003%
65	9.878	2730	2733	2735	rBV3	945	475	0.00%	0.001%
66	9.923	2745	2747	2751	rBV5	1015	602	0.00%	0.002%
67	9.948	2753	2755	2756	rBV2	1253	626	0.00%	0.002%
68	9.981	2763	2765	2767	rBV3	1295	667	0.00%	0.002%
69	10.032	2779	2781	2784	rBV3	1372	938	0.01%	0.003%
70	10.106	2802	2804	2810	rVB8	2300	1747	0.01%	0.005%
71	10.145	2813	2816	2817	rBV3	925	519	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016445.D
 Acq On : 02 Jun 2020 22:44
 Operator : SY/MD
 Sample : L2843-03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	10.164	2820	2822	2825	rBV3	1097	769	0.01%	0.002%
73	10.238	2834	2845	2861	rBV	435486	678831	4.94%	1.949%
74	10.511	2926	2930	2933	rBV4	935	724	0.01%	0.002%
75	10.566	2940	2947	2949	rBV6	2110	2022	0.01%	0.006%
76	10.598	2954	2957	2958	rBV2	1321	750	0.01%	0.002%
77	10.659	2972	2976	2982	rBV5	1867	1787	0.01%	0.005%
78	10.691	2982	2986	2988	rBV5	1194	1004	0.01%	0.003%
79	10.739	2998	3001	3002	rBV3	948	640	0.00%	0.002%
80	10.878	3041	3044	3046	rBV4	1335	834	0.01%	0.002%
81	10.910	3050	3054	3055	rBV4	1312	833	0.01%	0.002%
82	10.990	3077	3079	3080	rBV2	1523	609	0.00%	0.002%
83	11.206	3141	3146	3149	rBV6	3243	3023	0.02%	0.009%
84	11.270	3155	3166	3181	rBV	716495	1082918	7.88%	3.109%
85	11.511	3236	3241	3245	rBV8	1946	2034	0.01%	0.006%
86	11.646	3271	3283	3302	rBV	700007	1080491	7.86%	3.102%
87	11.865	3348	3351	3353	rBV3	1841	1289	0.01%	0.004%
88	11.955	3374	3379	3380	rBV4	1371	1306	0.01%	0.004%
89	12.000	3388	3393	3396	rVB5	1671	1536	0.01%	0.004%
90	12.019	3396	3399	3400	rBV3	1317	736	0.01%	0.002%
91	12.032	3400	3403	3406	rVV5	1343	1038	0.01%	0.003%
92	12.225	3461	3463	3466	rBV4	1256	942	0.01%	0.003%
93	13.064	3721	3724	3727	rBV3	1733	1162	0.01%	0.003%
94	13.096	3732	3734	3736	rBV3	1443	817	0.01%	0.002%
95	14.000	4013	4015	4021	rVB7	1006	725	0.01%	0.002%
96	14.061	4031	4034	4035	rBV3	1119	629	0.00%	0.002%
97	14.228	4084	4086	4089	rBV3	1477	970	0.01%	0.003%
98	14.440	4151	4152	4155	rBV3	1015	685	0.00%	0.002%
99	14.524	4175	4178	4183	rBV6	1226	1073	0.01%	0.003%
100	14.926	4297	4303	4305	rBV6	1949	1621	0.01%	0.005%


Sum of corrected areas: 34834069

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060320\
Data File : VV016445.D
Acq On : 02 Jun 2020 22:44
Operator : SY/MD
Sample : L2843-03
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

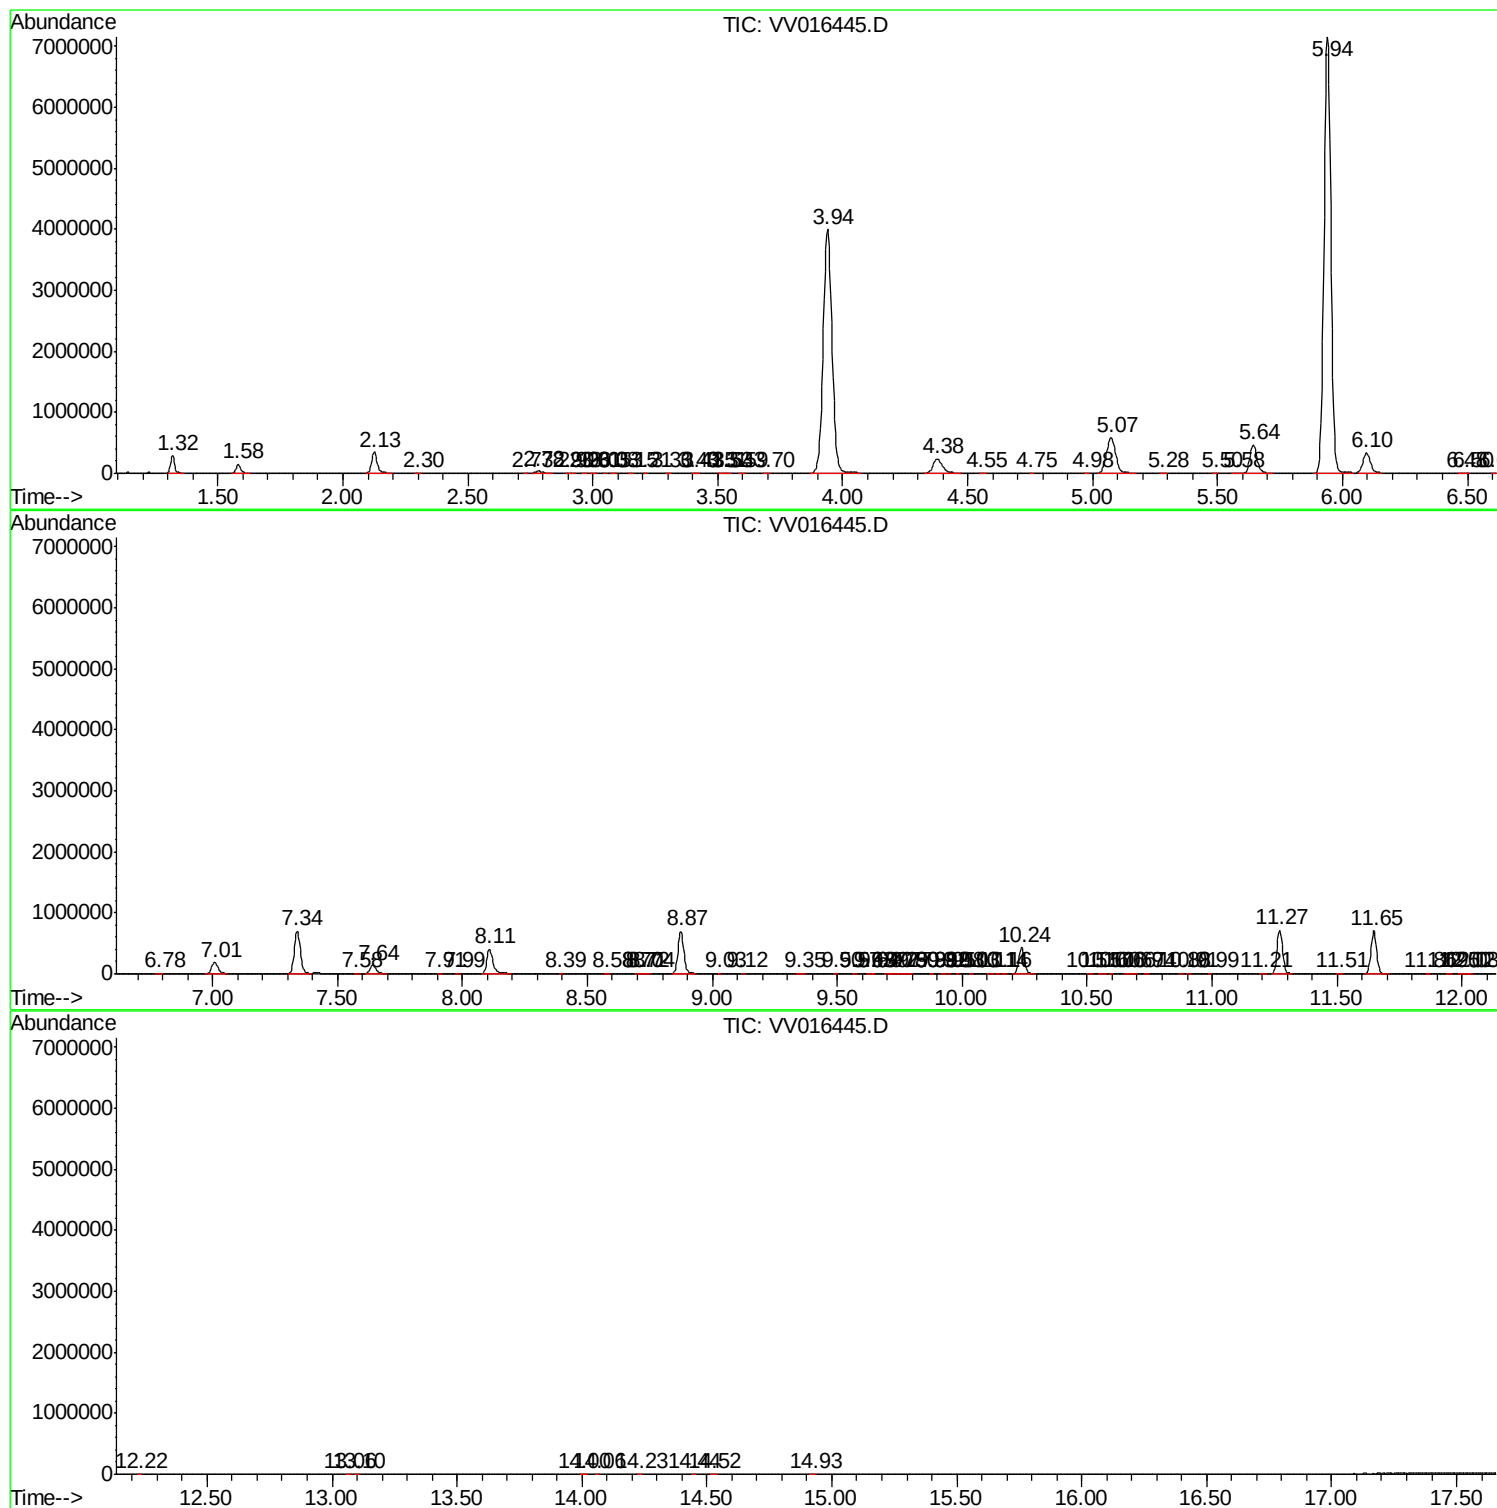

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV060320\
Data File : VV016445.D
Acq On : 02 Jun 2020 22:44
Operator : SY/MD
Sample : L2843-03
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0AA6

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060320\
Data File : VV016445.D
Acq On : 02 Jun 2020 22:44
Operator : SY/MD
Sample : L2843-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc