

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016446.D
 Acq On : 02 Jun 2020 23:06
 Operator : SY/MD
 Sample : L2843-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	64	71	93	rVB2	318312	352600	1.02%	0.661%
2	1.579	145	152	166	rVB	142467	175792	0.51%	0.329%
3	2.126	312	322	341	rBV	337693	515986	1.50%	0.967%
4	2.595	463	468	472	rVB7	1878	1984	0.01%	0.004%
5	2.621	472	476	477	rBV3	1265	834	0.00%	0.002%
6	2.708	501	503	505	rBV2	1321	544	0.00%	0.001%
7	2.730	508	510	512	rBV3	1813	623	0.00%	0.001%
8	2.785	519	527	542	rVB2	29069	53993	0.16%	0.101%
9	2.962	576	582	585	rBV6	1300	1355	0.00%	0.003%
10	2.991	589	591	595	rVB4	1252	742	0.00%	0.001%
11	3.010	595	597	599	rBV3	981	461	0.00%	0.001%
12	3.045	606	608	610	rBV3	1127	598	0.00%	0.001%
13	3.184	648	651	655	rBV3	971	856	0.00%	0.002%
14	3.213	655	660	662	rBV6	2663	2261	0.01%	0.004%
15	3.344	695	701	703	rBV6	1645	1402	0.00%	0.003%
16	3.438	725	730	733	rBV7	1918	1424	0.00%	0.003%
17	3.717	814	817	821	rBV4	1589	1226	0.00%	0.002%
18	3.778	833	836	838	rBV3	1366	732	0.00%	0.001%
19	3.852	854	859	860	rBV3	1326	1064	0.00%	0.002%
20	3.939	866	886	918	rBV	3000560	7431585	21.60%	13.929%
21	4.380	1008	1023	1048	rVB	244409	615843	1.79%	1.154%
22	4.872	1172	1176	1177	rBV3	1217	736	0.00%	0.001%
23	4.926	1190	1193	1194	rBV4	1585	1013	0.00%	0.002%
24	5.074	1222	1239	1267	rBV2	581044	1525257	4.43%	2.859%
25	5.270	1298	1300	1305	rBV5	1965	1379	0.00%	0.003%
26	5.357	1325	1327	1332	rBV6	1292	896	0.00%	0.002%
27	5.560	1387	1390	1393	rBV5	1536	1275	0.00%	0.002%
28	5.643	1402	1416	1440	rBV	467904	930356	2.70%	1.744%
29	5.846	1477	1479	1482	rBV4	1038	545	0.00%	0.001%
30	5.942	1491	1509	1543	rBV	17687447	34406654	100.00%	64.486%
31	6.097	1547	1557	1579	rVB	346698	690788	2.01%	1.295%
32	6.460	1668	1670	1671	rBV2	1638	758	0.00%	0.001%
33	6.547	1693	1697	1699	rBV4	1966	1431	0.00%	0.003%
34	6.810	1776	1779	1780	rBV4	1287	735	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016446.D
 Acq On : 02 Jun 2020 23:06
 Operator : SY/MD
 Sample : L2843-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.962	1823	1826	1828	rBV4	1284	737	0.00%	0.001%
36	7.007	1829	1840	1856	rVV	183666	325625	0.95%	0.610%
37	7.277	1922	1924	1926	rBV3	1489	595	0.00%	0.001%
38	7.338	1931	1943	1958	rBV	700331	1209296	3.51%	2.267%
39	7.643	2028	2038	2053	rBV	129525	218937	0.64%	0.410%
40	7.871	2101	2109	2117	rVB10	5959	10772	0.03%	0.020%
41	8.042	2160	2162	2164	rVB2	1313	489	0.00%	0.001%
42	8.058	2164	2167	2169	rBV2	1401	885	0.00%	0.002%
43	8.109	2172	2183	2210	rVV	408024	724211	2.10%	1.357%
44	8.576	2324	2328	2330	rBV4	937	672	0.00%	0.001%
45	8.720	2371	2373	2374	rBV2	1207	476	0.00%	0.001%
46	8.746	2378	2381	2383	rBV4	1303	940	0.00%	0.002%
47	8.875	2409	2421	2444	rBV	711927	1159420	3.37%	2.173%
48	9.132	2496	2501	2504	rBV6	1720	1507	0.00%	0.003%
49	9.167	2508	2512	2515	rBV4	2463	2741	0.01%	0.005%
50	9.232	2530	2532	2534	rBV3	1581	746	0.00%	0.001%
51	9.254	2537	2539	2542	rVB4	1393	699	0.00%	0.001%
52	9.280	2545	2547	2549	rBV2	932	442	0.00%	0.001%
53	9.424	2589	2592	2596	rVB6	2230	1756	0.01%	0.003%
54	9.447	2596	2599	2601	rBV4	1624	1046	0.00%	0.002%
55	9.553	2628	2632	2637	rBV8	1938	2131	0.01%	0.004%
56	9.669	2665	2668	2669	rBV3	1255	657	0.00%	0.001%
57	9.701	2675	2678	2680	rBV2	840	525	0.00%	0.001%
58	9.714	2680	2682	2684	rBV3	1155	681	0.00%	0.001%
59	9.817	2712	2714	2716	rBV3	1260	618	0.00%	0.001%
60	9.852	2723	2725	2729	rVB5	1278	888	0.00%	0.002%
61	9.990	2766	2768	2771	rVB4	1081	591	0.00%	0.001%
62	10.087	2796	2798	2801	rBV4	1097	690	0.00%	0.001%
63	10.145	2812	2816	2819	rBV5	913	568	0.00%	0.001%
64	10.238	2833	2845	2860	rBV	450501	699424	2.03%	1.311%
65	10.396	2890	2894	2895	rBV3	1957	1166	0.00%	0.002%
66	10.531	2933	2936	2941	rBV6	1712	1664	0.00%	0.003%
67	10.553	2941	2943	2946	rBV4	1411	966	0.00%	0.002%
68	10.730	2994	2998	3000	rBV3	837	580	0.00%	0.001%
69	10.759	3005	3007	3010	rBV4	931	744	0.00%	0.001%
70	10.900	3048	3051	3053	rBV3	791	489	0.00%	0.001%
71	11.093	3109	3111	3117	rVB6	1683	1371	0.00%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016446.D
 Acq On : 02 Jun 2020 23:06
 Operator : SY/MD
 Sample : L2843-04
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	11.125	3117	3121	3125	rVB7	1057	929	0.00%	0.002%
73	11.158	3128	3131	3133	rBV3	956	649	0.00%	0.001%
74	11.270	3154	3166	3181	rBV	729355	1112919	3.23%	2.086%
75	11.485	3230	3233	3238	rVB5	1589	1553	0.00%	0.003%
76	11.518	3238	3243	3245	rBV4	1506	1431	0.00%	0.003%
77	11.550	3248	3253	3254	rBV5	3433	3168	0.01%	0.006%
78	11.646	3269	3283	3300	rBV	711769	1113331	3.24%	2.087%
79	11.842	3341	3344	3346	rVB2	1088	686	0.00%	0.001%
80	11.858	3346	3349	3351	rBV3	2177	1317	0.00%	0.002%
81	12.022	3398	3400	3401	rBV2	1143	574	0.00%	0.001%
82	12.141	3434	3437	3440	rVB5	1066	522	0.00%	0.001%
83	12.157	3440	3442	3448	rBV5	842	905	0.00%	0.002%
84	12.273	3476	3478	3482	rVB4	1732	1140	0.00%	0.002%
85	12.437	3528	3529	3533	rVB3	1152	681	0.00%	0.001%
86	12.582	3570	3574	3580	rVB8	1924	2236	0.01%	0.004%
87	12.608	3580	3582	3584	rBV3	824	546	0.00%	0.001%
88	12.797	3637	3641	3643	rBV2	1826	1368	0.00%	0.003%
89	12.881	3663	3667	3668	rBV3	1213	840	0.00%	0.002%
90	13.042	3715	3717	3722	rBV5	1249	1026	0.00%	0.002%
91	13.093	3731	3733	3736	rBV4	1216	762	0.00%	0.001%
92	13.177	3756	3759	3760	rBV3	964	700	0.00%	0.001%
93	13.408	3829	3831	3834	rVB4	1639	658	0.00%	0.001%
94	13.453	3842	3845	3847	rBV3	1679	1096	0.00%	0.002%
95	13.759	3936	3940	3941	rBV3	1940	1034	0.00%	0.002%
96	13.968	4001	4005	4008	rBV5	1281	1029	0.00%	0.002%
97	14.264	4093	4097	4099	rBV5	1384	1084	0.00%	0.002%
98	14.360	4121	4127	4129	rBV7	1614	1644	0.00%	0.003%
99	14.765	4251	4253	4255	rBV2	1324	632	0.00%	0.001%
100	15.283	4412	4414	4418	rBV5	1684	1125	0.00%	0.002%


Sum of corrected areas: 53355058

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060320\
Data File : VV016446.D
Acq On : 02 Jun 2020 23:06
Operator : SY/MD
Sample : L2843-04
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
C0AA7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

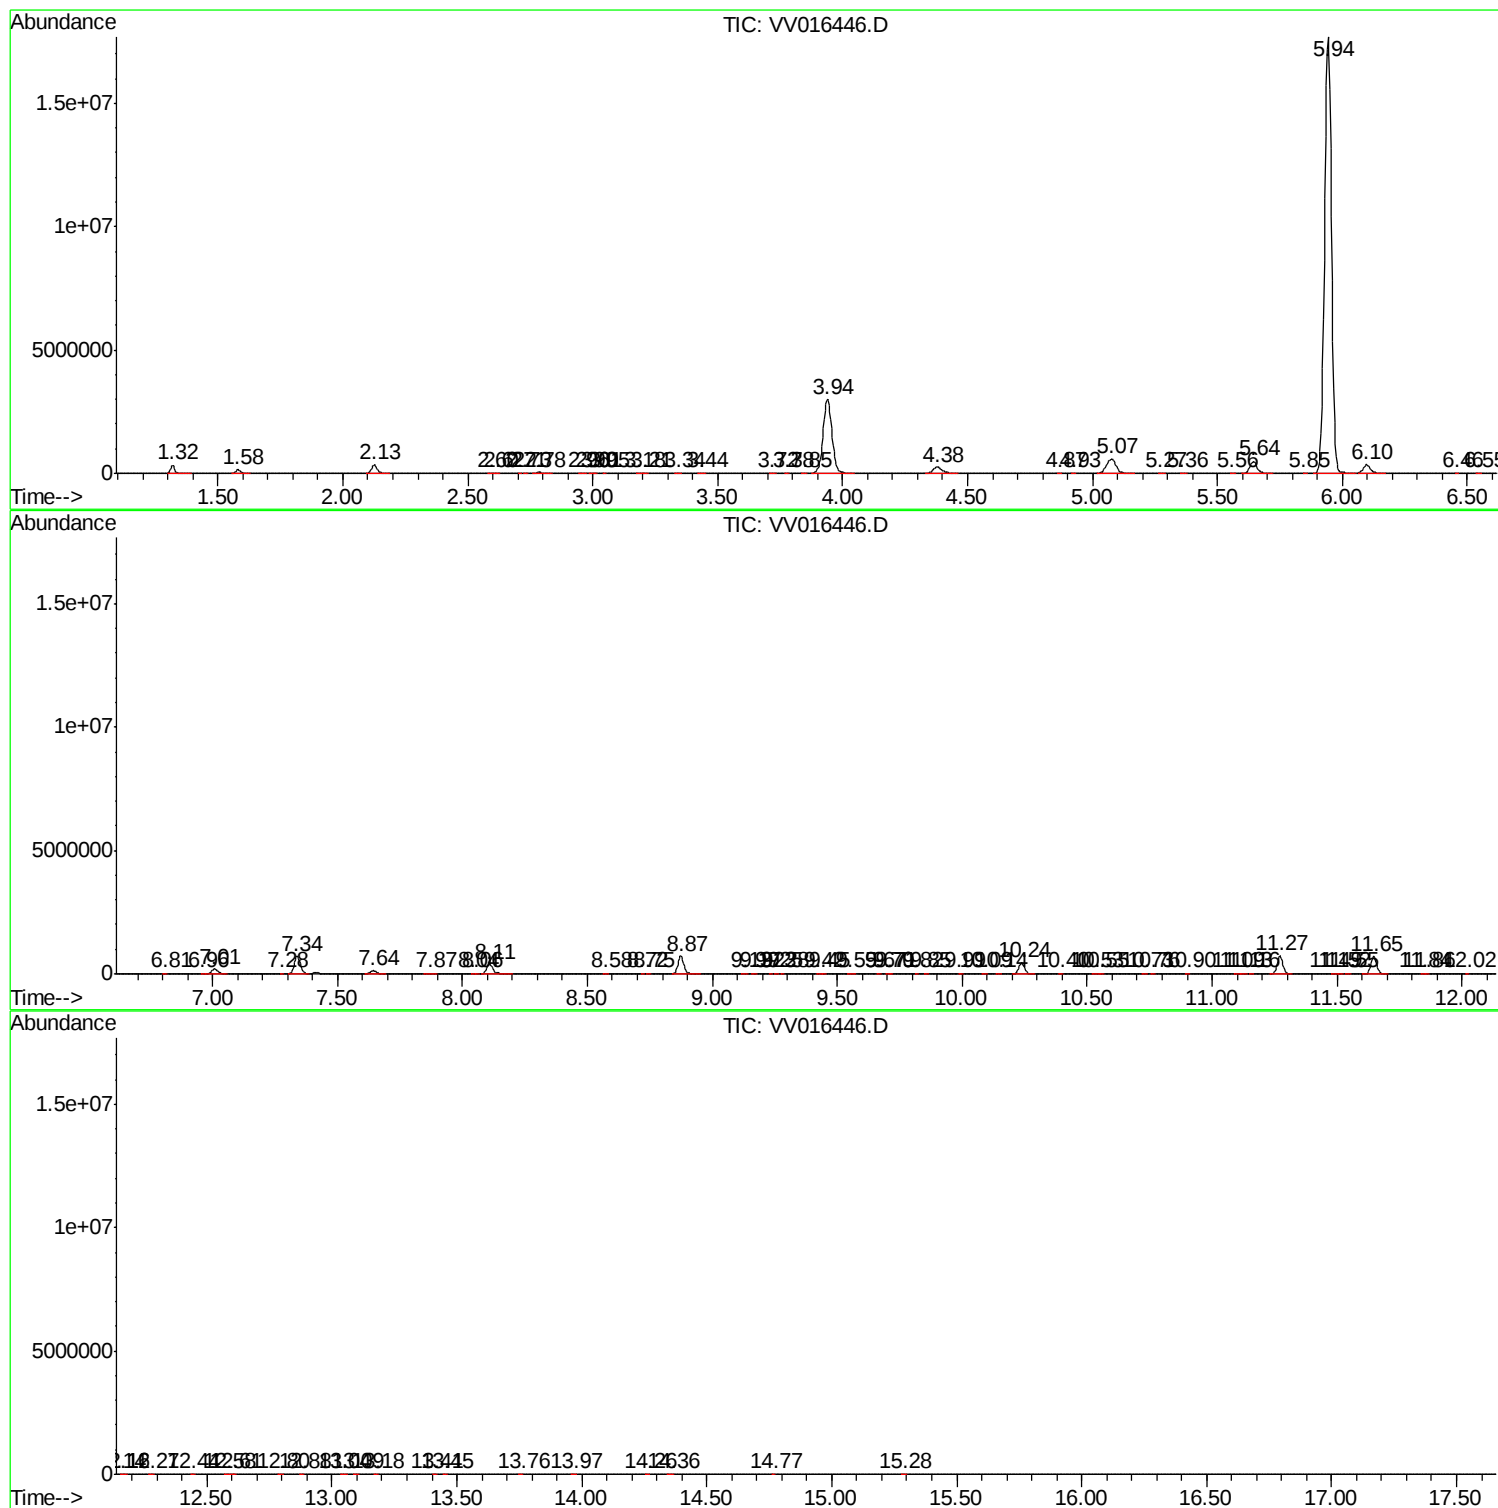

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060320\
Data File : VV016446.D
Acq On : 02 Jun 2020 23:06
Operator : SY/MD
Sample : L2843-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060320\
Data File : VV016446.D
Acq On : 02 Jun 2020 23:06
Operator : SY/MD
Sample : L2843-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA7

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc