

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016451.D
 Acq On : 03 Jun 2020 12:54
 Operator : SY/MD
 Sample : VV0603WBL02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK65

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	65	70	83	rVB	224358	231919	14.71%	1.932%
2	1.576	146	151	164	rVB	160185	182041	11.55%	1.517%
3	2.122	312	321	334	rBV	338916	492626	31.24%	4.105%
4	2.569	458	460	461	rBV2	1540	632	0.04%	0.005%
5	2.592	465	467	470	rBV3	1276	689	0.04%	0.006%
6	2.775	518	524	527	rBV7	1770	1956	0.12%	0.016%
7	2.839	540	544	546	rBV4	1233	1035	0.07%	0.009%
8	2.904	560	564	566	rBV6	819	593	0.04%	0.005%
9	2.974	580	586	589	rBV7	2339	2484	0.16%	0.021%
10	3.151	638	641	643	rBV3	1752	1019	0.06%	0.008%
11	3.380	710	712	715	rVB4	1577	774	0.05%	0.006%
12	3.399	715	718	720	rBV3	757	590	0.04%	0.005%
13	3.466	732	739	744	rBV3	1949	2372	0.15%	0.020%
14	3.547	760	764	768	rBV5	1641	1580	0.10%	0.013%
15	3.685	805	807	811	rBV4	778	612	0.04%	0.005%
16	3.711	811	815	816	rBV4	1434	854	0.05%	0.007%
17	3.791	837	840	841	rBV2	890	575	0.04%	0.005%
18	3.897	862	873	905	rVV2	123877	345084	21.89%	2.875%
19	4.151	950	952	956	rBV4	1229	866	0.05%	0.007%
20	4.376	1008	1022	1043	rVB	250773	602364	38.20%	5.019%
21	4.592	1087	1089	1091	rBV3	1577	1026	0.07%	0.009%
22	4.698	1120	1122	1126	rVB5	1280	753	0.05%	0.006%
23	4.720	1126	1129	1131	rBV4	1715	1107	0.07%	0.009%
24	4.756	1136	1140	1142	rVB4	1553	968	0.06%	0.008%
25	4.775	1142	1146	1151	rBV7	2044	1856	0.12%	0.015%
26	4.810	1154	1157	1160	rBV6	1181	842	0.05%	0.007%
27	4.849	1165	1169	1172	rBV5	1264	1142	0.07%	0.010%
28	4.939	1195	1197	1199	rBV3	1236	582	0.04%	0.005%
29	4.994	1210	1214	1217	rBV5	1702	1525	0.10%	0.013%
30	5.074	1220	1239	1264	rBV2	618207	1576677	100.00%	13.137%
31	5.289	1304	1306	1307	rBV2	1573	672	0.04%	0.006%
32	5.643	1402	1416	1441	rBV	475461	953250	60.46%	7.943%
33	6.023	1531	1534	1535	rBV3	1360	684	0.04%	0.006%
34	6.093	1544	1556	1582	rVB	354245	704103	44.66%	5.867%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016451.D
 Acq On : 03 Jun 2020 12:54
 Operator : SY/MD
 Sample : VV0603WBL02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK65

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.437	1660	1663	1667	rVB5	1368	1042	0.07%	0.009%
36	6.511	1682	1686	1689	rBV5	1935	1717	0.11%	0.014%
37	6.563	1699	1702	1704	rBV3	1029	744	0.05%	0.006%
38	6.601	1711	1714	1715	rBV2	1558	1055	0.07%	0.009%
39	6.717	1747	1750	1752	rBV4	1452	833	0.05%	0.007%
40	6.817	1779	1781	1784	rBV4	1021	543	0.03%	0.005%
41	6.871	1795	1798	1801	rVB4	1829	1260	0.08%	0.010%
42	6.932	1815	1817	1819	rVB3	1171	566	0.04%	0.005%
43	6.952	1819	1823	1826	rBV4	1174	958	0.06%	0.008%
44	7.006	1830	1840	1858	rVV	197199	349078	22.14%	2.909%
45	7.338	1931	1943	1963	rBV	734084	1246700	79.07%	10.388%
46	7.640	2027	2037	2053	rBV2	139040	241190	15.30%	2.010%
47	7.932	2125	2128	2131	rBV4	1026	834	0.05%	0.007%
48	8.055	2164	2166	2167	rBV2	1215	566	0.04%	0.005%
49	8.106	2172	2182	2205	rVV	471250	773322	49.05%	6.443%
50	8.778	2385	2391	2395	rBV7	2189	3147	0.20%	0.026%
51	8.820	2401	2404	2407	rVB4	1564	952	0.06%	0.008%
52	8.875	2407	2421	2444	rBV	725172	1167239	74.03%	9.726%
53	9.064	2477	2480	2482	rBV4	2160	1232	0.08%	0.010%
54	9.267	2541	2543	2547	rVB4	1813	1150	0.07%	0.010%
55	9.289	2547	2550	2551	rBV3	1102	606	0.04%	0.005%
56	9.357	2569	2571	2576	rVB3	1567	1083	0.07%	0.009%
57	9.428	2591	2593	2596	rVB5	2327	1241	0.08%	0.010%
58	9.479	2605	2609	2611	rVB3	1041	824	0.05%	0.007%
59	9.505	2611	2617	2621	rBV7	2078	2218	0.14%	0.018%
60	9.540	2626	2628	2630	rBV3	1119	701	0.04%	0.006%
61	9.682	2669	2672	2673	rBV3	1086	559	0.04%	0.005%
62	9.701	2675	2678	2680	rBV4	1345	678	0.04%	0.006%
63	9.746	2688	2692	2694	rBV3	1508	1178	0.07%	0.010%
64	9.829	2713	2718	2719	rBV4	1489	1102	0.07%	0.009%
65	9.839	2719	2721	2724	rVV3	1362	749	0.05%	0.006%
66	9.936	2749	2751	2755	rVV4	1248	857	0.05%	0.007%
67	10.038	2781	2783	2787	rVB5	1028	705	0.04%	0.006%
68	10.067	2787	2792	2795	rBV7	2518	2119	0.13%	0.018%
69	10.138	2811	2814	2816	rBV4	1850	1437	0.09%	0.012%
70	10.238	2829	2845	2863	rBV	475434	752610	47.73%	6.271%
71	10.566	2943	2947	2949	rBV4	1876	1369	0.09%	0.011%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016451.D
 Acq On : 03 Jun 2020 12:54
 Operator : SY/MD
 Sample : VV0603WBL02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK65

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	10.720	2993	2995	2997	rVB3	1570	703	0.04%	0.006%
73	10.781	3012	3014	3015	rBV2	1306	721	0.05%	0.006%
74	10.846	3030	3034	3036	rBV3	1107	853	0.05%	0.007%
75	10.936	3057	3062	3064	rBV4	2231	1911	0.12%	0.016%
76	11.103	3112	3114	3116	rBV3	987	547	0.03%	0.005%
77	11.154	3127	3130	3133	rBV4	1387	952	0.06%	0.008%
78	11.270	3155	3166	3185	rBV	743258	1127257	71.50%	9.392%
79	11.521	3242	3244	3246	rBV3	1156	499	0.03%	0.004%
80	11.646	3272	3283	3300	rBV	755040	1162023	73.70%	9.682%
81	12.151	3438	3440	3442	rBV3	1470	699	0.04%	0.006%
82	12.292	3479	3484	3485	rBV5	1748	1335	0.08%	0.011%
83	12.350	3496	3502	3503	rBV5	2130	1934	0.12%	0.016%
84	12.530	3554	3558	3559	rBV2	1615	978	0.06%	0.008%
85	12.604	3576	3581	3584	rBV5	1621	1467	0.09%	0.012%
86	12.649	3592	3595	3596	rBV3	930	552	0.04%	0.005%
87	12.698	3607	3610	3612	rBV4	1206	811	0.05%	0.007%
88	12.907	3671	3675	3679	rBV5	1146	1124	0.07%	0.009%
89	13.013	3705	3708	3710	rBV3	1139	754	0.05%	0.006%
90	13.061	3717	3723	3726	rBV7	1669	2154	0.14%	0.018%
91	13.206	3763	3768	3769	rBV4	2013	1462	0.09%	0.012%
92	13.231	3775	3776	3779	rBV2	1638	662	0.04%	0.006%
93	13.251	3779	3782	3784	rBV3	1194	858	0.05%	0.007%
94	13.447	3841	3843	3846	rBV4	1542	1119	0.07%	0.009%
95	14.042	4025	4028	4029	rBV2	1709	907	0.06%	0.008%
96	14.132	4049	4056	4058	rBV7	4676	5015	0.32%	0.042%
97	14.270	4097	4099	4100	rBV2	1598	688	0.04%	0.006%
98	14.386	4131	4135	4136	rBV2	1276	856	0.05%	0.007%
99	14.492	4165	4168	4172	rBV7	2173	2074	0.13%	0.017%
100	14.710	4234	4236	4237	rBV	1804	809	0.05%	0.007%


Sum of corrected areas: 12001740

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060320\
Data File : VV016451.D
Acq On : 03 Jun 2020 12:54
Operator : SY/MD
Sample : VV0603WBL02
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK65

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

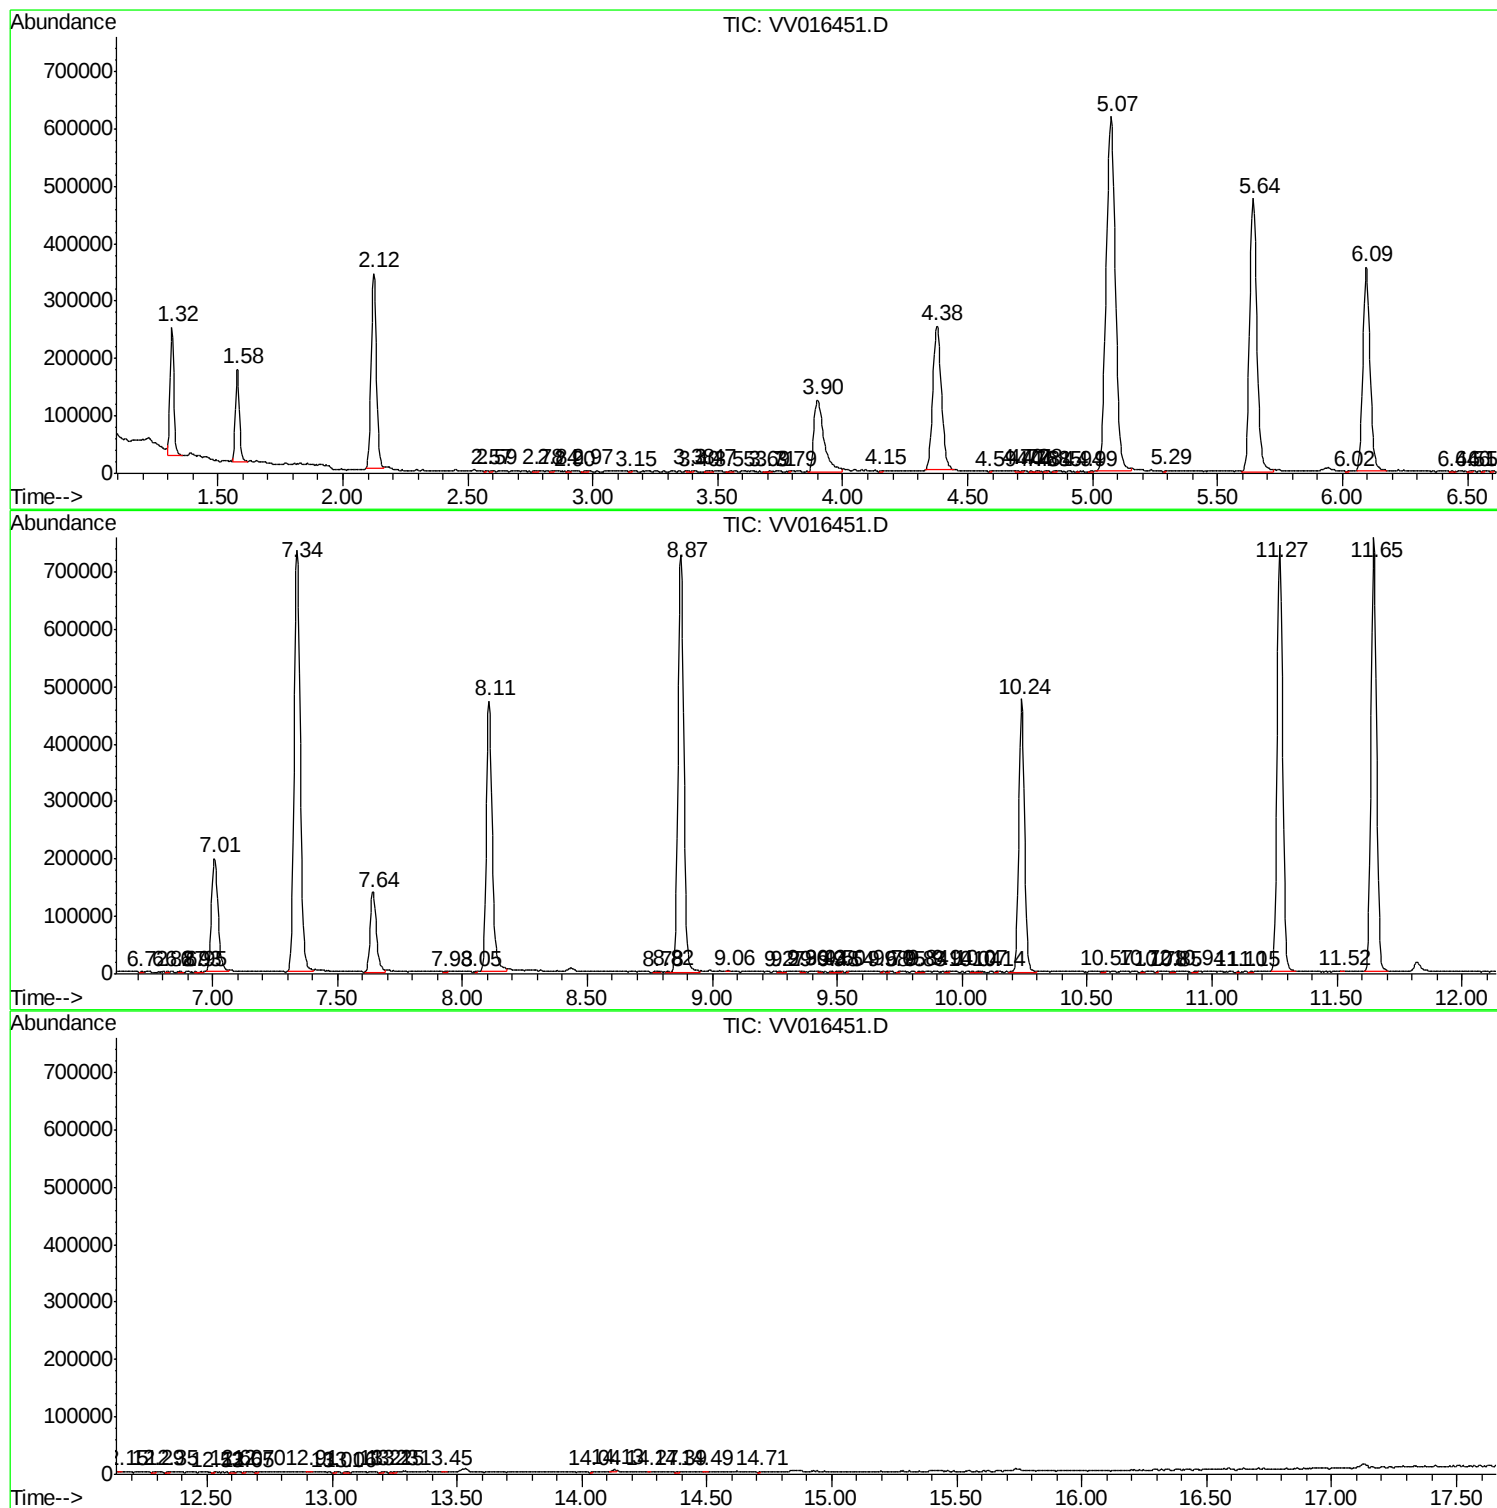

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060320\
Data File : VV016451.D
Acq On : 03 Jun 2020 12:54
Operator : SY/MD
Sample : VV0603WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK65

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV060320\
Data File : VV016451.D
Acq On : 03 Jun 2020 12:54
Operator : SY/MD
Sample : VV0603WBL02
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VBLK65

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc