

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016452.D
 Acq On : 03 Jun 2020 13:22
 Operator : SY/MD
 Sample : L2843-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	85	rVB2	575623	600913	2.42%	1.176%
2	1.576	146	151	163	rVB	158056	172931	0.70%	0.338%
3	2.123	311	321	334	rBV2	343825	520272	2.09%	1.018%
4	2.306	367	378	390	rBV3	10776	27574	0.11%	0.054%
5	2.624	471	477	478	rBV5	1930	1397	0.01%	0.003%
6	2.778	514	525	537	rBV	54584	96161	0.39%	0.188%
7	2.933	570	573	576	rVB3	1869	1085	0.00%	0.002%
8	3.032	600	604	605	rBV4	1249	737	0.00%	0.001%
9	3.055	609	611	615	rVV5	1150	831	0.00%	0.002%
10	3.071	615	616	621	rVB6	1168	691	0.00%	0.001%
11	3.145	636	639	641	rBV4	1266	865	0.00%	0.002%
12	3.161	641	644	646	rBV4	1129	693	0.00%	0.001%
13	3.177	646	649	651	rBV3	1601	1134	0.00%	0.002%
14	3.193	651	654	656	rBV3	1116	826	0.00%	0.002%
15	3.264	674	676	680	rVB4	1463	825	0.00%	0.002%
16	3.547	761	764	769	rBV4	1213	1000	0.00%	0.002%
17	3.576	769	773	778	rVV7	1041	1039	0.00%	0.002%
18	3.666	797	801	803	rBV5	1723	1158	0.00%	0.002%
19	3.762	827	831	834	rBV6	992	802	0.00%	0.002%
20	3.804	839	844	850	rBV8	1389	1401	0.01%	0.003%
21	3.836	852	854	857	rVB4	1770	788	0.00%	0.002%
22	3.933	862	884	922	rBV	5831796	14277499	57.48%	27.937%
23	4.373	1008	1021	1043	rVB2	243730	593729	2.39%	1.162%
24	4.759	1137	1141	1144	rBV6	1414	1222	0.00%	0.002%
25	4.839	1162	1166	1169	rBV6	1004	898	0.00%	0.002%
26	4.907	1183	1187	1188	rBV4	1276	842	0.00%	0.002%
27	5.071	1220	1238	1265	rBV2	589841	1523856	6.13%	2.982%
28	5.640	1399	1415	1448	rBV	473586	955104	3.84%	1.869%
29	5.939	1490	1508	1539	rBV	12737891	24841201	100.00%	48.608%
30	6.093	1546	1556	1574	rVB	336221	668918	2.69%	1.309%
31	6.335	1628	1631	1633	rBV4	2439	1606	0.01%	0.003%
32	6.576	1704	1706	1711	rBV5	1057	806	0.00%	0.002%
33	6.608	1711	1716	1719	rBV7	1665	1335	0.01%	0.003%
34	6.624	1719	1721	1723	rBV3	1239	647	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016452.D
 Acq On : 03 Jun 2020 13:22
 Operator : SY/MD
 Sample : L2843-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.794	1772	1774	1777	rVB4	1280	626	0.00%	0.001%
36	6.910	1808	1810	1814	rBV5	687	599	0.00%	0.001%
37	7.007	1829	1840	1861	rVV	193942	345322	1.39%	0.676%
38	7.273	1921	1923	1925	rBV3	1427	775	0.00%	0.002%
39	7.338	1930	1943	1958	rBV	709059	1215462	4.89%	2.378%
40	7.576	2015	2017	2021	rVB3	1456	882	0.00%	0.002%
41	7.595	2021	2023	2026	rBV3	1522	1042	0.00%	0.002%
42	7.640	2027	2037	2055	rVV	138810	236170	0.95%	0.462%
43	7.865	2100	2107	2119	rVB10	6691	10661	0.04%	0.021%
44	8.106	2170	2182	2207	rBV	439863	736677	2.97%	1.441%
45	8.354	2256	2259	2262	rVB5	1195	867	0.00%	0.002%
46	8.431	2280	2283	2285	rBV4	1699	844	0.00%	0.002%
47	8.672	2354	2358	2360	rBV5	1701	1179	0.00%	0.002%
48	8.749	2379	2382	2384	rBV4	936	662	0.00%	0.001%
49	8.871	2409	2420	2446	rVB	713660	1178040	4.74%	2.305%
50	9.093	2487	2489	2493	rBV5	1256	666	0.00%	0.001%
51	9.199	2519	2522	2523	rBV2	1257	689	0.00%	0.001%
52	9.235	2531	2533	2537	rVB5	1620	1163	0.00%	0.002%
53	9.373	2573	2576	2581	rVB7	1219	1036	0.00%	0.002%
54	9.399	2581	2584	2586	rBV4	935	592	0.00%	0.001%
55	9.495	2611	2614	2618	rBV5	1133	947	0.00%	0.002%
56	9.566	2626	2636	2640	rBV10	2527	3664	0.01%	0.007%
57	9.711	2677	2681	2683	rBV5	1118	825	0.00%	0.002%
58	9.733	2685	2688	2690	rVV3	1081	685	0.00%	0.001%
59	9.749	2690	2693	2694	rVV2	1105	667	0.00%	0.001%
60	9.823	2713	2716	2719	rVB4	1333	803	0.00%	0.002%
61	9.881	2732	2734	2737	rBV4	1238	727	0.00%	0.001%
62	9.955	2752	2757	2759	rVV6	1106	1060	0.00%	0.002%
63	10.019	2773	2777	2778	rVV4	964	645	0.00%	0.001%
64	10.029	2778	2780	2783	rVV2	1064	602	0.00%	0.001%
65	10.048	2783	2786	2789	rVB4	1501	1032	0.00%	0.002%
66	10.113	2804	2806	2810	rVB3	1837	895	0.00%	0.002%
67	10.238	2832	2845	2860	rBV	457604	713411	2.87%	1.396%
68	10.315	2867	2869	2871	rVB3	2147	1023	0.00%	0.002%
69	10.328	2871	2873	2874	rBV2	1497	644	0.00%	0.001%
70	10.363	2881	2884	2887	rVB4	1021	671	0.00%	0.001%
71	10.389	2887	2892	2893	rBV4	2051	1619	0.01%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016452.D
 Acq On : 03 Jun 2020 13:22
 Operator : SY/MD
 Sample : L2843-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	10.563	2944	2946	2950	rVB4	1288	619	0.00%	0.001%
73	10.707	2988	2991	2996	rVB6	1283	1009	0.00%	0.002%
74	10.740	2997	3001	3004	rVV3	893	617	0.00%	0.001%
75	10.852	3033	3036	3038	rBV3	1094	709	0.00%	0.001%
76	10.910	3051	3054	3058	rBV5	1063	931	0.00%	0.002%
77	10.984	3074	3077	3080	rBV4	1926	1238	0.00%	0.002%
78	11.039	3092	3094	3097	rBV3	836	614	0.00%	0.001%
79	11.093	3107	3111	3114	rVB5	1403	1073	0.00%	0.002%
80	11.116	3115	3118	3120	rBV3	1345	656	0.00%	0.001%
81	11.158	3124	3131	3132	rBV4	1780	1559	0.01%	0.003%
82	11.186	3138	3140	3141	rBV2	1559	716	0.00%	0.001%
83	11.270	3153	3166	3185	rBV	752757	1152819	4.64%	2.256%
84	11.527	3243	3246	3248	rBV4	1748	1042	0.00%	0.002%
85	11.646	3272	3283	3300	rVB	742145	1149659	4.63%	2.250%
86	11.762	3315	3319	3320	rBV4	2040	1499	0.01%	0.003%
87	11.926	3367	3370	3372	rBV3	1475	895	0.00%	0.002%
88	12.167	3443	3445	3447	rBV2	1713	1066	0.00%	0.002%
89	12.621	3582	3586	3587	rBV3	1838	1309	0.01%	0.003%
90	12.952	3687	3689	3690	rBV2	1713	728	0.00%	0.001%
91	13.038	3713	3716	3720	rVB4	1119	893	0.00%	0.002%
92	13.067	3720	3725	3728	rBV6	1649	1656	0.01%	0.003%
93	13.225	3771	3774	3775	rBV2	1433	598	0.00%	0.001%
94	13.453	3837	3845	3847	rBV8	2352	3136	0.01%	0.006%
95	13.527	3860	3868	3875	rBV3	6466	11345	0.05%	0.022%
96	13.849	3966	3968	3972	rVB4	1096	661	0.00%	0.001%
97	14.029	4022	4024	4028	rVB3	1556	929	0.00%	0.002%
98	14.051	4028	4031	4032	rBV3	1433	787	0.00%	0.002%
99	14.485	4163	4166	4168	rBV4	1351	677	0.00%	0.001%
100	15.064	4343	4346	4348	rBV5	1702	1180	0.00%	0.002%


Sum of corrected areas: 51105280

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060320\
Data File : VV016452.D
Acq On : 03 Jun 2020 13:22
Operator : SY/MD
Sample : L2843-07
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
C0AB1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

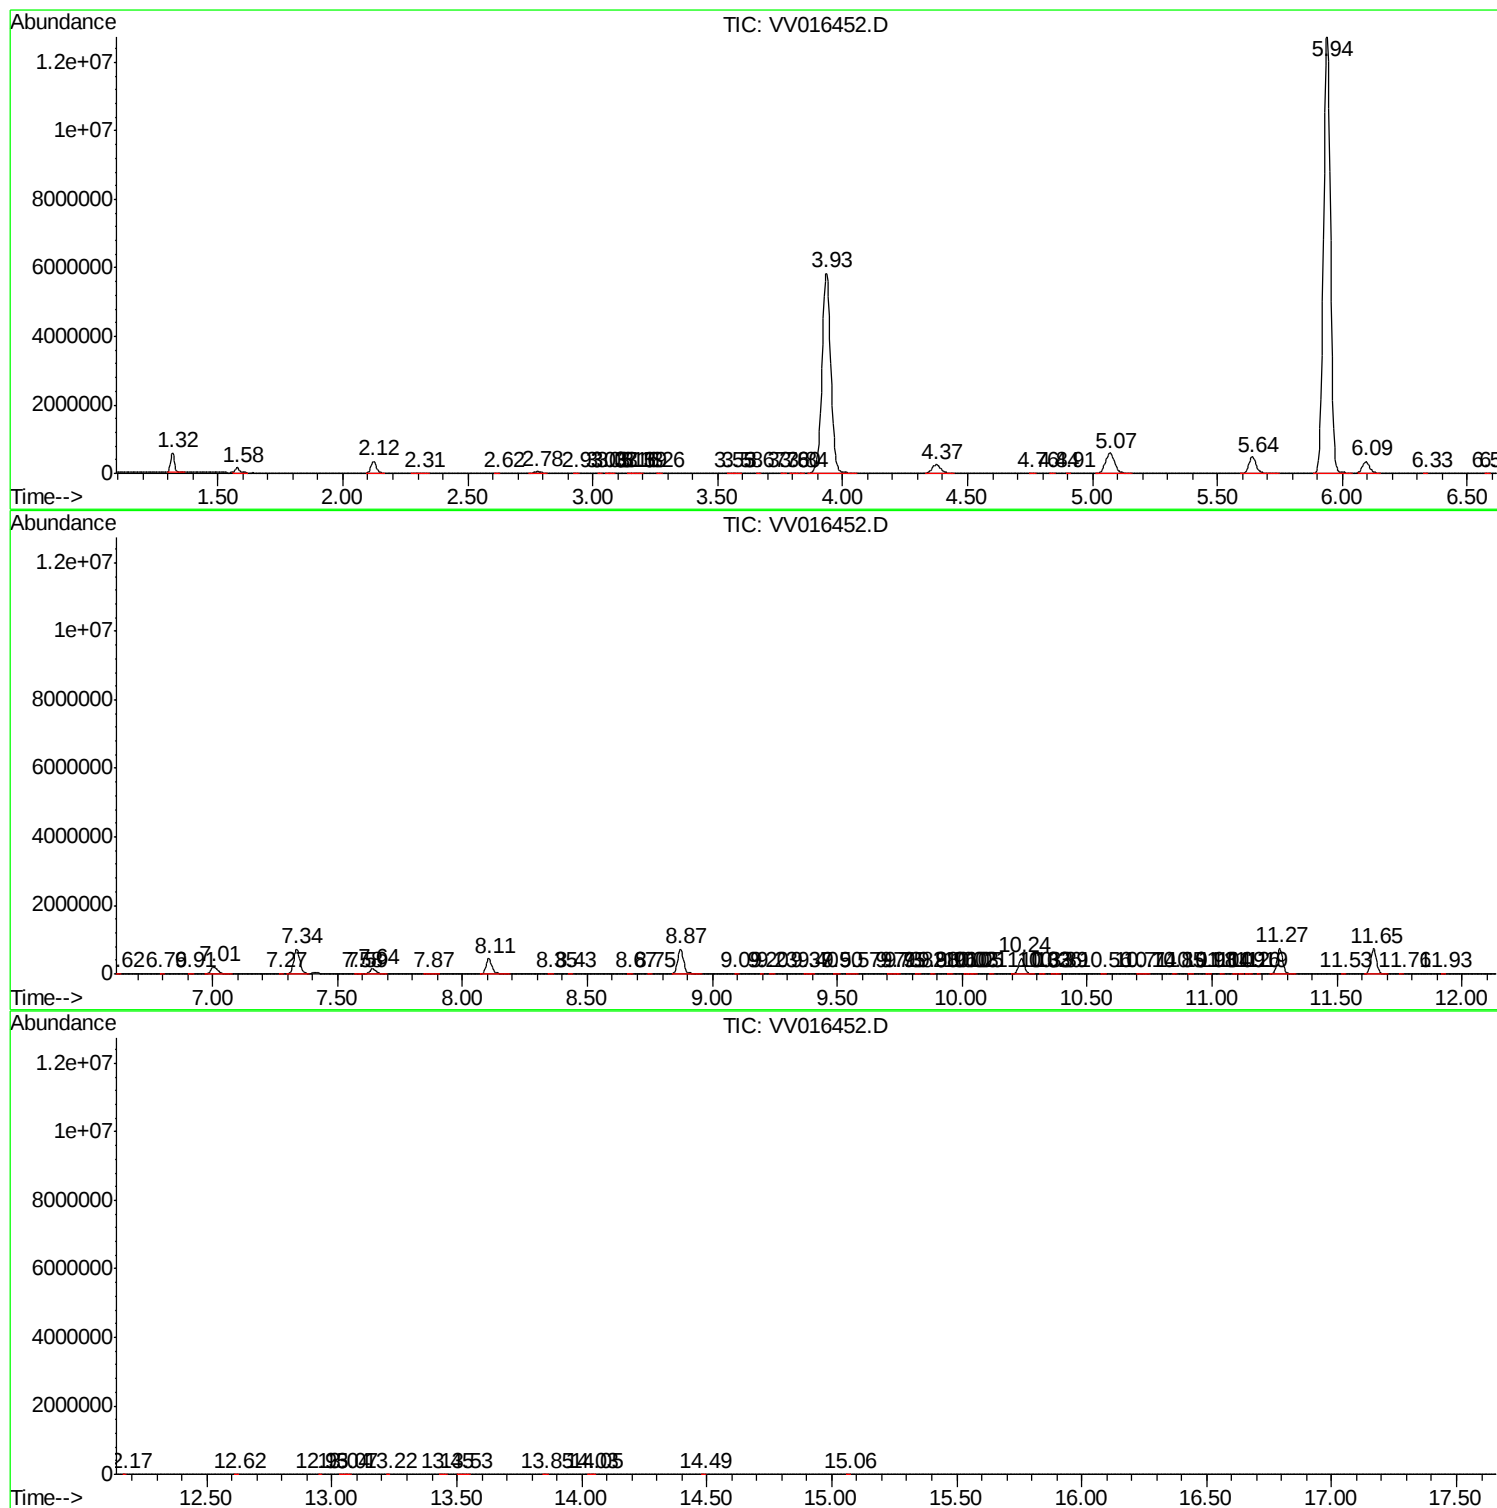

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV060320\
Data File : VV016452.D
Acq On : 03 Jun 2020 13:22
Operator : SY/MD
Sample : L2843-07
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0AB1

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060320\
Data File : VV016452.D
Acq On : 03 Jun 2020 13:22
Operator : SY/MD
Sample : L2843-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB1

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc