

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016453.D
 Acq On : 03 Jun 2020 13:45
 Operator : SY/MD
 Sample : L2843-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	65	70	82	rVB	205477	214472	2.29%	0.985%
2	1.579	146	152	161	rVB	150645	163933	1.75%	0.753%
3	2.123	312	321	334	rBV	317895	466543	4.99%	2.143%
4	2.586	463	465	467	rBV2	1762	948	0.01%	0.004%
5	2.785	517	527	533	rBV4	8470	13972	0.15%	0.064%
6	2.907	560	565	568	rBV6	1323	1443	0.02%	0.007%
7	3.148	639	640	643	rBV3	1131	568	0.01%	0.003%
8	3.193	652	654	657	rBV3	1122	783	0.01%	0.004%
9	3.431	724	728	730	rBV5	1078	580	0.01%	0.003%
10	3.444	730	732	733	rBV2	779	317	0.00%	0.001%
11	3.592	774	778	781	rBV3	932	857	0.01%	0.004%
12	3.627	787	789	790	rBV2	837	220	0.00%	0.001%
13	3.663	798	800	802	rBV3	1012	517	0.01%	0.002%
14	3.750	824	827	830	rBV3	1512	1264	0.01%	0.006%
15	3.775	833	835	837	rVB3	1131	512	0.01%	0.002%
16	3.939	862	886	919	rBV2	597087	1722908	18.42%	7.914%
17	4.377	1006	1022	1047	rBV	228346	574271	6.14%	2.638%
18	4.724	1128	1130	1133	rVB4	1094	365	0.00%	0.002%
19	4.852	1168	1170	1172	rBV3	1134	430	0.00%	0.002%
20	4.949	1198	1200	1201	rBV2	1227	587	0.01%	0.003%
21	5.010	1217	1219	1220	rBV2	740	281	0.00%	0.001%
22	5.074	1221	1239	1264	rVV2	568019	1457442	15.59%	6.695%
23	5.643	1403	1416	1439	rBV	432821	865521	9.26%	3.976%
24	5.939	1492	1508	1529	rBV	4916916	9350934	100.00%	42.952%
25	6.097	1546	1557	1577	rVB	324458	644733	6.89%	2.962%
26	6.544	1694	1696	1702	rVB7	1541	1268	0.01%	0.006%
27	6.708	1746	1747	1751	rBV3	916	736	0.01%	0.003%
28	6.746	1756	1759	1763	rBV6	1968	1226	0.01%	0.006%
29	6.817	1779	1781	1785	rBV5	1412	687	0.01%	0.003%
30	6.862	1793	1795	1800	rVB5	1296	979	0.01%	0.004%
31	6.888	1800	1803	1805	rBV3	1080	875	0.01%	0.004%
32	7.010	1830	1841	1858	rBV	173668	306793	3.28%	1.409%
33	7.338	1931	1943	1963	rBV	670798	1151857	12.32%	5.291%
34	7.553	2008	2010	2014	rBV3	1177	659	0.01%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016453.D
 Acq On : 03 Jun 2020 13:45
 Operator : SY/MD
 Sample : L2843-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	7.643	2028	2038	2055	rBV	123890	210890	2.26%	0.969%
36	7.865	2101	2107	2108	rBV6	2558	2177	0.02%	0.010%
37	8.039	2157	2161	2163	rBV4	1202	815	0.01%	0.004%
38	8.106	2171	2182	2201	rBV	422184	710458	7.60%	3.263%
39	8.486	2298	2300	2303	rVB4	1264	462	0.00%	0.002%
40	8.669	2355	2357	2363	rBV6	1331	1016	0.01%	0.005%
41	8.875	2410	2421	2440	rVB	660570	1058855	11.32%	4.864%
42	9.138	2501	2503	2507	rBV5	1178	984	0.01%	0.005%
43	9.312	2555	2557	2560	rVB3	1373	668	0.01%	0.003%
44	9.335	2562	2564	2566	rBV4	1159	620	0.01%	0.003%
45	9.807	2709	2711	2714	rBV4	1121	419	0.00%	0.002%
46	9.843	2720	2722	2727	rBV5	1331	924	0.01%	0.004%
47	9.904	2739	2741	2742	rBV2	1073	459	0.00%	0.002%
48	10.016	2775	2776	2779	rBV3	1100	409	0.00%	0.002%
49	10.151	2815	2818	2819	rBV2	929	469	0.01%	0.002%
50	10.174	2823	2825	2826	rBV2	1110	415	0.00%	0.002%
51	10.238	2833	2845	2864	rBV	441792	688437	7.36%	3.162%
52	10.370	2882	2886	2889	rBV6	1686	1450	0.02%	0.007%
53	10.498	2925	2926	2927	rBV	497	98	0.00%	0.000%
54	10.598	2954	2957	2961	rVB5	2037	1718	0.02%	0.008%
55	10.624	2961	2965	2968	rBV4	825	811	0.01%	0.004%
56	10.762	3007	3008	3010	rVB2	1052	329	0.00%	0.002%
57	10.791	3015	3017	3020	rBV4	821	596	0.01%	0.003%
58	10.833	3028	3030	3032	rVB3	1020	433	0.00%	0.002%
59	10.846	3032	3034	3037	rBV4	1081	640	0.01%	0.003%
60	10.933	3059	3061	3063	rVB3	1132	457	0.00%	0.002%
61	11.084	3105	3108	3110	rBV4	1220	829	0.01%	0.004%
62	11.097	3110	3112	3114	rVB3	1251	525	0.01%	0.002%
63	11.106	3114	3115	3118	rBV3	729	485	0.01%	0.002%
64	11.170	3131	3135	3137	rBV3	1373	1004	0.01%	0.005%
65	11.270	3155	3166	3182	rBV	677327	1017684	10.88%	4.675%
66	11.386	3199	3202	3205	rVB3	1914	1188	0.01%	0.005%
67	11.476	3227	3230	3232	rBV2	972	638	0.01%	0.003%
68	11.646	3271	3283	3302	rBV	700926	1096751	11.73%	5.038%
69	11.910	3363	3365	3369	rBB5	1530	797	0.01%	0.004%
70	12.029	3399	3402	3404	rBV4	1298	865	0.01%	0.004%
71	12.100	3420	3424	3427	rBV4	2114	2087	0.02%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016453.D
 Acq On : 03 Jun 2020 13:45
 Operator : SY/MD
 Sample : L2843-08
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	12.209	3455	3458	3459	rBV2	1348	703	0.01%	0.003%
73	12.331	3494	3496	3498	rBV3	1004	368	0.00%	0.002%
74	12.434	3525	3528	3531	rBV5	1310	986	0.01%	0.005%
75	12.466	3534	3538	3539	rBV4	1112	742	0.01%	0.003%
76	12.543	3558	3562	3565	rVB5	1563	1242	0.01%	0.006%
77	12.569	3565	3570	3573	rBV7	1486	1606	0.02%	0.007%
78	12.656	3593	3597	3599	rBV4	1387	1183	0.01%	0.005%
79	12.727	3616	3619	3621	rVB4	1255	612	0.01%	0.003%
80	12.736	3621	3622	3623	rBV	898	330	0.00%	0.002%
81	13.190	3761	3763	3765	rBV3	1594	668	0.01%	0.003%
82	13.215	3770	3771	3772	rBV	847	229	0.00%	0.001%
83	13.235	3775	3777	3783	rVV6	1161	860	0.01%	0.004%
84	13.344	3808	3811	3814	rVB4	1684	931	0.01%	0.004%
85	13.360	3814	3816	3817	rBV2	1286	519	0.01%	0.002%
86	14.125	4051	4054	4058	rBV5	1982	2092	0.02%	0.010%


Sum of corrected areas: 21770414

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060320\
Data File : VV016453.D
Acq On : 03 Jun 2020 13:45
Operator : SY/MD
Sample : L2843-08
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

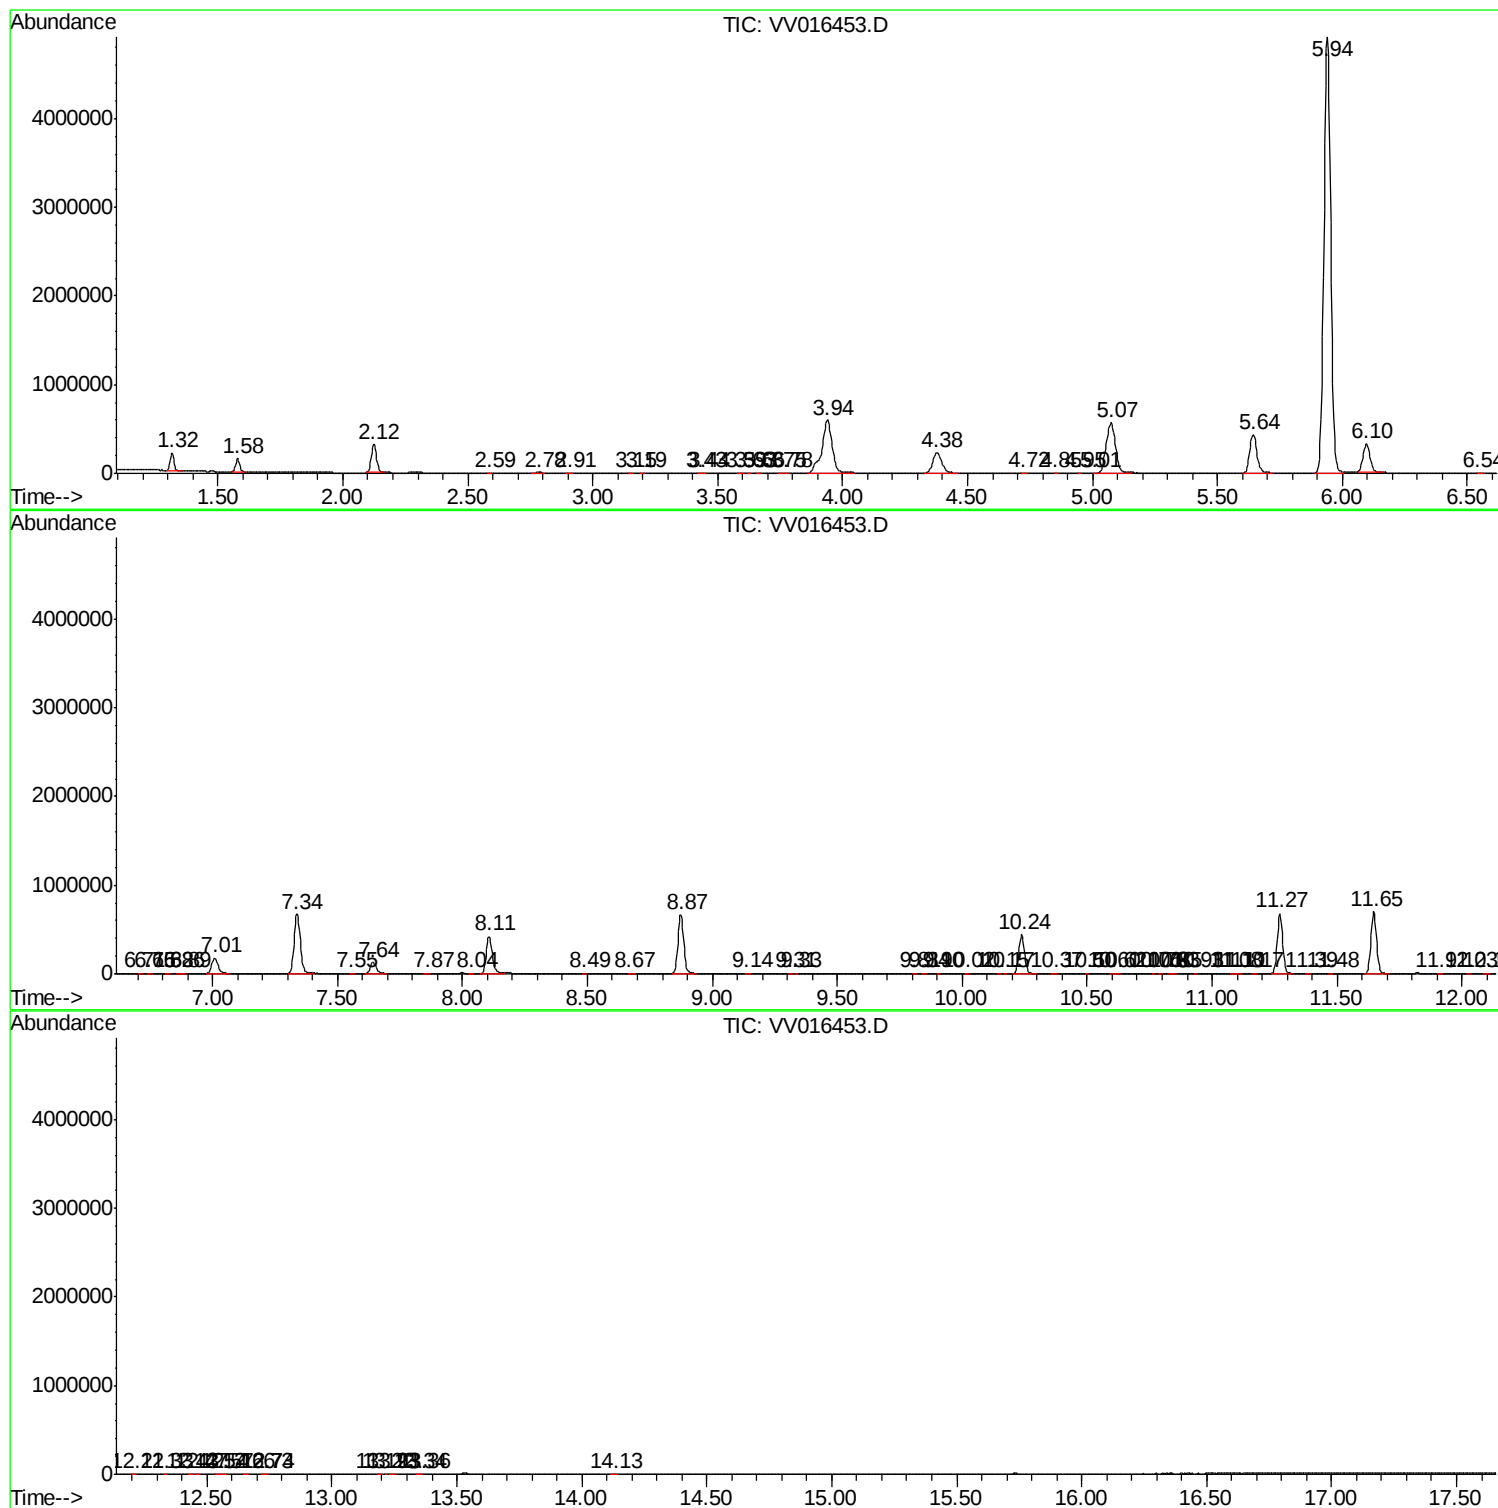

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV060320\
Data File : VV016453.D
Acq On : 03 Jun 2020 13:45
Operator : SY/MD
Sample : L2843-08
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0AB2

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060320\
Data File : VV016453.D
Acq On : 03 Jun 2020 13:45
Operator : SY/MD
Sample : L2843-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB2

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc