

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016454.D
 Acq On : 03 Jun 2020 14:09
 Operator : SY/MD
 Sample : L2843-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	88	rVB2	617389	670202	2.46%	1.273%
2	1.573	144	150	164	rVB	141712	161984	0.60%	0.308%
3	2.122	311	321	335	rBV2	335651	513569	1.89%	0.976%
4	2.589	463	466	468	rBV4	1388	1087	0.00%	0.002%
5	2.621	472	476	479	rVB4	1720	1299	0.00%	0.002%
6	2.647	481	484	486	rBV2	1389	743	0.00%	0.001%
7	2.669	486	491	492	rBV3	1251	1023	0.00%	0.002%
8	2.778	515	525	540	rVB2	54567	96207	0.35%	0.183%
9	2.917	564	568	569	rBV4	1389	1075	0.00%	0.002%
10	3.020	596	600	601	rBV3	711	606	0.00%	0.001%
11	3.206	652	658	660	rBV7	1705	1922	0.01%	0.004%
12	3.264	671	676	678	rBV6	1703	1528	0.01%	0.003%
13	3.331	694	697	699	rBV3	1074	603	0.00%	0.001%
14	3.370	703	709	712	rBV5	1702	1853	0.01%	0.004%
15	3.495	745	748	752	rVB4	1630	964	0.00%	0.002%
16	3.531	757	759	763	rBV5	665	635	0.00%	0.001%
17	3.759	828	830	832	rBV3	1313	609	0.00%	0.001%
18	3.856	856	860	862	rBV3	1106	759	0.00%	0.001%
19	3.936	862	885	920	rBV	5717508	13891309	51.07%	26.393%
20	4.376	1008	1022	1047	rVB	240483	593526	2.18%	1.128%
21	4.528	1065	1069	1072	rBV4	1908	1797	0.01%	0.003%
22	4.618	1095	1097	1101	rBV3	1334	990	0.00%	0.002%
23	4.685	1115	1118	1119	rBV3	1530	781	0.00%	0.001%
24	4.817	1154	1159	1167	rVB9	2190	3113	0.01%	0.006%
25	4.888	1178	1181	1183	rBV4	954	642	0.00%	0.001%
26	5.013	1217	1220	1221	rBV2	905	603	0.00%	0.001%
27	5.071	1221	1238	1267	rVV2	573665	1483674	5.46%	2.819%
28	5.344	1319	1323	1325	rBV3	2045	1429	0.01%	0.003%
29	5.386	1334	1336	1339	rBV4	1455	1107	0.00%	0.002%
30	5.515	1374	1376	1379	rBV3	1404	649	0.00%	0.001%
31	5.589	1397	1399	1401	rBV3	1171	729	0.00%	0.001%
32	5.640	1403	1415	1433	rVV	461059	909032	3.34%	1.727%
33	5.872	1483	1487	1490	rBV6	1517	1367	0.01%	0.003%
34	5.939	1490	1508	1542	rVV	14126410	27198350	100.00%	51.675%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016454.D
 Acq On : 03 Jun 2020 14:09
 Operator : SY/MD
 Sample : L2843-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.093	1546	1556	1582	rVB	333095	678456	2.49%	1.289%
36	6.582	1705	1708	1710	rBV3	1467	819	0.00%	0.002%
37	6.637	1720	1725	1728	rBV6	1583	1346	0.00%	0.003%
38	6.830	1782	1785	1786	rBV3	1401	668	0.00%	0.001%
39	6.881	1796	1801	1802	rBV6	1224	1057	0.00%	0.002%
40	7.007	1829	1840	1860	rBV	175189	310535	1.14%	0.590%
41	7.116	1871	1874	1876	rBV4	1247	929	0.00%	0.002%
42	7.338	1931	1943	1959	rBV	692240	1165700	4.29%	2.215%
43	7.640	2028	2037	2056	rBV	124157	216898	0.80%	0.412%
44	8.106	2172	2182	2198	rBV	434988	721621	2.65%	1.371%
45	8.341	2252	2255	2258	rBV5	1678	1050	0.00%	0.002%
46	8.437	2283	2285	2291	rBV7	1380	1218	0.00%	0.002%
47	8.550	2317	2320	2324	rVB5	1849	1171	0.00%	0.002%
48	8.582	2327	2330	2334	rBV5	1522	1515	0.01%	0.003%
49	8.617	2337	2341	2343	rBV2	1571	1224	0.00%	0.002%
50	8.678	2356	2360	2366	rBV8	1682	1751	0.01%	0.003%
51	8.714	2369	2371	2375	rVB3	1964	1041	0.00%	0.002%
52	8.772	2386	2389	2393	rVB5	1927	1433	0.01%	0.003%
53	8.804	2396	2399	2402	rBV4	1974	1388	0.01%	0.003%
54	8.871	2409	2420	2444	rBV	694354	1128432	4.15%	2.144%
55	9.264	2539	2542	2543	rBV3	1258	652	0.00%	0.001%
56	9.479	2603	2609	2611	rBV7	1252	1124	0.00%	0.002%
57	9.566	2634	2636	2638	rBV3	1301	798	0.00%	0.002%
58	9.669	2664	2668	2671	rVB4	1237	1080	0.00%	0.002%
59	9.833	2715	2719	2720	rBV3	992	611	0.00%	0.001%
60	9.846	2721	2723	2726	rVV3	1178	769	0.00%	0.001%
61	9.907	2739	2742	2745	rBV4	1812	1244	0.00%	0.002%
62	9.945	2751	2754	2758	rBV5	1438	1388	0.01%	0.003%
63	10.238	2830	2845	2862	rBV	445852	689948	2.54%	1.311%
64	10.347	2877	2879	2880	rBV2	1479	602	0.00%	0.001%
65	10.395	2891	2894	2899	rBV6	2328	2160	0.01%	0.004%
66	10.714	2989	2993	2997	rBV6	1156	1234	0.00%	0.002%
67	10.810	3017	3023	3026	rBV6	1734	1784	0.01%	0.003%
68	10.862	3036	3039	3043	rBV4	1344	1281	0.00%	0.002%
69	10.881	3043	3045	3049	rVV4	1364	833	0.00%	0.002%
70	11.270	3154	3166	3181	rBV	693491	1052669	3.87%	2.000%
71	11.418	3209	3212	3216	rBV6	1332	1372	0.01%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016454.D
 Acq On : 03 Jun 2020 14:09
 Operator : SY/MD
 Sample : L2843-09
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	11.479	3228	3231	3235	rVB4	1824	1369	0.01%	0.003%
73	11.498	3235	3237	3241	rBV4	742	593	0.00%	0.001%
74	11.524	3241	3245	3246	rBV4	1120	793	0.00%	0.002%
75	11.588	3264	3265	3269	rBV4	836	571	0.00%	0.001%
76	11.646	3271	3283	3298	rVV	684903	1064156	3.91%	2.022%
77	11.919	3365	3368	3370	rBV3	1068	662	0.00%	0.001%
78	12.042	3403	3406	3409	rBV4	1188	1025	0.00%	0.002%
79	12.119	3425	3430	3434	rVV7	1367	1782	0.01%	0.003%
80	12.167	3438	3445	3448	rBV8	1295	1526	0.01%	0.003%
81	12.212	3454	3459	3460	rBV4	1043	896	0.00%	0.002%
82	12.302	3485	3487	3489	rBV3	1513	760	0.00%	0.001%
83	12.338	3496	3498	3502	rBV4	1489	1000	0.00%	0.002%
84	12.357	3502	3504	3505	rBV2	1150	558	0.00%	0.001%
85	12.437	3525	3529	3530	rBV2	1554	1063	0.00%	0.002%
86	12.489	3541	3545	3549	rBV6	992	1044	0.00%	0.002%
87	12.698	3608	3610	3612	rBV2	1083	636	0.00%	0.001%
88	12.749	3623	3626	3627	rBV3	1277	808	0.00%	0.002%
89	12.817	3643	3647	3650	rBV4	1002	989	0.00%	0.002%
90	12.865	3660	3662	3664	rBV3	1477	884	0.00%	0.002%
91	13.135	3743	3746	3747	rBV3	945	563	0.00%	0.001%
92	13.235	3774	3777	3779	rBV4	1041	757	0.00%	0.001%
93	13.357	3813	3815	3820	rVB5	1614	953	0.00%	0.002%
94	13.379	3820	3822	3824	rBV3	1580	658	0.00%	0.001%
95	13.421	3831	3835	3836	rBV3	895	674	0.00%	0.001%
96	13.566	3878	3880	3885	rBV3	1091	1004	0.00%	0.002%
97	13.698	3919	3921	3925	rVB3	1147	609	0.00%	0.001%
98	13.862	3966	3972	3974	rBV5	2338	1882	0.01%	0.004%
99	14.653	4214	4218	4220	rBV4	1316	868	0.00%	0.002%
100	15.254	4403	4405	4406	rBV2	1595	603	0.00%	0.001%


Sum of corrected areas: 52633253

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060320\
Data File : VV016454.D
Acq On : 03 Jun 2020 14:09
Operator : SY/MD
Sample : L2843-09
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
C0AB4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

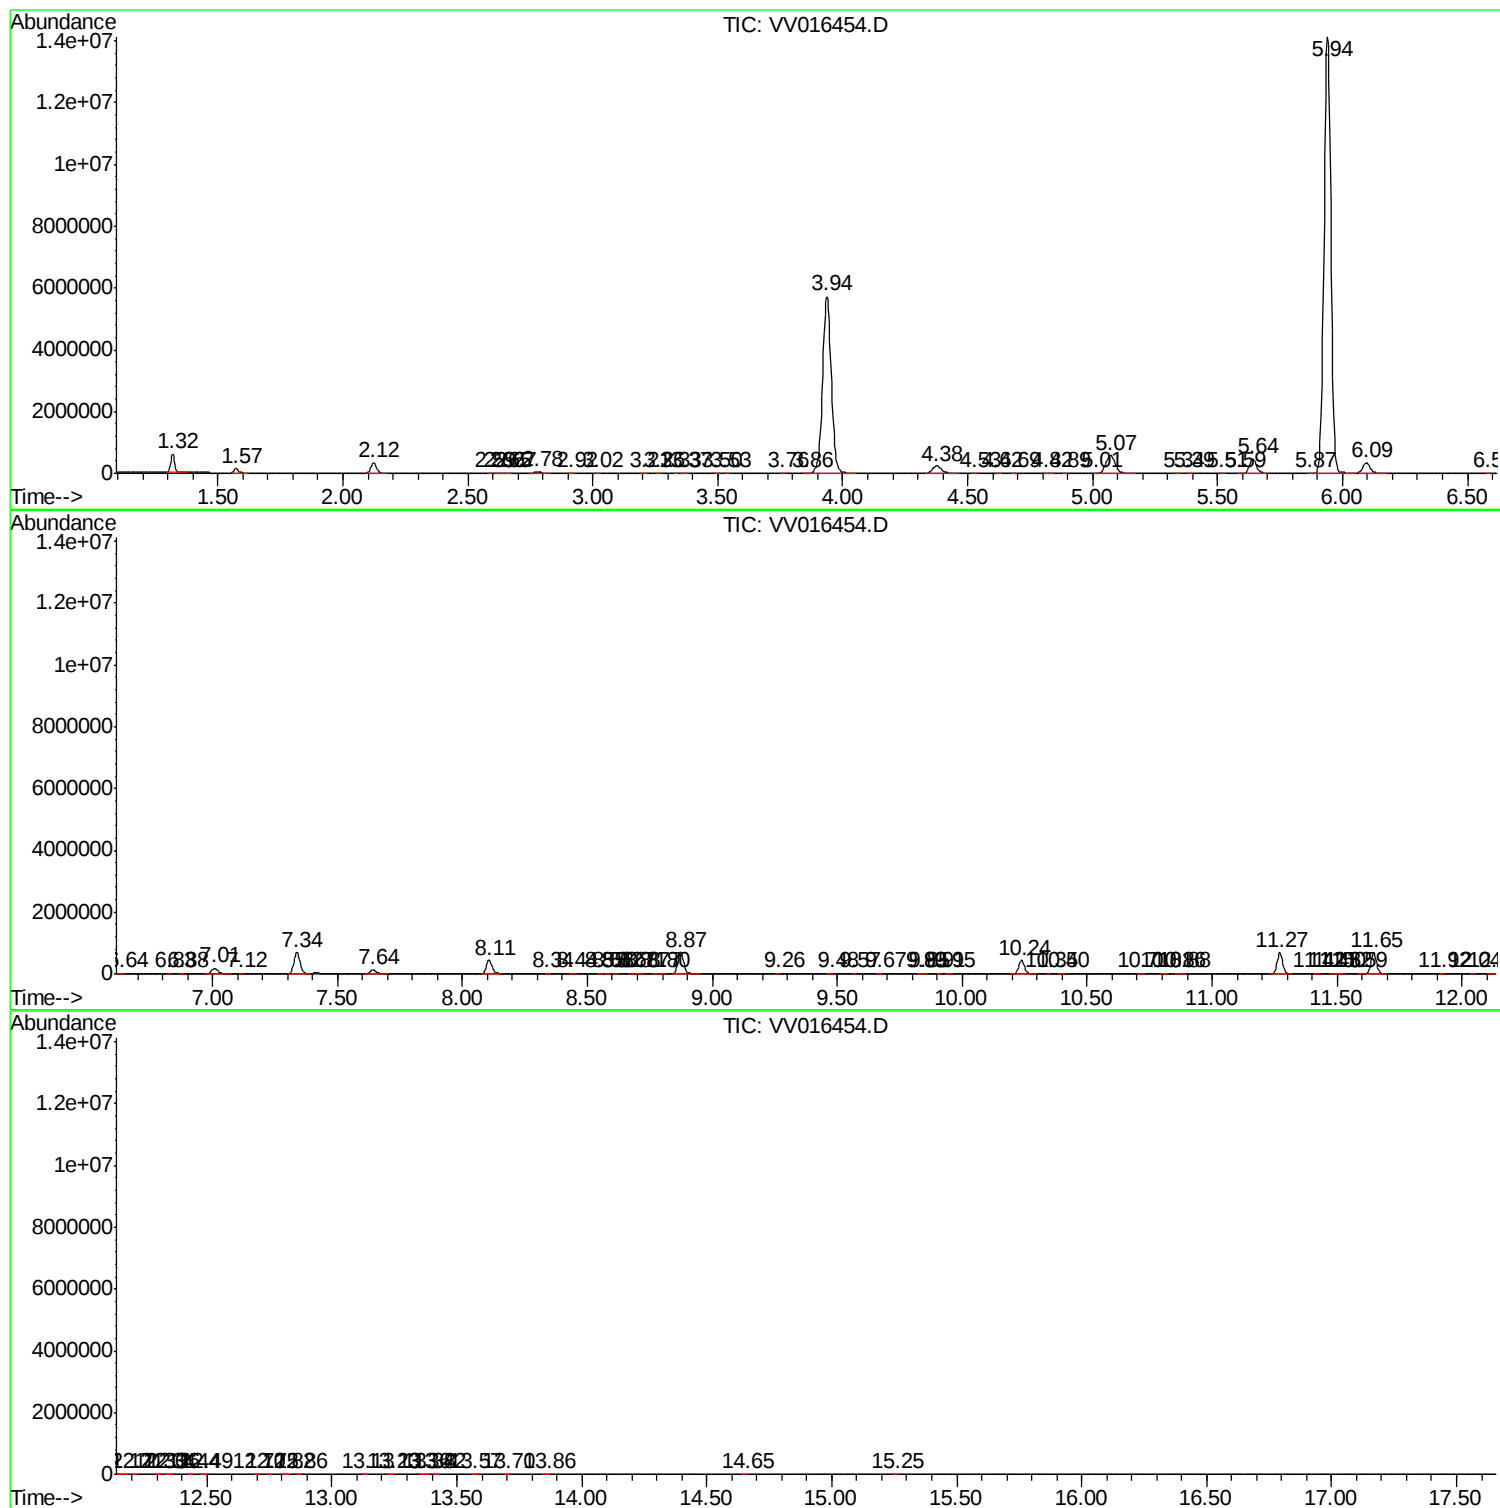

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060320\
Data File : VV016454.D
Acq On : 03 Jun 2020 14:09
Operator : SY/MD
Sample : L2843-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060320\
Data File : VV016454.D
Acq On : 03 Jun 2020 14:09
Operator : SY/MD
Sample : L2843-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB4

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc