

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016456.D
 Acq On : 03 Jun 2020 14:56
 Operator : SY/MD
 Sample : L2843-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	65	71	88	rVB2	606339	650526	4.36%	1.641%
2	1.576	145	151	165	rVB	152659	174743	1.17%	0.441%
3	2.123	311	321	334	rBV2	338163	518958	3.47%	1.309%
4	2.470	427	429	432	rBV3	1503	784	0.01%	0.002%
5	2.502	436	439	442	rBV4	1292	1108	0.01%	0.003%
6	2.643	478	483	486	rBV6	2200	2448	0.02%	0.006%
7	2.782	516	526	541	rVB	52123	93382	0.63%	0.236%
8	2.904	561	564	567	rVB5	1549	927	0.01%	0.002%
9	3.016	596	599	601	rBV4	1791	1152	0.01%	0.003%
10	3.055	607	611	614	rBV5	1154	1272	0.01%	0.003%
11	3.129	630	634	635	rBV3	1244	882	0.01%	0.002%
12	3.203	655	657	659	rBV3	1316	702	0.00%	0.002%
13	3.402	717	719	724	rVB5	1400	820	0.01%	0.002%
14	3.441	724	731	732	rBV5	1325	1116	0.01%	0.003%
15	3.473	739	741	745	rVB4	1458	993	0.01%	0.003%
16	3.515	752	754	761	rVB8	1793	1725	0.01%	0.004%
17	3.553	761	766	768	rBV5	1719	1584	0.01%	0.004%
18	3.695	807	810	813	rBV5	1334	1055	0.01%	0.003%
19	3.936	863	885	922	rVV	6119736	14936567	100.00%	37.681%
20	4.306	998	1000	1003	rBV3	1664	1071	0.01%	0.003%
21	4.376	1009	1022	1046	rVB	238587	583572	3.91%	1.472%
22	4.894	1181	1183	1186	rVB3	1458	689	0.00%	0.002%
23	4.907	1186	1187	1189	rBV2	1213	575	0.00%	0.001%
24	4.933	1191	1195	1199	rVB5	1349	1044	0.01%	0.003%
25	4.952	1199	1201	1207	rVB5	1489	1239	0.01%	0.003%
26	4.997	1212	1215	1217	rBV3	1333	692	0.00%	0.002%
27	5.074	1221	1239	1270	rBV2	578588	1501182	10.05%	3.787%
28	5.489	1367	1368	1370	rBV2	1508	717	0.00%	0.002%
29	5.640	1403	1415	1436	rBV	460258	913503	6.12%	2.305%
30	5.939	1491	1508	1540	rBV	6774889	12975135	86.87%	32.733%
31	6.093	1546	1556	1575	rVB	331251	659153	4.41%	1.663%
32	6.560	1699	1701	1703	rBV3	1291	663	0.00%	0.002%
33	6.730	1751	1754	1756	rBV4	1047	757	0.01%	0.002%
34	6.775	1764	1768	1770	rBV6	1279	1107	0.01%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016456.D
 Acq On : 03 Jun 2020 14:56
 Operator : SY/MD
 Sample : L2843-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.820	1780	1782	1784	rBV3	1450	736	0.00%	0.002%
36	6.894	1799	1805	1807	rVB6	1586	1458	0.01%	0.004%
37	7.007	1827	1840	1857	rBV	190396	346351	2.32%	0.874%
38	7.180	1892	1894	1896	rBV3	1271	625	0.00%	0.002%
39	7.338	1931	1943	1958	rBV	698092	1188714	7.96%	2.999%
40	7.640	2027	2037	2056	rBV	132770	231971	1.55%	0.585%
41	7.868	2099	2108	2116	rBV	5675	10364	0.07%	0.026%
42	7.936	2127	2129	2132	rBV3	1371	862	0.01%	0.002%
43	8.045	2162	2163	2167	rBV4	1204	927	0.01%	0.002%
44	8.106	2170	2182	2200	rBV	444766	744864	4.99%	1.879%
45	8.701	2364	2367	2369	rBV3	1588	723	0.00%	0.002%
46	8.756	2382	2384	2388	rVB4	1569	914	0.01%	0.002%
47	8.875	2409	2421	2445	rVB	684389	1133870	7.59%	2.860%
48	9.026	2466	2468	2470	rBV3	1496	865	0.01%	0.002%
49	9.154	2506	2508	2509	rBV2	1552	586	0.00%	0.001%
50	9.254	2535	2539	2541	rBV3	1248	1107	0.01%	0.003%
51	9.328	2559	2562	2563	rBV3	1255	706	0.00%	0.002%
52	9.341	2563	2566	2569	rBV3	1106	1081	0.01%	0.003%
53	9.547	2627	2630	2631	rBV3	1558	638	0.00%	0.002%
54	9.736	2687	2689	2693	rVB4	1132	691	0.00%	0.002%
55	10.055	2784	2788	2790	rVV3	1538	1254	0.01%	0.003%
56	10.068	2790	2792	2796	rVB4	2006	1278	0.01%	0.003%
57	10.119	2806	2808	2811	rBV4	1627	764	0.01%	0.002%
58	10.238	2831	2845	2860	rBV	450856	706127	4.73%	1.781%
59	10.354	2878	2881	2883	rBV5	1139	733	0.00%	0.002%
60	10.534	2936	2937	2940	rBV2	1398	647	0.00%	0.002%
61	10.572	2947	2949	2954	rVB5	1956	1348	0.01%	0.003%
62	10.601	2954	2958	2962	rVB6	1420	1290	0.01%	0.003%
63	10.624	2963	2965	2969	rVB3	1480	754	0.01%	0.002%
64	10.643	2969	2971	2973	rBV3	1438	794	0.01%	0.002%
65	10.675	2976	2981	2983	rBV5	1448	1151	0.01%	0.003%
66	10.704	2987	2990	2992	rBV3	1214	737	0.00%	0.002%
67	10.797	3016	3019	3021	rBV4	1736	1037	0.01%	0.003%
68	10.868	3036	3041	3043	rBV5	1496	1327	0.01%	0.003%
69	10.981	3074	3076	3079	rBV3	1191	689	0.00%	0.002%
70	11.023	3086	3089	3091	rBV4	1430	943	0.01%	0.002%
71	11.039	3092	3094	3096	rVV2	2138	1115	0.01%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016456.D
 Acq On : 03 Jun 2020 14:56
 Operator : SY/MD
 Sample : L2843-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	11.068	3099	3103	3104	rVV4	1478	995	0.01%	0.003%
73	11.077	3104	3106	3111	rVB4	1281	874	0.01%	0.002%
74	11.270	3155	3166	3185	rBV	705812	1078372	7.22%	2.720%
75	11.428	3213	3215	3217	rBV3	1610	934	0.01%	0.002%
76	11.646	3271	3283	3298	rBV	709170	1102521	7.38%	2.781%
77	11.794	3327	3329	3333	rBV5	1561	963	0.01%	0.002%
78	11.974	3381	3385	3389	rBV5	1231	1144	0.01%	0.003%
79	12.064	3410	3413	3417	rBV5	1385	1097	0.01%	0.003%
80	12.267	3474	3476	3480	rBV4	1237	725	0.00%	0.002%
81	12.302	3485	3487	3491	rBV5	947	718	0.00%	0.002%
82	12.479	3539	3542	3545	rBV4	1153	719	0.00%	0.002%
83	12.559	3565	3567	3569	rVB3	1537	593	0.00%	0.001%
84	12.627	3585	3588	3593	rVB7	1481	1138	0.01%	0.003%
85	12.656	3593	3597	3599	rBV5	1342	1108	0.01%	0.003%
86	12.669	3599	3601	3603	rBV3	1223	663	0.00%	0.002%
87	12.788	3636	3638	3642	rBV5	1308	796	0.01%	0.002%
88	12.952	3686	3689	3692	rBV4	1654	1257	0.01%	0.003%
89	12.974	3694	3696	3702	rVB4	1639	1396	0.01%	0.004%
90	13.154	3748	3752	3756	rBV6	1286	1374	0.01%	0.003%
91	13.460	3843	3847	3850	rBV5	1929	1778	0.01%	0.004%
92	13.527	3860	3868	3876	rBV3	6194	9919	0.07%	0.025%
93	13.733	3930	3932	3935	rBV4	1486	995	0.01%	0.003%
94	13.749	3935	3937	3940	rVB4	1720	784	0.01%	0.002%
95	13.772	3940	3944	3949	rBV8	1859	1756	0.01%	0.004%
96	13.971	4002	4006	4008	rBV2	1266	1085	0.01%	0.003%
97	14.209	4076	4080	4081	rBV3	1790	1216	0.01%	0.003%
98	14.501	4167	4171	4173	rBV4	1956	1331	0.01%	0.003%
99	14.553	4185	4187	4191	rBV5	1468	983	0.01%	0.002%
100	15.469	4470	4472	4474	rBV3	1440	704	0.00%	0.002%


Sum of corrected areas: 39639822

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060320\
Data File : VV016456.D
Acq On : 03 Jun 2020 14:56
Operator : SY/MD
Sample : L2843-06
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

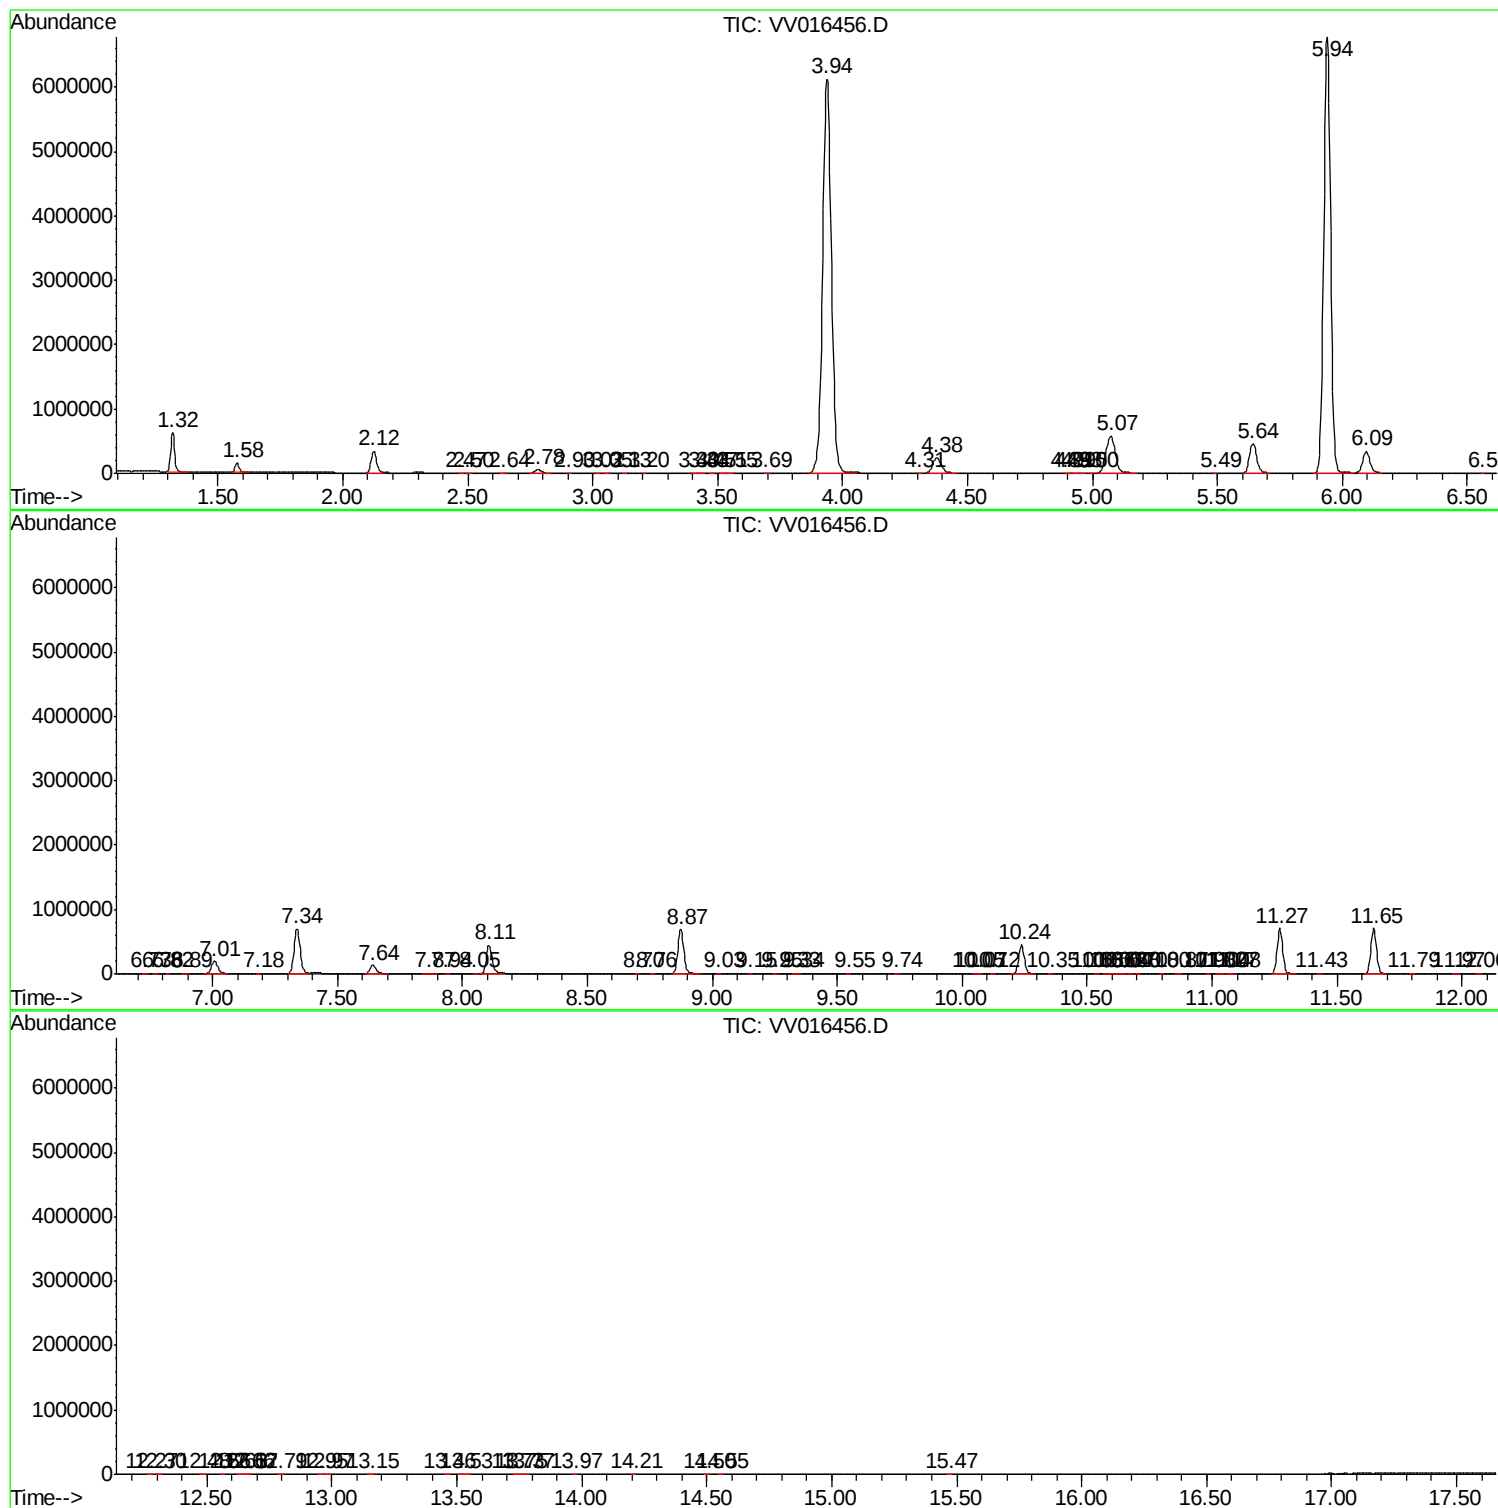

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060320\
Data File : VV016456.D
Acq On : 03 Jun 2020 14:56
Operator : SY/MD
Sample : L2843-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV060320\
Data File : VV016456.D
Acq On : 03 Jun 2020 14:56
Operator : SY/MD
Sample : L2843-06
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0AB0

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc