

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016457.D
 Acq On : 03 Jun 2020 15:23
 Operator : SY/MD
 Sample : VIBLK50
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK50

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	65	70	80	rVB	176728	179446	12.07%	1.597%
2	1.576	145	151	160	rVB	145281	154270	10.38%	1.373%
3	2.119	311	320	336	rBV	285416	416737	28.04%	3.710%
4	2.428	411	416	420	rBV7	1601	1711	0.12%	0.015%
5	2.592	466	467	470	rBV3	1235	645	0.04%	0.006%
6	2.647	481	484	485	rBV3	1227	737	0.05%	0.007%
7	2.824	537	539	542	rBV4	1169	914	0.06%	0.008%
8	2.888	554	559	562	rBV6	972	962	0.06%	0.009%
9	2.910	562	566	568	rBV3	1299	1060	0.07%	0.009%
10	2.939	573	575	580	rBV6	1280	1228	0.08%	0.011%
11	3.026	599	602	604	rBV3	914	619	0.04%	0.006%
12	3.039	604	606	608	rBV3	1325	703	0.05%	0.006%
13	3.081	617	619	623	rVB3	1235	738	0.05%	0.007%
14	3.100	623	625	626	rBV2	1311	598	0.04%	0.005%
15	3.245	667	670	675	rBV6	1905	1605	0.11%	0.014%
16	3.309	686	690	693	rBV5	1156	841	0.06%	0.007%
17	3.450	731	734	736	rBV3	1163	798	0.05%	0.007%
18	3.537	757	761	763	rBV5	1310	820	0.06%	0.007%
19	3.627	786	789	791	rBV3	1357	705	0.05%	0.006%
20	3.782	830	837	840	rBV8	1307	1196	0.08%	0.011%
21	3.833	847	853	854	rBV5	1063	802	0.05%	0.007%
22	3.897	862	873	903	rBV	119654	349247	23.49%	3.109%
23	4.184	958	962	964	rBV5	1327	1162	0.08%	0.010%
24	4.373	1007	1021	1046	rVB	240590	588883	39.62%	5.242%
25	4.666	1109	1112	1116	rVB5	1266	1050	0.07%	0.009%
26	4.688	1116	1119	1120	rBV3	1161	693	0.05%	0.006%
27	4.721	1128	1129	1133	rVB3	1204	698	0.05%	0.006%
28	4.740	1133	1135	1138	rBV4	1497	829	0.06%	0.007%
29	4.782	1144	1148	1150	rBV4	1390	899	0.06%	0.008%
30	4.814	1156	1158	1161	rBV3	857	587	0.04%	0.005%
31	5.000	1212	1216	1219	rBV6	1182	1109	0.07%	0.010%
32	5.071	1221	1238	1266	rVV2	576044	1486474	100.00%	13.233%
33	5.328	1315	1318	1319	rBV3	1240	713	0.05%	0.006%
34	5.640	1402	1415	1440	rBV	455941	903949	60.81%	8.047%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016457.D
 Acq On : 03 Jun 2020 15:23
 Operator : SY/MD
 Sample : VIBLK50
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK50

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.093	1543	1556	1575	rBV	342788	680058	45.75%	6.054%
36	6.367	1639	1641	1645	rBV4	1366	1030	0.07%	0.009%
37	6.399	1645	1651	1653	rBV6	1496	1193	0.08%	0.011%
38	6.489	1676	1679	1682	rVB4	1473	1011	0.07%	0.009%
39	6.511	1682	1686	1690	rBV5	1040	1035	0.07%	0.009%
40	6.547	1695	1697	1699	rBV3	1398	680	0.05%	0.006%
41	6.585	1705	1709	1711	rBV4	1536	1136	0.08%	0.010%
42	6.746	1756	1759	1764	rVB6	1584	886	0.06%	0.008%
43	6.791	1770	1773	1774	rBV3	1243	679	0.05%	0.006%
44	6.827	1778	1784	1788	rBV7	1154	1090	0.07%	0.010%
45	7.007	1829	1840	1862	rVB	185699	328268	22.08%	2.922%
46	7.338	1931	1943	1962	rBV	682498	1183643	79.63%	10.537%
47	7.640	2027	2037	2052	rBV	133453	223315	15.02%	1.988%
48	7.798	2084	2086	2089	rBV3	1914	1324	0.09%	0.012%
49	7.852	2101	2103	2105	rBV3	1310	686	0.05%	0.006%
50	7.910	2117	2121	2123	rBV4	1434	873	0.06%	0.008%
51	8.106	2171	2182	2209	rBV	440532	732359	49.27%	6.519%
52	8.508	2303	2307	2308	rBV4	1446	1030	0.07%	0.009%
53	8.627	2341	2344	2345	rBV3	1152	566	0.04%	0.005%
54	8.675	2357	2359	2362	rVB4	1121	547	0.04%	0.005%
55	8.717	2370	2372	2373	rBV2	1314	586	0.04%	0.005%
56	8.820	2401	2404	2407	rBV5	1064	892	0.06%	0.008%
57	8.871	2409	2420	2436	rVV	692981	1095450	73.69%	9.752%
58	9.331	2560	2563	2564	rBV3	1133	585	0.04%	0.005%
59	9.428	2590	2593	2596	rVB4	1459	780	0.05%	0.007%
60	9.524	2620	2623	2625	rBV4	1644	877	0.06%	0.008%
61	9.556	2628	2633	2636	rBV6	1908	1724	0.12%	0.015%
62	9.778	2700	2702	2705	rBV3	1084	683	0.05%	0.006%
63	9.997	2766	2770	2775	rVB5	1459	1298	0.09%	0.012%
64	10.129	2808	2811	2816	rVB6	1243	1243	0.08%	0.011%
65	10.164	2816	2822	2825	rBV7	1808	1809	0.12%	0.016%
66	10.238	2833	2845	2860	rBV	462142	714079	48.04%	6.357%
67	10.373	2885	2887	2889	rVV3	1214	553	0.04%	0.005%
68	10.476	2913	2919	2921	rBV7	1500	1680	0.11%	0.015%
69	10.511	2928	2930	2936	rVB5	1748	1842	0.12%	0.016%
70	10.814	3021	3024	3027	rBV4	1236	994	0.07%	0.009%
71	10.955	3065	3068	3069	rBV2	1059	568	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016457.D
 Acq On : 03 Jun 2020 15:23
 Operator : SY/MD
 Sample : VIBLK50
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK50

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	11.035	3091	3093	3098	rVB5	1399	1006	0.07%	0.009%
73	11.109	3114	3116	3119	rVB4	946	556	0.04%	0.005%
74	11.135	3119	3124	3128	rBV6	1470	1671	0.11%	0.015%
75	11.164	3128	3133	3136	rBV5	1855	1259	0.08%	0.011%
76	11.270	3154	3166	3185	rBV	669300	1019225	68.57%	9.073%
77	11.408	3208	3209	3212	rBV3	1233	747	0.05%	0.007%
78	11.476	3227	3230	3234	rBV5	2146	1831	0.12%	0.016%
79	11.646	3270	3283	3300	rBV	711042	1089513	73.30%	9.699%
80	11.932	3369	3372	3377	rBV7	1028	1061	0.07%	0.009%
81	11.987	3386	3389	3391	rBV4	841	655	0.04%	0.006%
82	12.051	3406	3409	3412	rBV4	841	538	0.04%	0.005%
83	12.141	3434	3437	3440	rBV3	829	766	0.05%	0.007%
84	12.231	3462	3465	3466	rBV3	1146	597	0.04%	0.005%
85	12.447	3528	3532	3534	rBV4	1386	1057	0.07%	0.009%
86	12.460	3534	3536	3539	rVB4	1573	777	0.05%	0.007%
87	12.550	3562	3564	3566	rBV3	1398	660	0.04%	0.006%
88	12.592	3574	3577	3579	rVB4	1514	779	0.05%	0.007%
89	12.936	3681	3684	3687	rBV5	1791	1669	0.11%	0.015%
90	13.180	3756	3760	3764	rVB7	1319	1125	0.08%	0.010%
91	13.199	3764	3766	3767	rBV	1104	602	0.04%	0.005%
92	13.228	3772	3775	3777	rBV3	825	583	0.04%	0.005%
93	13.530	3862	3869	3876	rBV7	6440	8361	0.56%	0.074%
94	13.813	3955	3957	3961	rBV4	1497	929	0.06%	0.008%
95	14.103	4045	4047	4049	rVB4	1689	784	0.05%	0.007%
96	14.132	4053	4056	4059	rBV4	1390	1080	0.07%	0.010%
97	14.244	4086	4091	4092	rBV4	2252	1400	0.09%	0.012%
98	14.608	4202	4204	4207	rBV3	1193	862	0.06%	0.008%
99	14.717	4236	4238	4239	rBV2	1365	662	0.04%	0.006%
100	15.026	4329	4334	4337	rBV5	2231	2136	0.14%	0.019%


Sum of corrected areas: 11233371

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060320\
Data File : VV016457.D
Acq On : 03 Jun 2020 15:23
Operator : SY/MD
Sample : VIBLK50
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK50

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

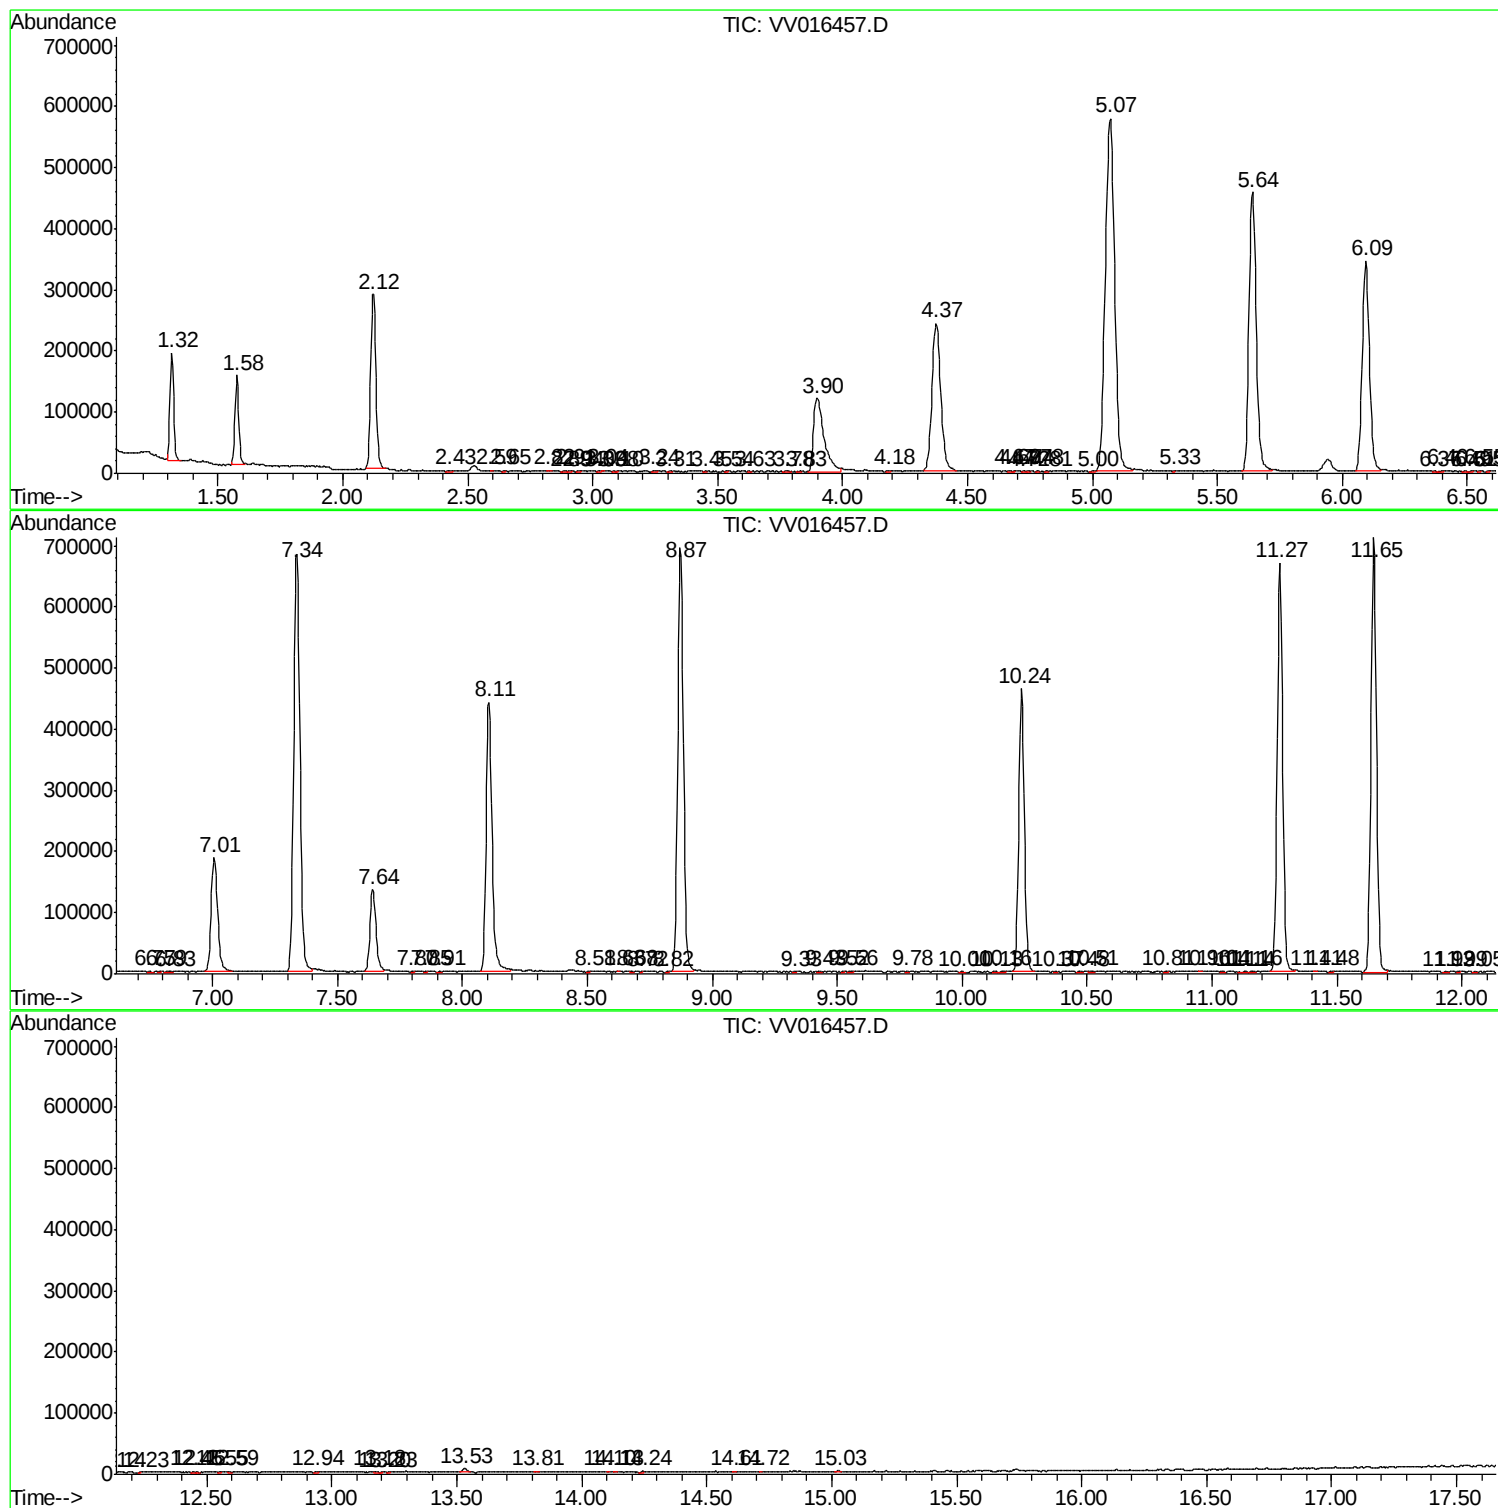

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060320\
Data File : VV016457.D
Acq On : 03 Jun 2020 15:23
Operator : SY/MD
Sample : VIBLK50
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK50

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV060320\
Data File : VV016457.D
Acq On : 03 Jun 2020 15:23
Operator : SY/MD
Sample : VIBLK50
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VIBLK50

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc