

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016459.D
 Acq On : 03 Jun 2020 16:12
 Operator : SY/MD
 Sample : L2843-02DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	65	70	83	rVB	215129	209236	13.66%	1.707%
2	1.573	144	150	161	rVB	150545	169104	11.04%	1.379%
3	2.122	311	321	340	rVB	322197	471795	30.81%	3.848%
4	2.457	423	425	431	rVB7	2147	1941	0.13%	0.016%
5	2.566	456	459	465	rVB8	1418	1176	0.08%	0.010%
6	2.592	465	467	470	rBV3	1321	799	0.05%	0.007%
7	2.746	511	515	517	rVV5	1219	859	0.06%	0.007%
8	2.846	544	546	553	rVB6	1313	962	0.06%	0.008%
9	2.878	553	556	558	rVB3	1527	728	0.05%	0.006%
10	2.904	559	564	567	rBV7	1148	1020	0.07%	0.008%
11	2.965	580	583	588	rVB7	1186	1178	0.08%	0.010%
12	2.997	588	593	596	rBV6	1223	1214	0.08%	0.010%
13	3.061	610	613	615	rBV2	1387	841	0.05%	0.007%
14	3.161	641	644	648	rBV5	1202	1001	0.07%	0.008%
15	3.251	670	672	675	rBV4	1446	987	0.06%	0.008%
16	3.296	684	686	690	rBV4	1293	845	0.06%	0.007%
17	3.392	710	716	719	rBV8	1268	1529	0.10%	0.012%
18	3.466	736	739	741	rBV3	1226	767	0.05%	0.006%
19	3.486	742	745	747	rBV3	1357	704	0.05%	0.006%
20	3.547	760	764	766	rVB4	1183	878	0.06%	0.007%
21	3.573	766	772	776	rBV6	1040	1078	0.07%	0.009%
22	3.611	780	784	786	rBV4	988	909	0.06%	0.007%
23	3.663	797	800	801	rBV3	1282	678	0.04%	0.006%
24	3.698	808	811	815	rBV4	1133	890	0.06%	0.007%
25	3.736	819	823	824	rBV5	1882	1296	0.08%	0.011%
26	3.894	861	872	903	rBV2	127403	425499	27.78%	3.471%
27	4.306	998	1000	1004	rVB3	1363	706	0.05%	0.006%
28	4.376	1004	1022	1049	rBV	242476	604347	39.46%	4.929%
29	4.560	1076	1079	1083	rBV2	967	711	0.05%	0.006%
30	4.608	1092	1094	1102	rVB8	2159	1877	0.12%	0.015%
31	4.772	1141	1145	1147	rBV4	1007	768	0.05%	0.006%
32	4.823	1159	1161	1166	rBV4	1187	1085	0.07%	0.009%
33	4.884	1177	1180	1182	rBV4	1259	839	0.05%	0.007%
34	4.917	1188	1190	1193	rBV3	1406	1020	0.07%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016459.D
 Acq On : 03 Jun 2020 16:12
 Operator : SY/MD
 Sample : L2843-02DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	4.933	1193	1195	1199	rVB5	1451	763	0.05%	0.006%
36	4.971	1205	1207	1211	rVB3	1131	645	0.04%	0.005%
37	5.071	1216	1238	1264	rBV2	594316	1531420	100.00%	12.491%
38	5.370	1329	1331	1333	rBV3	1445	690	0.05%	0.006%
39	5.460	1356	1359	1361	rBV4	1432	954	0.06%	0.008%
40	5.576	1392	1395	1398	rBV5	884	611	0.04%	0.005%
41	5.595	1398	1401	1402	rBV2	1057	702	0.05%	0.006%
42	5.640	1402	1415	1434	rBV	464230	915313	59.77%	7.466%
43	5.801	1463	1465	1468	rVB4	1591	615	0.04%	0.005%
44	5.939	1495	1508	1525	rBV	311145	603095	39.38%	4.919%
45	6.093	1544	1556	1581	rVB	337904	673791	44.00%	5.496%
46	6.328	1627	1629	1631	rBV3	1065	678	0.04%	0.006%
47	6.402	1649	1652	1657	rVB6	1346	1123	0.07%	0.009%
48	6.543	1686	1696	1697	rBV7	1250	1677	0.11%	0.014%
49	7.006	1827	1840	1860	rBV2	186715	340709	22.25%	2.779%
50	7.206	1900	1902	1905	rVB5	1706	777	0.05%	0.006%
51	7.235	1908	1911	1915	rBV6	1536	1277	0.08%	0.010%
52	7.338	1930	1943	1968	rBV	693645	1204525	78.65%	9.825%
53	7.640	2027	2037	2055	rBV	135101	227865	14.88%	1.859%
54	7.865	2104	2107	2112	rVB6	1310	875	0.06%	0.007%
55	7.952	2130	2134	2136	rVB5	1207	859	0.06%	0.007%
56	8.106	2172	2182	2207	rBV	460556	754953	49.30%	6.158%
57	8.547	2315	2319	2321	rBV4	1111	882	0.06%	0.007%
58	8.621	2339	2342	2344	rBV3	1540	935	0.06%	0.008%
59	8.875	2407	2421	2440	rBV	695296	1123521	73.36%	9.164%
60	9.026	2465	2468	2471	rBV3	1469	1229	0.08%	0.010%
61	9.074	2481	2483	2488	rVB6	1197	755	0.05%	0.006%
62	9.350	2567	2569	2570	rBV2	1264	689	0.04%	0.006%
63	9.524	2620	2623	2627	rVB4	1244	925	0.06%	0.008%
64	9.550	2627	2631	2633	rBV5	1927	1276	0.08%	0.010%
65	9.572	2636	2638	2642	rBV5	1421	989	0.06%	0.008%
66	9.643	2659	2660	2664	rVB4	1915	833	0.05%	0.007%
67	9.701	2676	2678	2681	rBV3	1198	754	0.05%	0.006%
68	9.826	2713	2717	2718	rBV2	1094	612	0.04%	0.005%
69	10.238	2832	2845	2861	rBV	466247	725606	47.38%	5.919%
70	10.424	2900	2903	2904	rBV2	1214	698	0.05%	0.006%
71	10.775	3007	3012	3014	rBV5	1424	1369	0.09%	0.011%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016459.D
 Acq On : 03 Jun 2020 16:12
 Operator : SY/MD
 Sample : L2843-02DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	10.858	3036	3038	3041	rVB4	1606	774	0.05%	0.006%
73	10.884	3041	3046	3048	rBV5	1540	1421	0.09%	0.012%
74	10.929	3057	3060	3063	rBV5	2156	1171	0.08%	0.010%
75	11.013	3079	3086	3088	rBV7	1760	1945	0.13%	0.016%
76	11.270	3154	3166	3187	rBV	698270	1073329	70.09%	8.755%
77	11.424	3212	3214	3219	rVB6	1429	1042	0.07%	0.008%
78	11.556	3252	3255	3257	rBV4	1340	790	0.05%	0.006%
79	11.646	3271	3283	3300	rBV	729021	1117928	73.00%	9.119%
80	11.791	3325	3328	3329	rBV3	1172	712	0.05%	0.006%
81	11.868	3349	3352	3353	rBV3	1104	682	0.04%	0.006%
82	12.064	3409	3413	3415	rBV3	1114	965	0.06%	0.008%
83	12.122	3427	3431	3437	rVB9	1000	1022	0.07%	0.008%
84	12.427	3523	3526	3529	rBV5	1179	642	0.04%	0.005%
85	12.482	3540	3543	3545	rVB5	1870	910	0.06%	0.007%
86	12.627	3585	3588	3592	rVB5	1267	929	0.06%	0.008%
87	12.659	3593	3598	3599	rBV4	1072	807	0.05%	0.007%
88	12.871	3661	3664	3665	rBV3	1102	613	0.04%	0.005%
89	13.193	3761	3764	3766	rBV4	1133	789	0.05%	0.006%
90	13.228	3773	3775	3779	rVB4	1800	841	0.05%	0.007%
91	13.283	3790	3792	3795	rVB4	1873	708	0.05%	0.006%
92	13.344	3809	3811	3815	rBV4	1131	782	0.05%	0.006%
93	13.450	3840	3844	3845	rBV4	1183	867	0.06%	0.007%
94	13.527	3860	3868	3878	rBV7	5347	9412	0.61%	0.077%
95	13.611	3892	3894	3898	rBV3	1646	1252	0.08%	0.010%
96	13.701	3920	3922	3925	rBV3	1450	923	0.06%	0.008%
97	14.000	4010	4015	4017	rBV5	1590	1293	0.08%	0.011%
98	14.624	4207	4209	4210	rBV2	1522	798	0.05%	0.007%
99	14.665	4220	4222	4226	rBV4	1597	974	0.06%	0.008%
100	14.923	4300	4302	4305	rVB3	2519	1374	0.09%	0.011%


Sum of corrected areas: 12259952

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060320\
Data File : VV016459.D
Acq On : 03 Jun 2020 16:12
Operator : SY/MD
Sample : L2843-02DL 10X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA5DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

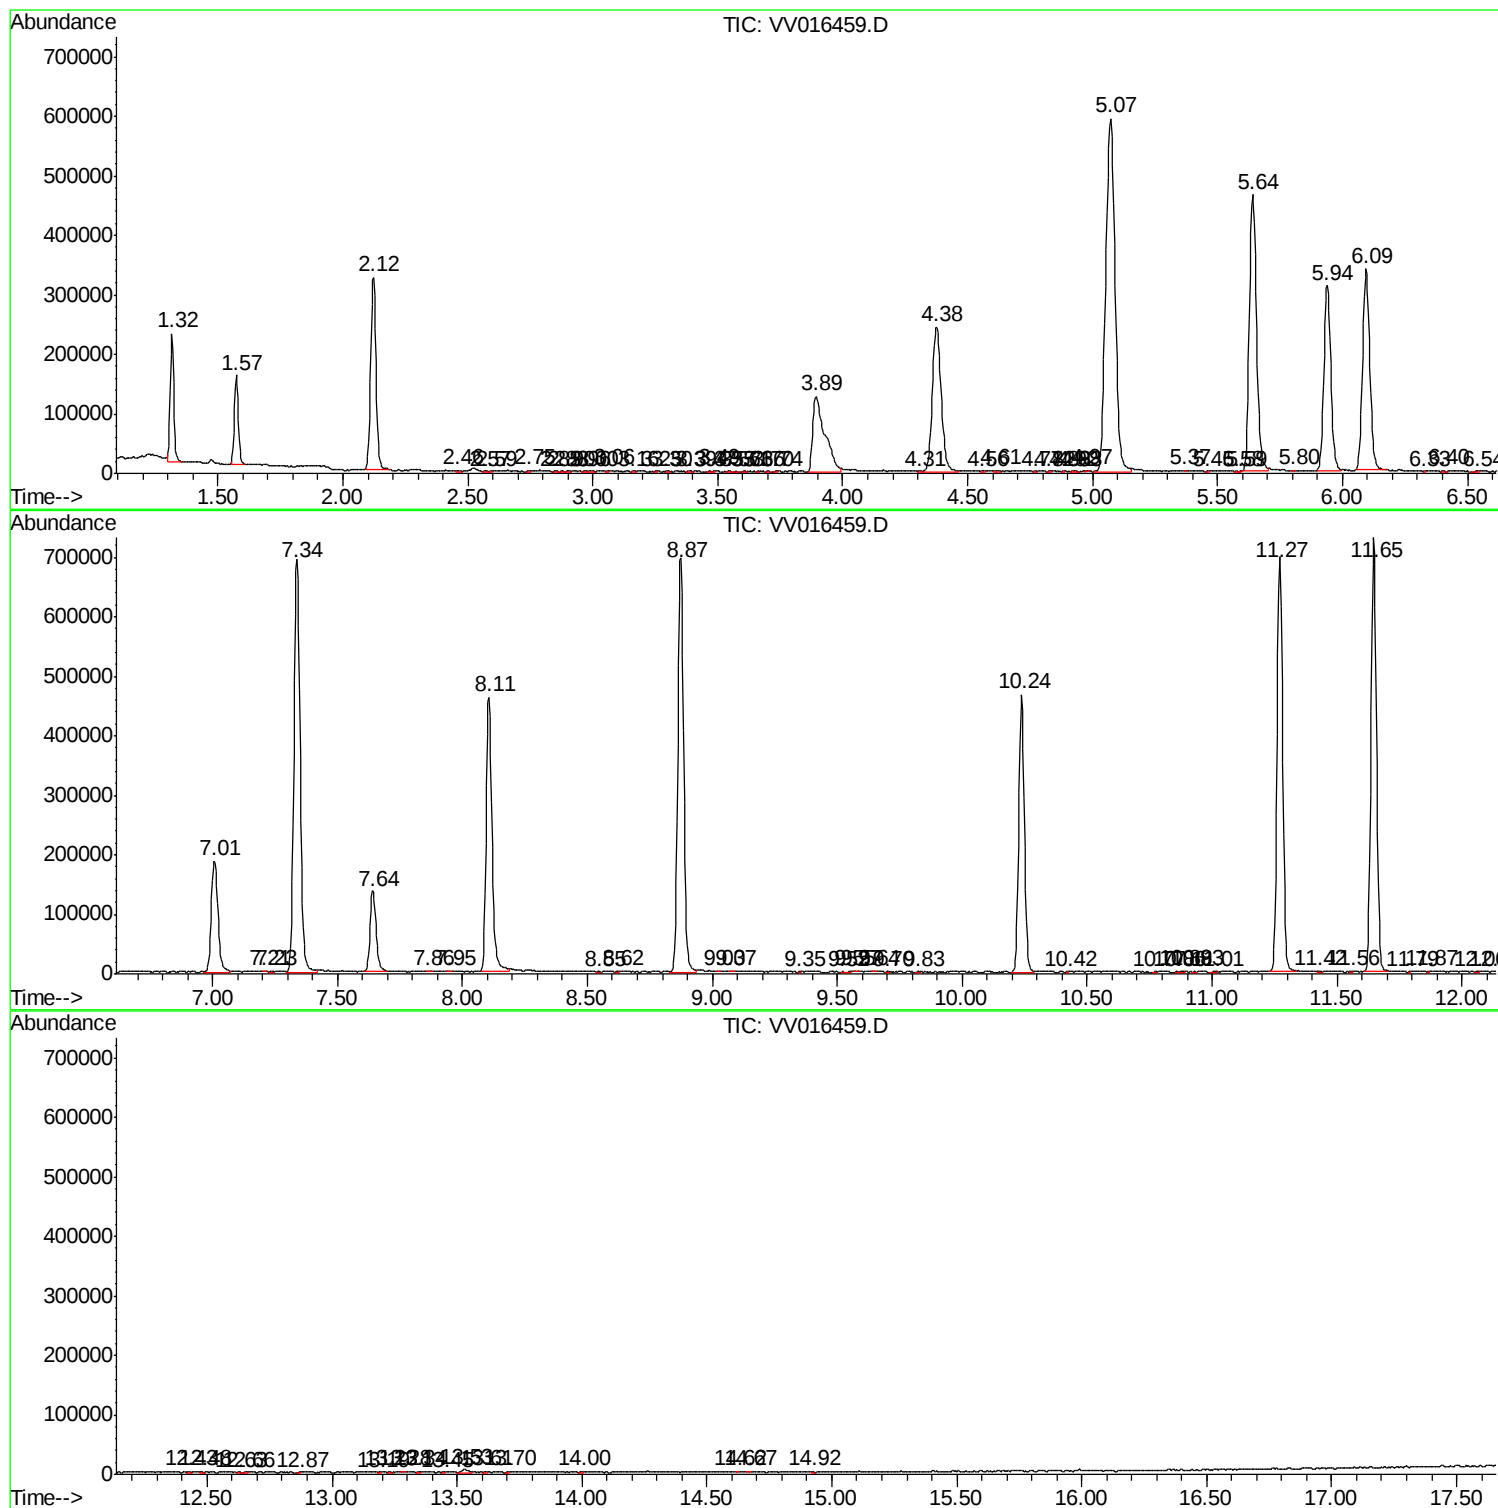

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060320\
Data File : VV016459.D
Acq On : 03 Jun 2020 16:12
Operator : SY/MD
Sample : L2843-02DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA5DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060320\
Data File : VV016459.D
Acq On : 03 Jun 2020 16:12
Operator : SY/MD
Sample : L2843-02DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA5DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc