

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016460.D
 Acq On : 03 Jun 2020 16:35
 Operator : SY/MD
 Sample : L2843-03DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	83	rVB	203754	203240	14.01%	1.509%
2	1.576	144	151	165	rVB	146013	164728	11.36%	1.223%
3	2.123	310	321	343	rBV	306400	460061	31.72%	3.415%
4	2.608	469	472	475	rVB4	1823	943	0.07%	0.007%
5	2.624	475	477	479	rBV3	1026	735	0.05%	0.005%
6	2.926	569	571	574	rVV4	1088	555	0.04%	0.004%
7	3.254	669	673	675	rBV4	1509	1192	0.08%	0.009%
8	3.270	675	678	681	rVV5	1161	680	0.05%	0.005%
9	3.338	697	699	702	rVB4	1029	546	0.04%	0.004%
10	3.354	702	704	706	rBV3	1657	1090	0.08%	0.008%
11	3.537	758	761	762	rBV2	954	539	0.04%	0.004%
12	3.585	773	776	779	rVB4	966	548	0.04%	0.004%
13	3.605	779	782	785	rBV5	1365	687	0.05%	0.005%
14	3.621	785	787	791	rBV5	991	834	0.06%	0.006%
15	3.663	798	800	805	rVB3	989	722	0.05%	0.005%
16	3.698	808	811	813	rBV4	1371	884	0.06%	0.007%
17	3.753	825	828	831	rVV4	1620	1021	0.07%	0.008%
18	3.778	835	836	841	rBV4	1014	733	0.05%	0.005%
19	3.814	845	847	851	rVB3	2402	1322	0.09%	0.010%
20	3.849	855	858	860	rVB3	1182	561	0.04%	0.004%
21	3.936	860	885	909	rBV2	420414	1285901	88.67%	9.546%
22	4.376	1003	1022	1051	rVV	235853	582753	40.18%	4.326%
23	4.749	1134	1138	1139	rBV3	1658	1015	0.07%	0.008%
24	4.769	1142	1144	1148	rVB3	1076	613	0.04%	0.005%
25	4.830	1158	1163	1165	rBV4	1257	1117	0.08%	0.008%
26	4.904	1184	1186	1190	rBV3	1019	685	0.05%	0.005%
27	4.971	1203	1207	1209	rBV4	1186	839	0.06%	0.006%
28	5.007	1216	1218	1220	rBV4	899	537	0.04%	0.004%
29	5.071	1222	1238	1261	rVV2	567555	1450188	100.00%	10.765%
30	5.344	1321	1323	1327	rBV4	1387	946	0.07%	0.007%
31	5.640	1401	1415	1440	rBV	455696	911067	62.82%	6.763%
32	5.939	1494	1508	1535	rBV	715059	1391159	95.93%	10.327%
33	6.093	1542	1556	1575	rBV	326496	657581	45.34%	4.881%
34	6.293	1614	1618	1623	rBV9	1443	1527	0.11%	0.011%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016460.D
 Acq On : 03 Jun 2020 16:35
 Operator : SY/MD
 Sample : L2843-03DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.527	1688	1691	1692	rBV3	1745	896	0.06%	0.007%
36	6.727	1749	1753	1754	rBV3	1820	1160	0.08%	0.009%
37	6.778	1766	1769	1773	rBV5	1906	1501	0.10%	0.011%
38	6.839	1786	1788	1791	rBV4	1216	663	0.05%	0.005%
39	6.917	1810	1812	1814	rBV3	1128	647	0.04%	0.005%
40	7.007	1830	1840	1863	rBV	184531	327658	22.59%	2.432%
41	7.338	1930	1943	1963	rBV	677447	1160753	80.04%	8.617%
42	7.640	2027	2037	2054	rBV	131001	220643	15.21%	1.638%
43	8.026	2155	2157	2159	rBV3	1226	695	0.05%	0.005%
44	8.106	2172	2182	2210	rBV	429305	709848	48.95%	5.269%
45	8.727	2372	2375	2378	rBV5	1240	1062	0.07%	0.008%
46	8.875	2408	2421	2442	rBV	680403	1104577	76.17%	8.199%
47	9.170	2509	2513	2517	rVB6	2433	1758	0.12%	0.013%
48	9.367	2571	2574	2575	rBV4	1365	688	0.05%	0.005%
49	9.482	2607	2610	2614	rBV4	1503	1271	0.09%	0.009%
50	9.531	2622	2625	2626	rBV3	1400	735	0.05%	0.005%
51	9.614	2647	2651	2654	rBV5	1378	985	0.07%	0.007%
52	9.633	2655	2657	2659	rVB3	1978	627	0.04%	0.005%
53	9.733	2686	2688	2692	rVB4	1678	964	0.07%	0.007%
54	9.752	2692	2694	2696	rBV3	985	658	0.05%	0.005%
55	9.785	2701	2704	2711	rBV7	1140	1383	0.10%	0.010%
56	9.849	2721	2724	2727	rBV5	1291	850	0.06%	0.006%
57	9.952	2754	2756	2758	rBV3	1115	661	0.05%	0.005%
58	10.016	2774	2776	2778	rBV3	955	579	0.04%	0.004%
59	10.042	2782	2784	2789	rVV4	1070	634	0.04%	0.005%
60	10.087	2794	2798	2799	rBV5	1028	749	0.05%	0.006%
61	10.096	2799	2801	2804	rVB4	1675	1045	0.07%	0.008%
62	10.129	2808	2811	2812	rBV3	1020	584	0.04%	0.004%
63	10.199	2829	2833	2834	rBV4	1213	843	0.06%	0.006%
64	10.238	2834	2845	2861	rVB	435225	677998	46.75%	5.033%
65	10.392	2891	2893	2894	rBV2	1405	599	0.04%	0.004%
66	10.457	2909	2913	2917	rBV5	1683	1478	0.10%	0.011%
67	10.495	2923	2925	2929	rVB3	1960	1141	0.08%	0.008%
68	10.518	2929	2932	2935	rBV4	1475	1335	0.09%	0.010%
69	10.630	2964	2967	2969	rBV4	1753	1130	0.08%	0.008%
70	10.727	2992	2997	2998	rBV5	1122	710	0.05%	0.005%
71	10.794	3015	3018	3020	rBV3	1383	752	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016460.D
 Acq On : 03 Jun 2020 16:35
 Operator : SY/MD
 Sample : L2843-03DL 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	10.910	3052	3054	3057	rBV4	1133	779	0.05%	0.006%
73	11.138	3122	3125	3128	rVB6	1369	991	0.07%	0.007%
74	11.164	3128	3133	3136	rBV7	1936	1850	0.13%	0.014%
75	11.270	3154	3166	3186	rBV	674155	1032923	71.23%	7.668%
76	11.485	3231	3233	3236	rBV4	1382	914	0.06%	0.007%
77	11.521	3242	3244	3247	rBV3	1311	768	0.05%	0.006%
78	11.646	3269	3283	3300	rBV	672852	1050986	72.47%	7.802%
79	11.858	3347	3349	3353	rVB3	1267	763	0.05%	0.006%
80	12.077	3415	3417	3421	rBV3	998	609	0.04%	0.005%
81	12.138	3434	3436	3440	rVB4	970	669	0.05%	0.005%
82	12.174	3445	3447	3448	rBV2	1371	623	0.04%	0.005%
83	12.264	3472	3475	3480	rVB6	1512	1424	0.10%	0.011%
84	12.305	3486	3488	3492	rVB3	1385	707	0.05%	0.005%
85	12.460	3534	3536	3539	rVB5	1106	579	0.04%	0.004%
86	12.698	3607	3610	3611	rBV3	1029	675	0.05%	0.005%
87	12.977	3695	3697	3699	rBV2	1154	624	0.04%	0.005%
88	13.032	3712	3714	3718	rVB3	1679	1039	0.07%	0.008%
89	13.199	3764	3766	3768	rBV3	1164	562	0.04%	0.004%
90	13.344	3807	3811	3815	rBV6	1786	1653	0.11%	0.012%
91	13.530	3864	3869	3877	rBV6	3742	5081	0.35%	0.038%
92	13.608	3889	3893	3894	rBV4	1108	694	0.05%	0.005%
93	13.775	3941	3945	3947	rBV5	1387	1125	0.08%	0.008%
94	13.894	3980	3982	3984	rBV2	1616	980	0.07%	0.007%
95	14.212	4079	4081	4083	rBV3	1344	802	0.06%	0.006%
96	14.299	4106	4108	4110	rBV3	1420	854	0.06%	0.006%
97	14.778	4254	4257	4259	rBV3	1656	977	0.07%	0.007%
98	14.984	4319	4321	4324	rBV3	1052	758	0.05%	0.006%
99	15.045	4338	4340	4343	rBV2	1513	1101	0.08%	0.008%
100	15.125	4361	4365	4369	rBV5	1945	1955	0.13%	0.015%


Sum of corrected areas: 13471274

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060320\
Data File : VV016460.D
Acq On : 03 Jun 2020 16:35
Operator : SY/MD
Sample : L2843-03DL 10X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

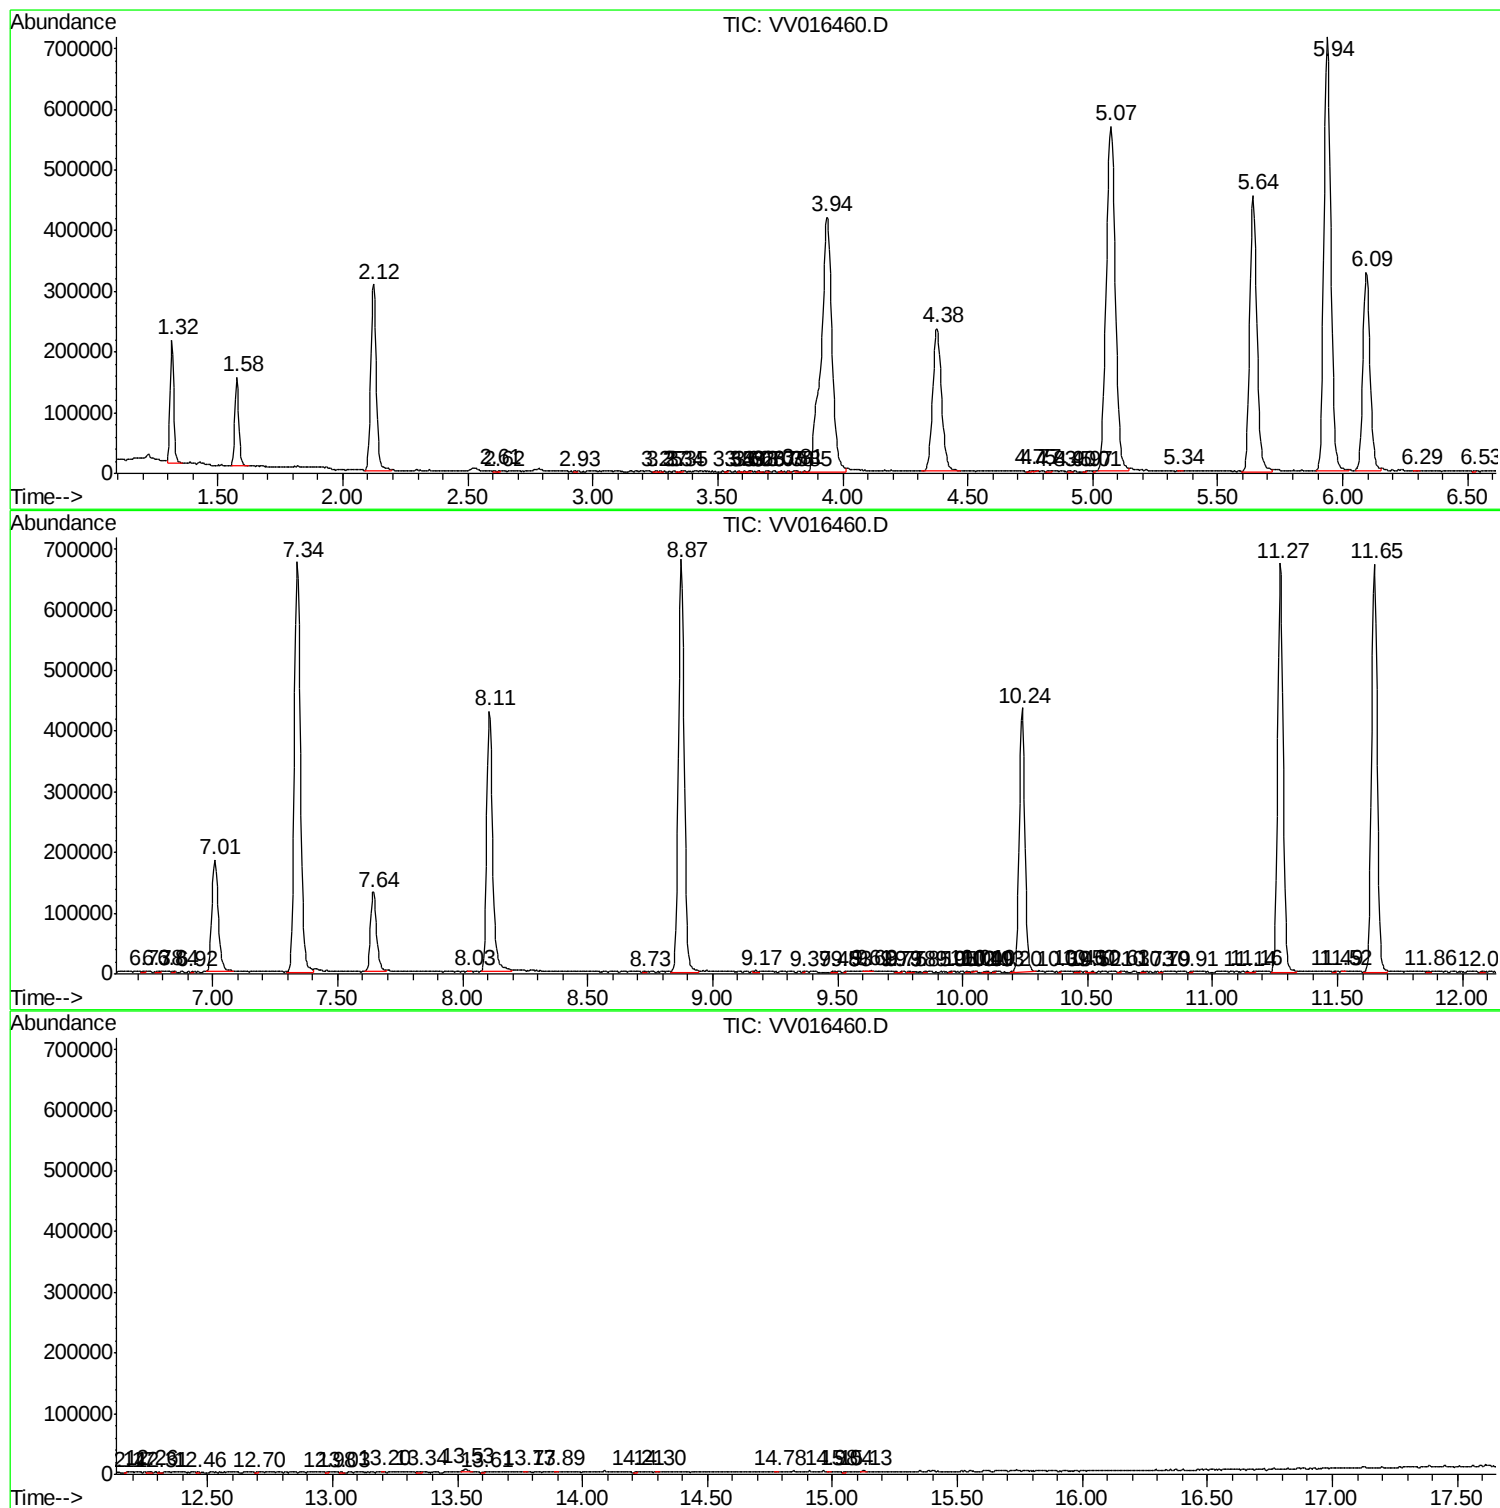

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060320\
Data File : VV016460.D
Acq On : 03 Jun 2020 16:35
Operator : SY/MD
Sample : L2843-03DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV060320\
Data File : VV016460.D
Acq On : 03 Jun 2020 16:35
Operator : SY/MD
Sample : L2843-03DL 10X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0AA6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc