

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016461.D
 Acq On : 03 Jun 2020 16:59
 Operator : SY/MD
 Sample : L2843-04DL 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA7DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	80	rVB	187708	192651	11.98%	1.571%
2	1.573	144	150	162	rVB	130441	153288	9.53%	1.250%
3	2.123	311	321	336	rBV	298952	434869	27.04%	3.546%
4	2.524	439	446	452	rBV5	6386	9843	0.61%	0.080%
5	2.631	476	479	481	rBV4	1460	1100	0.07%	0.009%
6	2.785	518	527	534	rBV4	4060	7597	0.47%	0.062%
7	2.881	555	557	559	rBV3	1178	406	0.03%	0.003%
8	2.933	571	573	580	rVB8	905	679	0.04%	0.006%
9	2.965	580	583	585	rBV3	1537	1135	0.07%	0.009%
10	3.023	599	601	603	rBV3	898	492	0.03%	0.004%
11	3.103	623	626	630	rBV5	903	867	0.05%	0.007%
12	3.129	632	634	636	rVB3	933	317	0.02%	0.003%
13	3.328	694	696	698	rBV2	900	332	0.02%	0.003%
14	3.360	704	706	707	rBV2	818	217	0.01%	0.002%
15	3.376	707	711	713	rBV5	1982	1217	0.08%	0.010%
16	3.463	735	738	739	rBV3	906	516	0.03%	0.004%
17	3.473	739	741	742	rVV2	470	215	0.01%	0.002%
18	3.611	781	784	786	rBV3	1012	715	0.04%	0.006%
19	3.637	791	792	796	rVB4	1066	549	0.03%	0.004%
20	3.653	796	797	799	rBV2	992	333	0.02%	0.003%
21	3.685	804	807	809	rBV3	1458	1151	0.07%	0.009%
22	3.749	825	827	828	rBV2	1075	550	0.03%	0.004%
23	3.811	843	846	848	rBV4	1190	703	0.04%	0.006%
24	3.897	862	873	877	rBV	115840	214363	13.33%	1.748%
25	4.293	994	996	997	rBV2	1044	353	0.02%	0.003%
26	4.376	1008	1022	1043	rVB2	226551	543488	33.79%	4.432%
27	4.582	1084	1086	1087	rBV2	1492	700	0.04%	0.006%
28	4.765	1141	1143	1145	rVB3	1505	511	0.03%	0.004%
29	4.888	1177	1181	1183	rBV3	1303	941	0.06%	0.008%
30	4.929	1192	1194	1196	rVB2	863	402	0.02%	0.003%
31	4.946	1196	1199	1200	rBV3	979	528	0.03%	0.004%
32	5.071	1222	1238	1264	rBV2	548627	1402356	87.19%	11.435%
33	5.640	1402	1415	1437	rBV	443021	888630	55.25%	7.246%
34	5.936	1494	1507	1532	rBV	838153	1608344	100.00%	13.115%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016461.D
 Acq On : 03 Jun 2020 16:59
 Operator : SY/MD
 Sample : L2843-04DL 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA7DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.093	1544	1556	1577	rBV	316842	628193	39.06%	5.122%
36	6.373	1641	1643	1645	rBV2	1036	491	0.03%	0.004%
37	6.640	1723	1726	1727	rBV2	1665	936	0.06%	0.008%
38	6.730	1751	1754	1756	rBV3	1202	773	0.05%	0.006%
39	6.765	1763	1765	1768	rVB4	1219	707	0.04%	0.006%
40	6.920	1811	1813	1816	rVB4	1175	614	0.04%	0.005%
41	7.007	1830	1840	1860	rBV	180579	314174	19.53%	2.562%
42	7.338	1932	1943	1961	rBV	642070	1104793	68.69%	9.009%
43	7.589	2019	2021	2026	rVB6	1590	941	0.06%	0.008%
44	7.643	2028	2038	2060	rVB	126205	215689	13.41%	1.759%
45	7.965	2135	2138	2141	rVB5	1693	926	0.06%	0.008%
46	8.106	2171	2182	2203	rBV	412960	679164	42.23%	5.538%
47	8.582	2327	2330	2335	rVB6	1297	1127	0.07%	0.009%
48	8.611	2336	2339	2344	rVV6	1887	1858	0.12%	0.015%
49	8.746	2379	2381	2383	rBV2	1683	729	0.05%	0.006%
50	8.781	2390	2392	2396	rBV4	1499	817	0.05%	0.007%
51	8.875	2409	2421	2442	rBV	669253	1084222	67.41%	8.841%
52	9.142	2502	2504	2505	rBV2	957	411	0.03%	0.003%
53	9.212	2524	2526	2529	rBV3	1520	874	0.05%	0.007%
54	9.315	2554	2558	2560	rBV4	1168	858	0.05%	0.007%
55	9.344	2566	2567	2570	rBV2	1362	632	0.04%	0.005%
56	9.367	2570	2574	2576	rVV4	1187	1078	0.07%	0.009%
57	9.415	2588	2589	2592	rBV4	1245	841	0.05%	0.007%
58	9.547	2627	2630	2632	rBV4	1299	736	0.05%	0.006%
59	9.563	2633	2635	2639	rVV5	1333	1056	0.07%	0.009%
60	9.601	2643	2647	2650	rBV5	1644	1601	0.10%	0.013%
61	9.717	2679	2683	2685	rBV4	2037	1432	0.09%	0.012%
62	9.762	2693	2697	2699	rBV3	1417	888	0.06%	0.007%
63	9.830	2716	2718	2720	rBV3	1242	640	0.04%	0.005%
64	9.894	2736	2738	2742	rVB3	1157	647	0.04%	0.005%
65	10.084	2795	2797	2798	rBV	1305	488	0.03%	0.004%
66	10.238	2834	2845	2859	rBV	428113	658669	40.95%	5.371%
67	10.418	2899	2901	2904	rVB3	1516	808	0.05%	0.007%
68	10.444	2904	2909	2915	rBV	10755	8259	0.51%	0.067%
69	10.473	2916	2918	2920	rVV2	981	443	0.03%	0.004%
70	10.955	3066	3068	3071	rBV4	1332	677	0.04%	0.006%
71	11.058	3097	3100	3102	rBV4	1443	908	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016461.D
 Acq On : 03 Jun 2020 16:59
 Operator : SY/MD
 Sample : L2843-04DL 20X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA7DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	11.090	3108	3110	3112	rBV3	1108	537	0.03%	0.004%
73	11.151	3127	3129	3133	rBV6	1032	665	0.04%	0.005%
74	11.270	3155	3166	3188	rVB	660453	1016402	63.20%	8.288%
75	11.563	3254	3257	3258	rBV3	807	475	0.03%	0.004%
76	11.646	3271	3283	3305	rVB	673557	1043560	64.88%	8.509%
77	11.775	3320	3323	3324	rBV3	1907	961	0.06%	0.008%
78	11.875	3351	3354	3357	rVB5	1488	959	0.06%	0.008%
79	11.929	3369	3371	3372	rBV2	961	404	0.03%	0.003%
80	12.042	3403	3406	3409	rBV4	1312	867	0.05%	0.007%
81	12.129	3430	3433	3436	rBV3	1320	1104	0.07%	0.009%
82	12.244	3467	3469	3470	rBV2	718	185	0.01%	0.002%
83	12.299	3485	3486	3488	rBV	628	307	0.02%	0.003%
84	12.344	3498	3500	3501	rBV2	1003	277	0.02%	0.002%
85	12.431	3522	3527	3528	rBV3	1203	1036	0.06%	0.008%
86	12.466	3534	3538	3540	rBV4	747	509	0.03%	0.004%
87	12.678	3599	3604	3605	rBV5	1428	1269	0.08%	0.010%
88	12.720	3614	3617	3621	rBV6	1192	1175	0.07%	0.010%
89	12.784	3634	3637	3639	rBV3	1347	705	0.04%	0.006%
90	13.064	3722	3724	3727	rBV3	1774	1095	0.07%	0.009%
91	13.238	3776	3778	3779	rBV2	797	301	0.02%	0.002%
92	13.273	3788	3789	3791	rBV2	1197	638	0.04%	0.005%
93	13.897	3979	3983	3986	rBV4	1910	1639	0.10%	0.013%


Sum of corrected areas: 12263528

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060320\
Data File : VV016461.D
Acq On : 03 Jun 2020 16:59
Operator : SY/MD
Sample : L2843-04DL 20X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA7DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

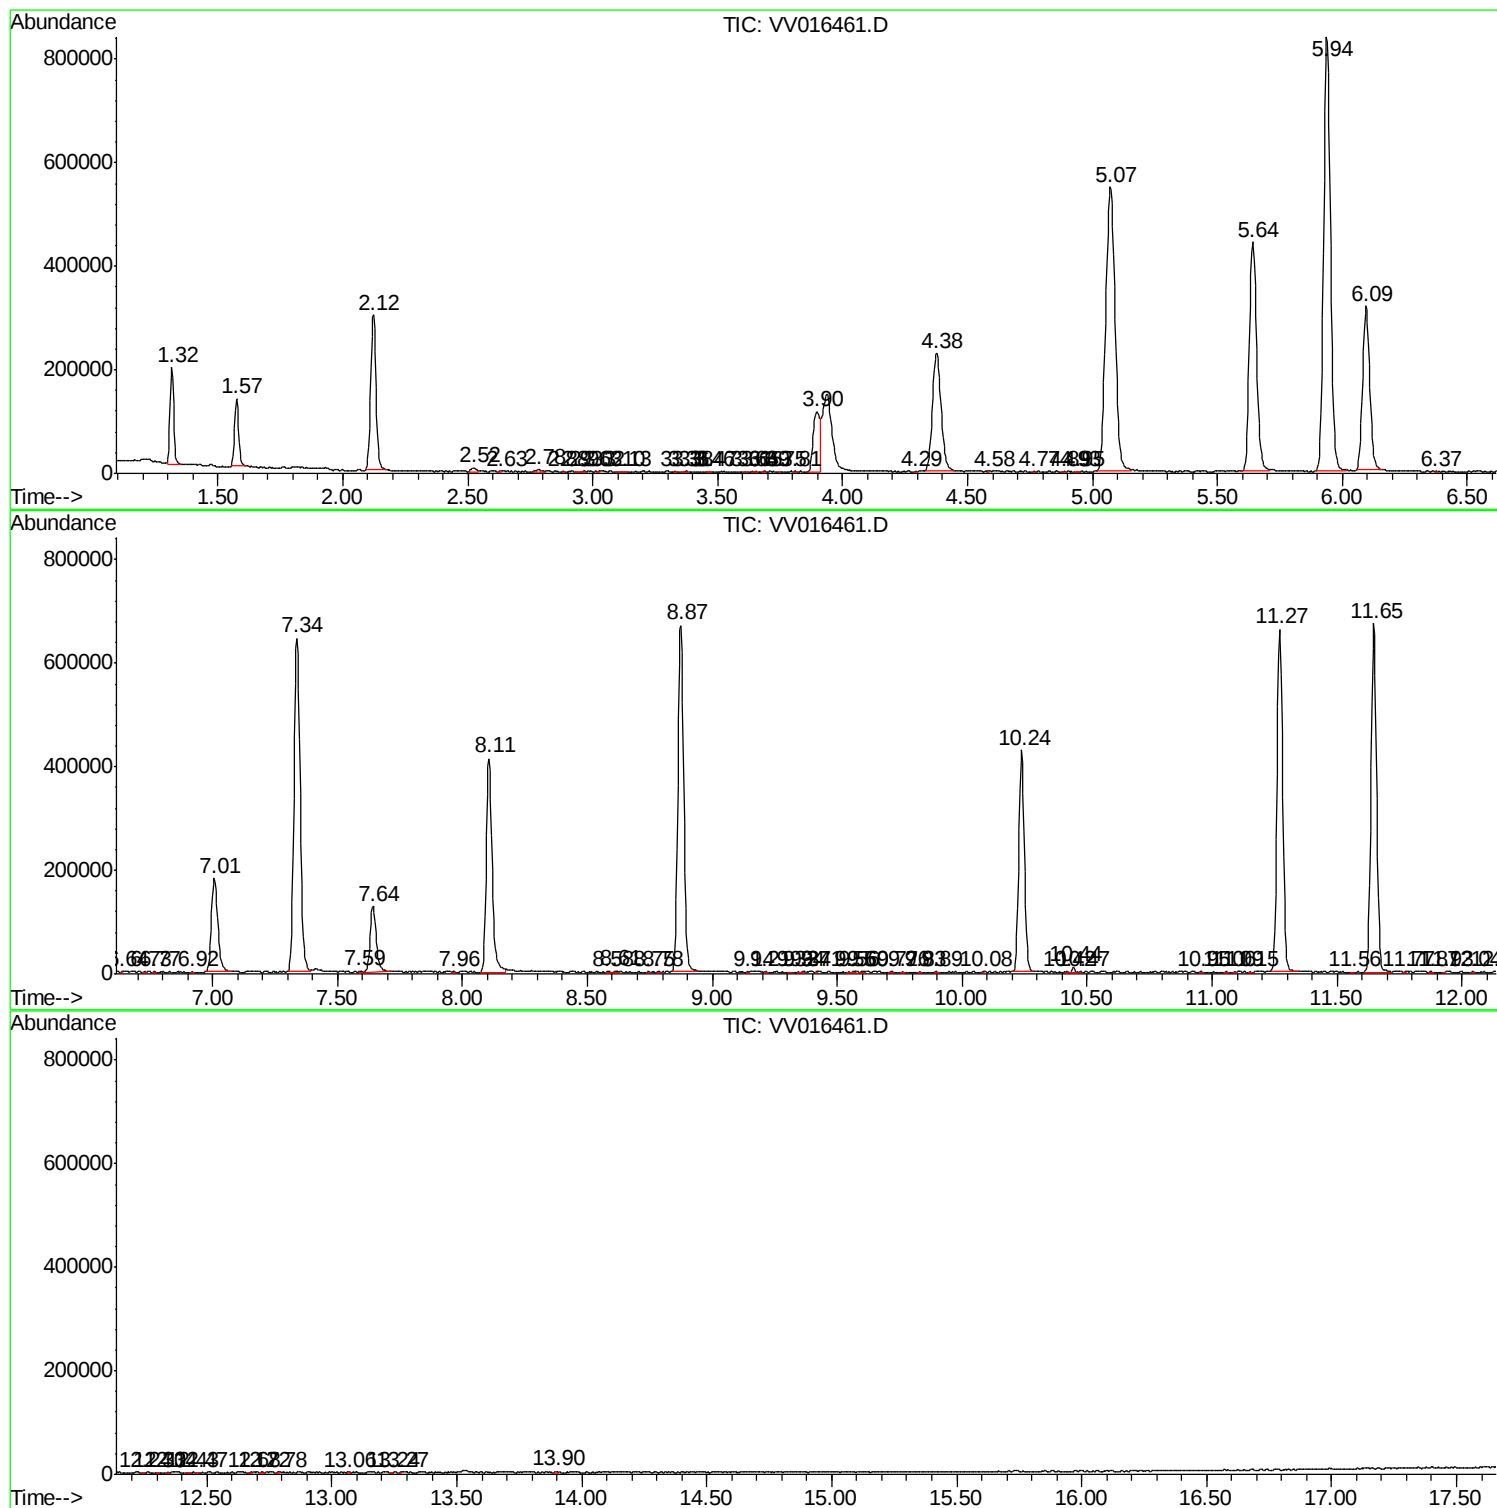

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060320\
Data File : VV016461.D
Acq On : 03 Jun 2020 16:59
Operator : SY/MD
Sample : L2843-04DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA7DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV060320\
Data File : VV016461.D
Acq On : 03 Jun 2020 16:59
Operator : SY/MD
Sample : L2843-04DL 20X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0AA7DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc