

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016463.D
 Acq On : 03 Jun 2020 17:46
 Operator : SY/MD
 Sample : L2843-06DL 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB0DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	65	70	81	rVB	196169	201684	13.95%	1.775%
2	1.573	144	150	163	rVB	138418	160427	11.09%	1.412%
3	2.122	310	321	337	rBV	306287	455468	31.49%	4.009%
4	2.524	440	446	456	rVB3	9206	13794	0.95%	0.121%
5	2.704	500	502	506	rVB4	1270	566	0.04%	0.005%
6	2.759	516	519	520	rBV3	1399	721	0.05%	0.006%
7	2.997	591	593	599	rBV4	1743	1323	0.09%	0.012%
8	3.061	611	613	615	rBV2	1378	695	0.05%	0.006%
9	3.251	668	672	674	rBV4	1387	982	0.07%	0.009%
10	3.286	680	683	688	rVB7	1318	1149	0.08%	0.010%
11	3.511	751	753	757	rVB3	1713	1042	0.07%	0.009%
12	3.547	757	764	769	rBV9	1377	2040	0.14%	0.018%
13	3.798	837	842	846	rVV7	1298	1271	0.09%	0.011%
14	3.843	853	856	858	rVB4	1008	562	0.04%	0.005%
15	3.894	862	872	877	rBV	118332	226752	15.68%	1.996%
16	4.251	981	983	985	rBV2	1341	644	0.04%	0.006%
17	4.283	989	993	994	rBV3	1122	706	0.05%	0.006%
18	4.376	1004	1022	1044	rBV	232579	569505	39.38%	5.012%
19	4.544	1072	1074	1078	rVB4	1648	1251	0.09%	0.011%
20	4.566	1078	1081	1083	rBV4	1145	624	0.04%	0.005%
21	4.627	1098	1100	1104	rBV4	1254	1056	0.07%	0.009%
22	4.733	1130	1133	1135	rVB4	1063	629	0.04%	0.006%
23	4.753	1135	1139	1141	rVB4	1770	1134	0.08%	0.010%
24	4.769	1141	1144	1148	rBV6	1196	1307	0.09%	0.012%
25	4.814	1155	1158	1160	rVB4	1427	938	0.06%	0.008%
26	4.830	1160	1163	1165	rBV4	1686	1034	0.07%	0.009%
27	4.949	1196	1200	1202	rBV4	898	662	0.05%	0.006%
28	5.071	1219	1238	1268	rBV2	558867	1446171	100.00%	12.728%
29	5.322	1314	1316	1317	rBV2	1239	600	0.04%	0.005%
30	5.595	1398	1401	1402	rBV3	1299	595	0.04%	0.005%
31	5.640	1402	1415	1443	rVV	462452	923209	63.84%	8.125%
32	5.839	1475	1477	1480	rBV3	1168	757	0.05%	0.007%
33	5.939	1495	1508	1525	rBV	159814	318122	22.00%	2.800%
34	6.093	1544	1556	1580	rVB	320735	645913	44.66%	5.685%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016463.D
 Acq On : 03 Jun 2020 17:46
 Operator : SY/MD
 Sample : L2843-06DL 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB0DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.447	1663	1666	1667	rBV2	1389	794	0.05%	0.007%
36	6.791	1767	1773	1775	rBV6	1502	1444	0.10%	0.013%
37	6.878	1798	1800	1803	rBV3	911	617	0.04%	0.005%
38	6.913	1807	1811	1812	rBV3	894	617	0.04%	0.005%
39	7.007	1828	1840	1856	rBV	178472	323473	22.37%	2.847%
40	7.148	1882	1884	1886	rBV3	1566	984	0.07%	0.009%
41	7.180	1891	1894	1897	rVV3	2731	1726	0.12%	0.015%
42	7.216	1901	1905	1909	rBV6	1576	1482	0.10%	0.013%
43	7.338	1929	1943	1965	rBV	673523	1145330	79.20%	10.080%
44	7.479	1981	1987	1995	rBV	2495	3701	0.26%	0.033%
45	7.643	2024	2038	2053	rBV	127534	221483	15.32%	1.949%
46	7.987	2143	2145	2149	rVB4	1483	746	0.05%	0.007%
47	8.106	2171	2182	2203	rBV	419044	694153	48.00%	6.109%
48	8.431	2279	2283	2288	rBV6	2163	2435	0.17%	0.021%
49	8.479	2295	2298	2301	rBV4	1554	1003	0.07%	0.009%
50	8.498	2301	2304	2306	rVV4	1241	675	0.05%	0.006%
51	8.531	2312	2314	2316	rBV3	1126	660	0.05%	0.006%
52	8.569	2322	2326	2329	rBV6	735	748	0.05%	0.007%
53	8.614	2338	2340	2343	rVB4	980	674	0.05%	0.006%
54	8.733	2373	2377	2381	rBV7	1756	1379	0.10%	0.012%
55	8.762	2381	2386	2388	rBV6	1671	1437	0.10%	0.013%
56	8.875	2409	2421	2442	rBV	701028	1124525	77.76%	9.897%
57	9.289	2546	2550	2551	rBV3	1413	931	0.06%	0.008%
58	9.338	2562	2565	2569	rBV5	1061	780	0.05%	0.007%
59	9.727	2684	2686	2689	rVB3	1225	637	0.04%	0.006%
60	9.797	2704	2708	2716	rVB8	1455	2053	0.14%	0.018%
61	9.846	2720	2723	2724	rBV2	1304	786	0.05%	0.007%
62	9.878	2731	2733	2735	rBV3	1251	590	0.04%	0.005%
63	10.068	2790	2792	2795	rBV4	1479	739	0.05%	0.007%
64	10.148	2813	2817	2819	rBV3	1332	1034	0.07%	0.009%
65	10.238	2832	2845	2859	rBV	434579	683491	47.26%	6.016%
66	10.402	2893	2896	2900	rBV4	1700	1227	0.08%	0.011%
67	10.489	2918	2923	2927	rVB5	1731	1785	0.12%	0.016%
68	10.518	2929	2932	2934	rBV4	1147	765	0.05%	0.007%
69	10.553	2942	2943	2949	rVB6	1479	1404	0.10%	0.012%
70	10.666	2976	2978	2980	rBV3	1273	713	0.05%	0.006%
71	10.846	3032	3034	3037	rVB3	1551	853	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016463.D
 Acq On : 03 Jun 2020 17:46
 Operator : SY/MD
 Sample : L2843-06DL 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB0DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	10.868	3037	3041	3044	rBV5	2425	2418	0.17%	0.021%
73	10.900	3049	3051	3055	rBV4	1543	1255	0.09%	0.011%
74	11.019	3086	3088	3090	rBV3	1138	668	0.05%	0.006%
75	11.064	3100	3102	3105	rVB3	1069	571	0.04%	0.005%
76	11.180	3135	3138	3139	rBV3	1300	655	0.05%	0.006%
77	11.270	3155	3166	3185	rBV	710760	1070258	74.01%	9.420%
78	11.450	3220	3222	3226	rVB5	1685	979	0.07%	0.009%
79	11.473	3226	3229	3232	rBV5	871	616	0.04%	0.005%
80	11.521	3242	3244	3247	rVB4	1274	616	0.04%	0.005%
81	11.537	3247	3249	3252	rBV3	1495	1049	0.07%	0.009%
82	11.646	3272	3283	3297	rBV	679014	1054158	72.89%	9.278%
83	11.936	3369	3373	3379	rVB8	945	843	0.06%	0.007%
84	12.116	3424	3429	3432	rBV7	1205	1094	0.08%	0.010%
85	12.141	3435	3437	3442	rVB4	2278	1214	0.08%	0.011%
86	12.309	3484	3489	3495	rBV8	1203	1274	0.09%	0.011%
87	12.338	3495	3498	3502	rVB5	1497	926	0.06%	0.008%
88	12.366	3502	3507	3508	rBV3	1501	1086	0.08%	0.010%
89	12.434	3526	3528	3532	rBV5	1231	884	0.06%	0.008%
90	12.479	3540	3542	3545	rBV4	1230	675	0.05%	0.006%
91	12.710	3609	3614	3619	rBV9	1905	2326	0.16%	0.020%
92	12.868	3660	3663	3666	rBV4	1452	1053	0.07%	0.009%
93	12.942	3683	3686	3691	rBV6	1056	892	0.06%	0.008%
94	13.000	3702	3704	3707	rBV4	1427	842	0.06%	0.007%
95	13.177	3755	3759	3761	rBV5	967	755	0.05%	0.007%
96	13.260	3782	3785	3787	rBV4	1094	786	0.05%	0.007%
97	13.354	3812	3814	3817	rBV3	1382	774	0.05%	0.007%
98	13.611	3890	3894	3895	rBV4	796	616	0.04%	0.005%
99	13.984	4008	4010	4013	rBV3	1128	604	0.04%	0.005%
100	15.157	4373	4375	4377	rBV2	1408	811	0.06%	0.007%


Sum of corrected areas: 11361905

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060320\
Data File : VV016463.D
Acq On : 03 Jun 2020 17:46
Operator : SY/MD
Sample : L2843-06DL 40X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB0DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

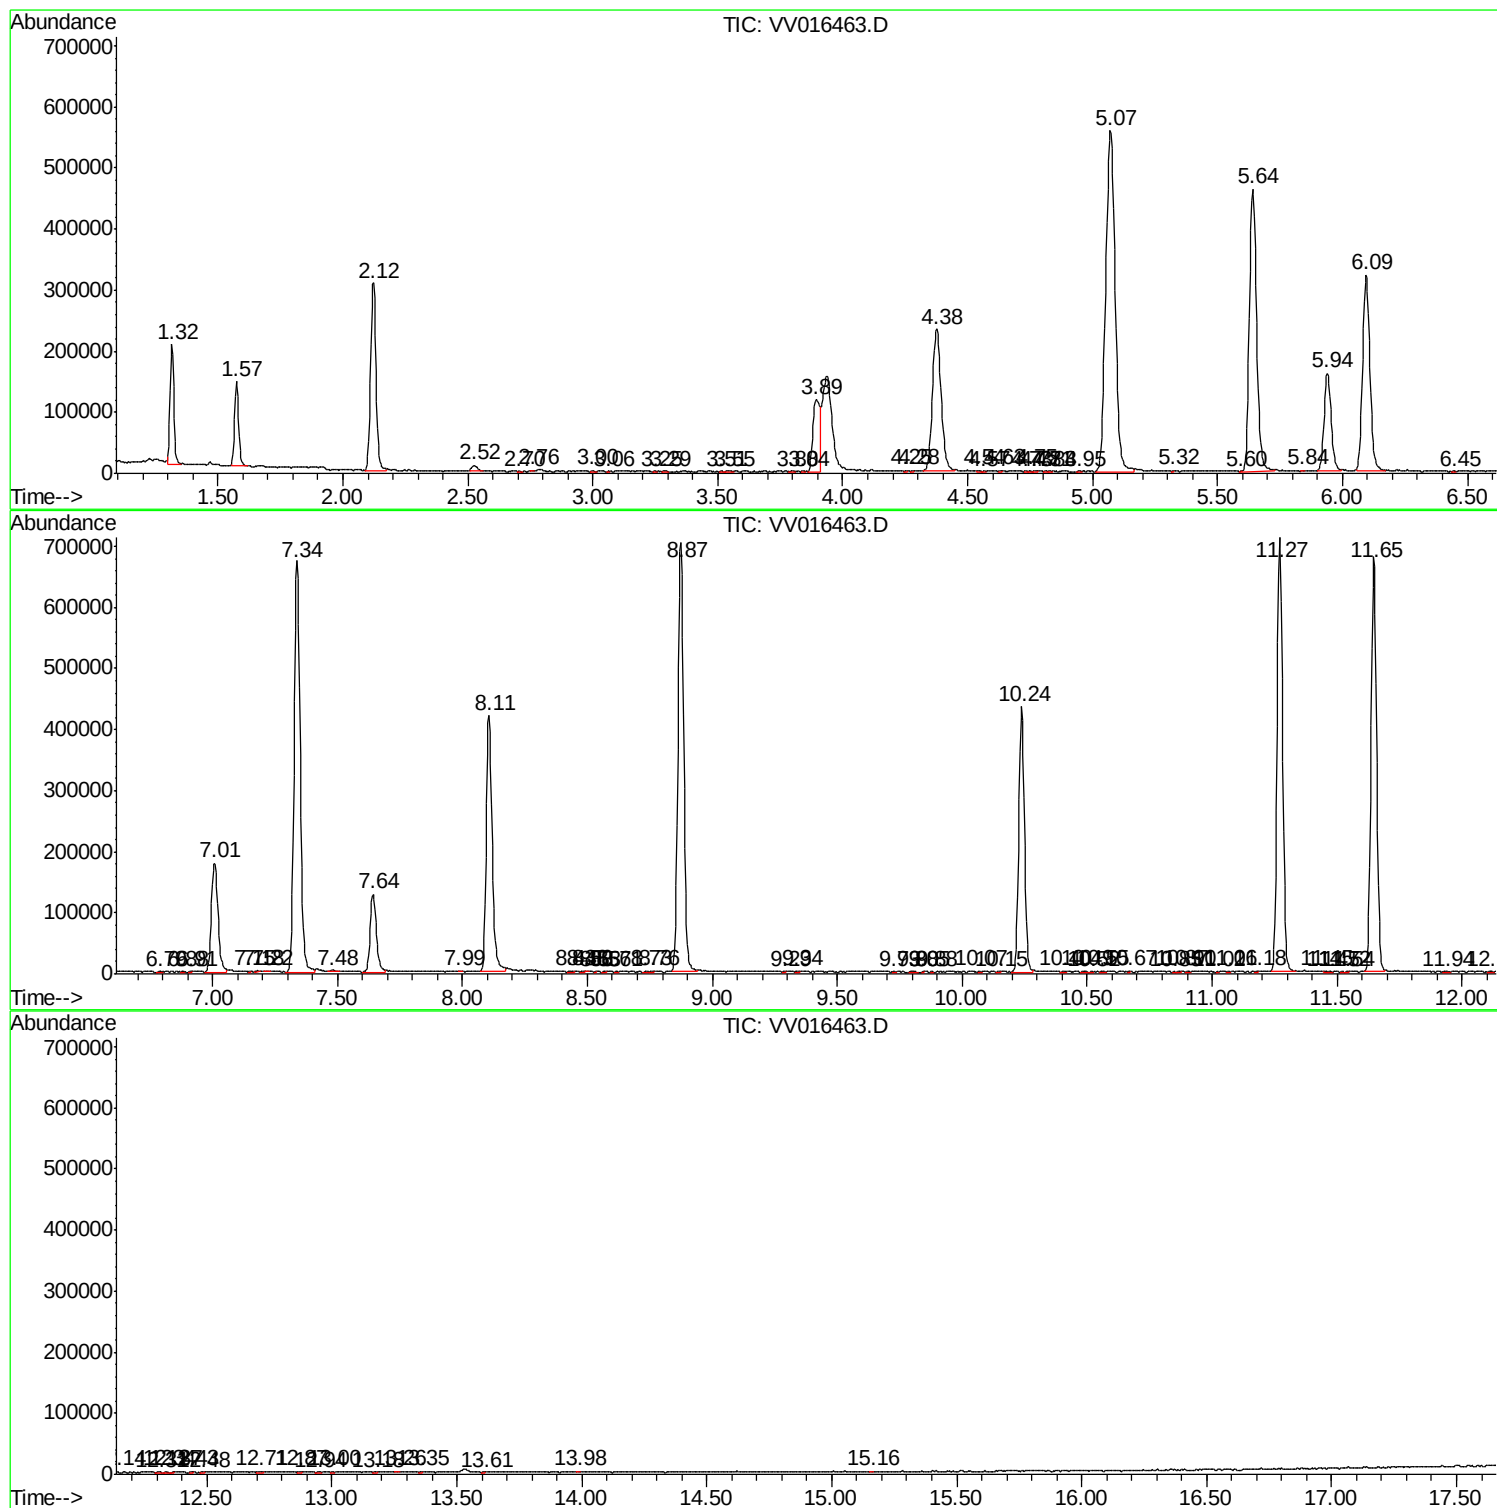

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060320\
Data File : VV016463.D
Acq On : 03 Jun 2020 17:46
Operator : SY/MD
Sample : L2843-06DL 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB0DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV060320\
Data File : VV016463.D
Acq On : 03 Jun 2020 17:46
Operator : SY/MD
Sample : L2843-06DL 40X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0AB0DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc