

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016464.D
 Acq On : 03 Jun 2020 18:10
 Operator : SY/MD
 Sample : L2843-07DL 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB1DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	81	rVB	189243	193618	13.71%	1.708%
2	1.576	144	151	165	rVB	137463	157742	11.17%	1.391%
3	2.122	311	321	337	rBV	297354	434729	30.78%	3.835%
4	2.251	359	361	363	rBV3	1540	726	0.05%	0.006%
5	2.653	483	486	488	rBV3	1197	888	0.06%	0.008%
6	2.736	511	512	515	rBV	1451	734	0.05%	0.006%
7	2.949	574	578	582	rBV7	1555	1334	0.09%	0.012%
8	3.042	603	607	609	rBV4	1585	1359	0.10%	0.012%
9	3.126	631	633	637	rVB4	1522	954	0.07%	0.008%
10	3.206	653	658	659	rBV4	1619	849	0.06%	0.007%
11	3.254	669	673	677	rBV5	951	847	0.06%	0.007%
12	3.408	717	721	723	rBV4	1492	881	0.06%	0.008%
13	3.441	726	731	732	rBV4	1242	933	0.07%	0.008%
14	3.450	732	734	741	rVB6	1275	1008	0.07%	0.009%
15	3.479	741	743	746	rBV4	1156	779	0.06%	0.007%
16	3.518	752	755	759	rBV5	1101	837	0.06%	0.007%
17	3.540	760	762	766	rVB4	1685	963	0.07%	0.008%
18	3.595	777	779	783	rVB4	2117	1472	0.10%	0.013%
19	3.727	815	820	822	rBV5	1396	1174	0.08%	0.010%
20	3.769	830	833	836	rBV4	1062	692	0.05%	0.006%
21	3.897	862	873	877	rBV	118064	221255	15.67%	1.952%
22	4.273	988	990	995	rBV4	1133	738	0.05%	0.007%
23	4.376	1005	1022	1049	rBV	230668	564721	39.98%	4.981%
24	4.650	1104	1107	1110	rBV6	1640	1184	0.08%	0.010%
25	4.691	1118	1120	1122	rBV3	1917	945	0.07%	0.008%
26	4.855	1167	1171	1175	rBV6	1824	1447	0.10%	0.013%
27	4.945	1197	1199	1203	rVV3	1386	1073	0.08%	0.009%
28	4.968	1203	1206	1207	rVV3	1208	876	0.06%	0.008%
29	5.071	1221	1238	1263	rBV2	550730	1412376	100.00%	12.458%
30	5.486	1365	1367	1369	rBV3	1383	752	0.05%	0.007%
31	5.576	1393	1395	1400	rVB5	1712	1145	0.08%	0.010%
32	5.640	1400	1415	1439	rBV	444547	888299	62.89%	7.835%
33	5.887	1488	1492	1494	rBV6	1173	943	0.07%	0.008%
34	5.939	1495	1508	1526	rVV2	287125	565502	40.04%	4.988%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016464.D
 Acq On : 03 Jun 2020 18:10
 Operator : SY/MD
 Sample : L2843-07DL 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB1DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.093	1543	1556	1579	rBV	316852	641876	45.45%	5.662%
36	6.305	1620	1622	1625	rVB4	1450	803	0.06%	0.007%
37	6.328	1625	1629	1631	rBV4	1785	1090	0.08%	0.010%
38	6.370	1639	1642	1644	rBV3	1087	814	0.06%	0.007%
39	6.434	1659	1662	1666	rBV5	1179	953	0.07%	0.008%
40	6.511	1684	1686	1691	rVB5	1293	881	0.06%	0.008%
41	6.614	1714	1718	1722	rBV6	1462	1486	0.11%	0.013%
42	6.730	1751	1754	1757	rVV6	1182	739	0.05%	0.007%
43	6.785	1767	1771	1775	rVB6	1195	998	0.07%	0.009%
44	6.804	1775	1777	1779	rBV3	1452	802	0.06%	0.007%
45	6.884	1798	1802	1803	rBV3	1529	816	0.06%	0.007%
46	7.006	1827	1840	1857	rBV	176120	319991	22.66%	2.822%
47	7.148	1882	1884	1888	rVV4	1424	938	0.07%	0.008%
48	7.289	1925	1928	1931	rBV4	861	672	0.05%	0.006%
49	7.338	1931	1943	1961	rBV	660586	1122930	79.51%	9.905%
50	7.640	2026	2037	2051	rBV	127654	212587	15.05%	1.875%
51	7.974	2139	2141	2143	rBV2	1159	743	0.05%	0.007%
52	7.990	2143	2146	2154	rVV9	2135	2253	0.16%	0.020%
53	8.106	2171	2182	2206	rBV	417879	696105	49.29%	6.140%
54	8.437	2280	2285	2287	rBV3	1720	1611	0.11%	0.014%
55	8.547	2317	2319	2322	rBV4	1335	724	0.05%	0.006%
56	8.874	2409	2421	2441	rBV	663845	1070941	75.83%	9.446%
57	9.022	2465	2467	2470	rBV3	1613	804	0.06%	0.007%
58	9.257	2536	2540	2543	rVB6	1761	1070	0.08%	0.009%
59	9.437	2590	2596	2599	rBV7	1365	1360	0.10%	0.012%
60	9.498	2611	2615	2618	rBV5	1203	1010	0.07%	0.009%
61	9.546	2627	2630	2631	rBV2	1405	833	0.06%	0.007%
62	9.788	2701	2705	2709	rBV7	1584	1616	0.11%	0.014%
63	9.900	2738	2740	2743	rVB4	1190	689	0.05%	0.006%
64	9.932	2743	2750	2751	rBV5	1246	1017	0.07%	0.009%
65	10.035	2780	2782	2785	rBV3	1109	729	0.05%	0.006%
66	10.051	2785	2787	2791	rVV3	1475	999	0.07%	0.009%
67	10.128	2809	2811	2813	rBV3	1668	751	0.05%	0.007%
68	10.167	2820	2823	2829	rVB6	1514	1321	0.09%	0.012%
69	10.238	2829	2845	2862	rBV	432253	676757	47.92%	5.969%
70	10.337	2874	2876	2882	rVB6	1891	1203	0.09%	0.011%
71	10.382	2886	2890	2894	rBV6	1747	1745	0.12%	0.015%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016464.D
 Acq On : 03 Jun 2020 18:10
 Operator : SY/MD
 Sample : L2843-07DL 40X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB1DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	10.440	2906	2908	2911	rBV3	1844	793	0.06%	0.007%
73	10.479	2917	2920	2923	rBV5	1485	1126	0.08%	0.010%
74	10.492	2923	2924	2930	rVB5	1199	764	0.05%	0.007%
75	10.614	2960	2962	2967	rBV4	1364	1072	0.08%	0.009%
76	10.701	2985	2989	2991	rBV4	1016	843	0.06%	0.007%
77	10.800	3013	3020	3022	rBV6	1176	1411	0.10%	0.012%
78	10.865	3037	3040	3042	rBV4	1423	873	0.06%	0.008%
79	10.878	3042	3044	3048	rVV3	1704	987	0.07%	0.009%
80	11.116	3114	3118	3121	rBV5	1567	1598	0.11%	0.014%
81	11.177	3134	3137	3138	rBV3	1393	852	0.06%	0.008%
82	11.270	3154	3166	3188	rVV	667257	1026369	72.67%	9.053%
83	11.521	3239	3244	3248	rBV6	1436	1452	0.10%	0.013%
84	11.566	3255	3258	3259	rBV3	1880	1009	0.07%	0.009%
85	11.646	3271	3283	3299	rBV	668273	1046032	74.06%	9.226%
86	11.858	3345	3349	3352	rBV4	1057	724	0.05%	0.006%
87	12.157	3439	3442	3444	rBV4	1008	772	0.05%	0.007%
88	12.466	3536	3538	3541	rVB3	1627	850	0.06%	0.007%
89	12.572	3568	3571	3574	rBV4	1584	1046	0.07%	0.009%
90	12.601	3578	3580	3585	rVB5	1380	941	0.07%	0.008%
91	12.813	3643	3646	3648	rBV4	1526	687	0.05%	0.006%
92	13.321	3802	3804	3809	rVB4	1467	950	0.07%	0.008%
93	13.424	3833	3836	3841	rBV6	1722	1718	0.12%	0.015%
94	13.517	3862	3865	3866	rBV3	2860	1561	0.11%	0.014%
95	13.836	3961	3964	3965	rBV	1383	828	0.06%	0.007%
96	14.112	4046	4050	4054	rBV4	1778	1815	0.13%	0.016%
97	14.157	4063	4064	4068	rBV4	1103	685	0.05%	0.006%
98	14.228	4081	4086	4088	rBV4	1619	1226	0.09%	0.011%
99	14.514	4172	4175	4179	rBV5	1203	1054	0.07%	0.009%
100	14.585	4194	4197	4199	rVB4	1727	795	0.06%	0.007%


Sum of corrected areas: 11337265

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060320\
Data File : VV016464.D
Acq On : 03 Jun 2020 18:10
Operator : SY/MD
Sample : L2843-07DL 40X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB1DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

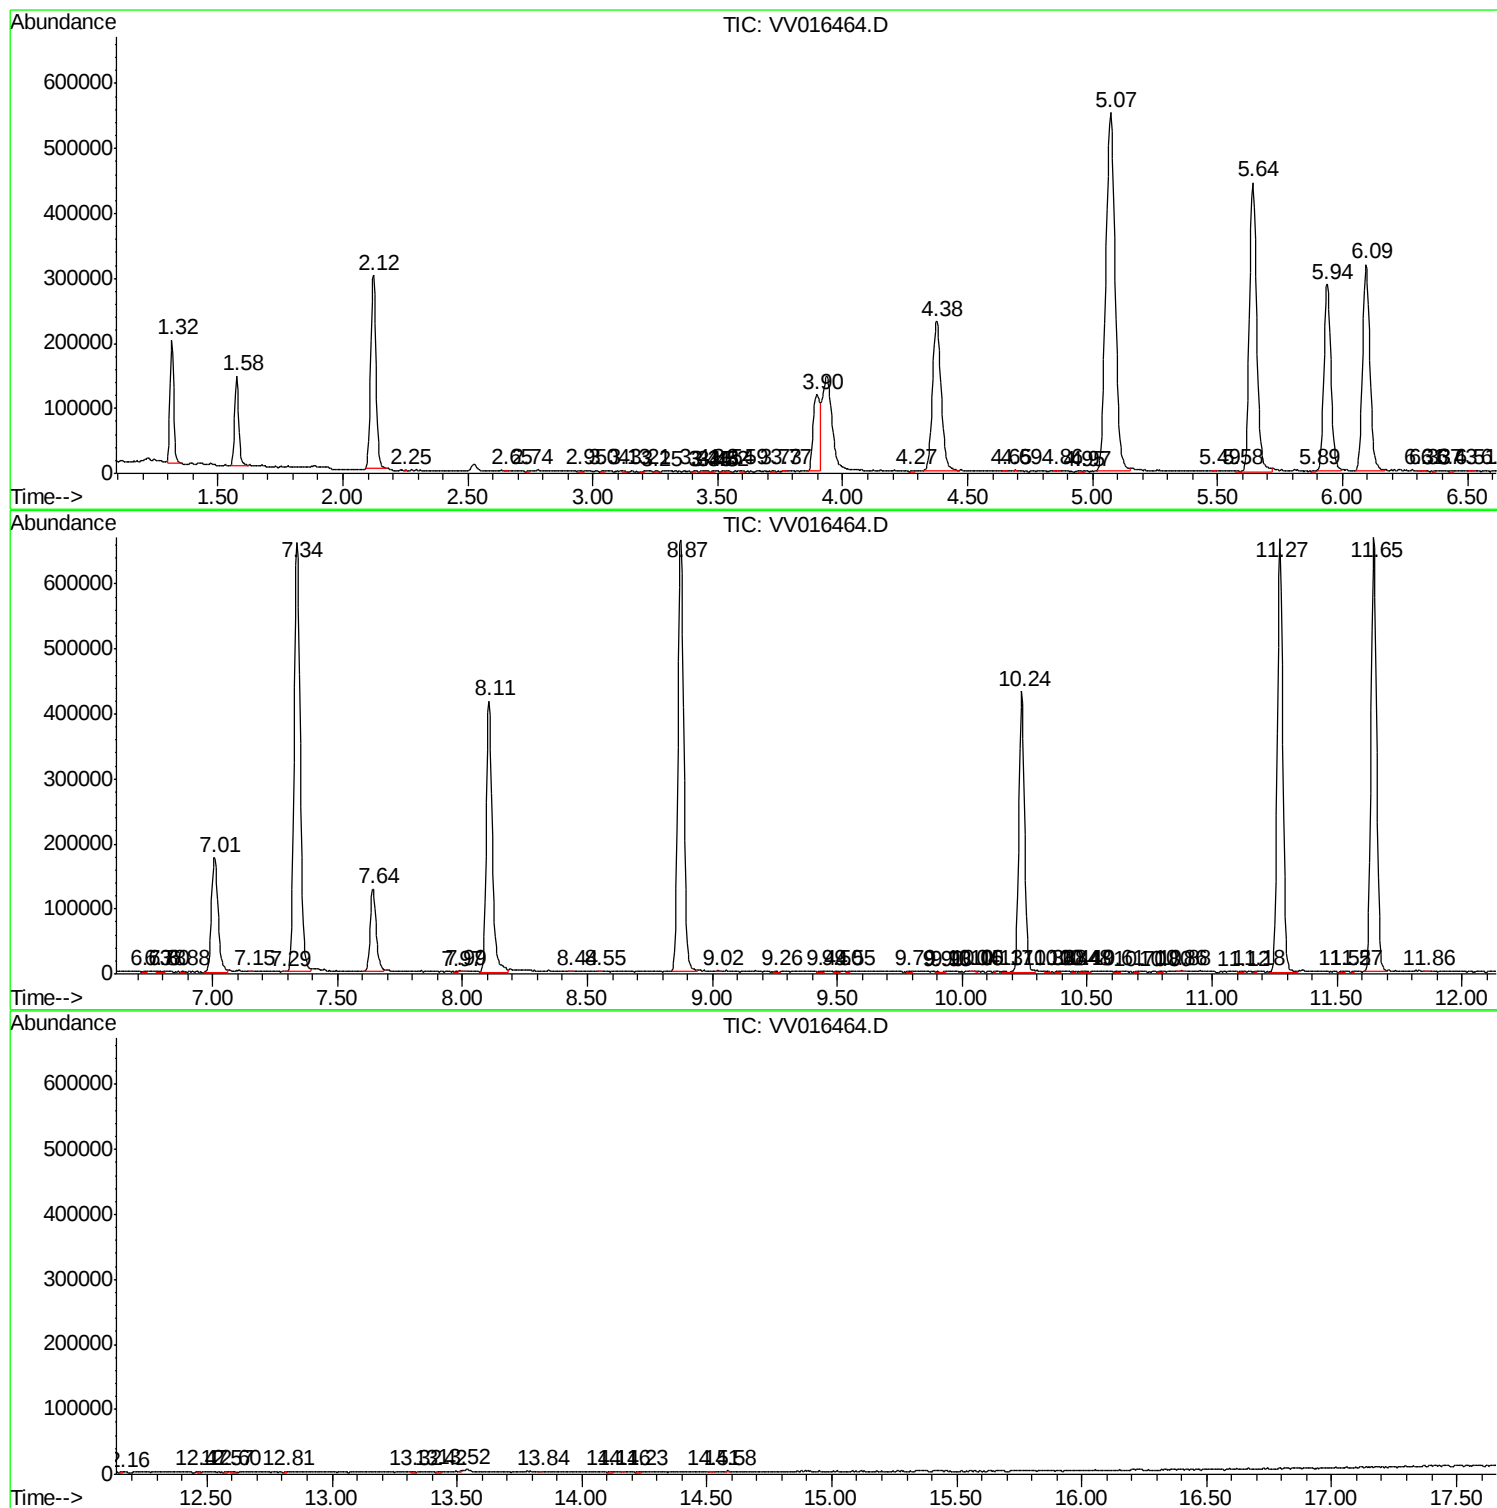

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060320\
Data File : VV016464.D
Acq On : 03 Jun 2020 18:10
Operator : SY/MD
Sample : L2843-07DL 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB1DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060320\
Data File : VV016464.D
Acq On : 03 Jun 2020 18:10
Operator : SY/MD
Sample : L2843-07DL 40X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB1DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc