

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016469.D
 Acq On : 03 Jun 2020 20:08
 Operator : SY/MD
 Sample : L2844-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AF4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	64	70	86	rVB	194842	192454	13.59%	1.778%
2	1.573	144	150	162	rVB	129264	151403	10.69%	1.399%
3	2.123	311	321	332	rBV	295924	434777	30.69%	4.016%
4	2.283	363	371	383	rBV	15962	27625	1.95%	0.255%
5	2.380	398	401	407	rVB8	2028	1967	0.14%	0.018%
6	2.566	457	459	463	rBV4	1293	964	0.07%	0.009%
7	2.692	496	498	499	rBV	1576	663	0.05%	0.006%
8	2.769	520	522	524	rBV3	1187	585	0.04%	0.005%
9	2.852	545	548	550	rBV4	1012	644	0.05%	0.006%
10	3.007	594	596	600	rVB3	1033	630	0.04%	0.006%
11	3.026	600	602	606	rBV5	816	673	0.05%	0.006%
12	3.100	622	625	627	rBV4	1211	685	0.05%	0.006%
13	3.142	633	638	639	rBV4	2089	1217	0.09%	0.011%
14	3.309	688	690	691	rBV2	744	386	0.03%	0.004%
15	3.418	722	724	728	rVB4	723	239	0.02%	0.002%
16	3.444	728	732	733	rBV3	1483	1046	0.07%	0.010%
17	3.473	739	741	744	rBV3	1202	666	0.05%	0.006%
18	3.560	765	768	774	rBV7	1790	2207	0.16%	0.020%
19	3.656	795	798	800	rBV4	999	424	0.03%	0.004%
20	3.682	804	806	808	rBV3	1386	682	0.05%	0.006%
21	3.756	824	829	830	rBV4	994	713	0.05%	0.007%
22	3.827	848	851	854	rBV5	1441	979	0.07%	0.009%
23	3.849	854	858	861	rBV6	1759	1276	0.09%	0.012%
24	3.894	862	872	901	rBV	109795	291140	20.55%	2.689%
25	4.293	994	996	999	rBV4	1254	702	0.05%	0.006%
26	4.373	1007	1021	1045	rBV	227267	551009	38.90%	5.090%
27	4.614	1090	1096	1098	rBV6	1641	1621	0.11%	0.015%
28	4.679	1114	1116	1117	rBV2	1335	558	0.04%	0.005%
29	4.846	1166	1168	1169	rBV2	546	129	0.01%	0.001%
30	4.868	1173	1175	1177	rBV3	936	289	0.02%	0.003%
31	4.962	1201	1204	1205	rBV2	1019	407	0.03%	0.004%
32	4.997	1212	1215	1220	rBV8	1343	1440	0.10%	0.013%
33	5.071	1220	1238	1263	rBV2	550270	1416641	100.00%	13.086%
34	5.325	1315	1317	1321	rBV4	1380	1295	0.09%	0.012%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016469.D
 Acq On : 03 Jun 2020 20:08
 Operator : SY/MD
 Sample : L2844-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AF4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	5.489	1366	1368	1370	rBV4	1586	670	0.05%	0.006%
36	5.640	1402	1415	1440	rBV	441667	878300	62.00%	8.113%
37	5.907	1495	1498	1499	rBV2	2094	1171	0.08%	0.011%
38	6.093	1544	1556	1581	rVB	316165	638613	45.08%	5.899%
39	6.351	1634	1636	1637	rBV2	1394	589	0.04%	0.005%
40	6.418	1653	1657	1658	rBV3	1077	753	0.05%	0.007%
41	6.540	1693	1695	1698	rVB3	823	344	0.02%	0.003%
42	6.714	1747	1749	1751	rBV3	1209	492	0.03%	0.005%
43	6.846	1786	1790	1793	rBV4	1345	1276	0.09%	0.012%
44	6.891	1803	1804	1805	rBV	793	166	0.01%	0.002%
45	6.913	1809	1811	1814	rVB3	1266	539	0.04%	0.005%
46	6.946	1814	1821	1823	rBV8	1077	1358	0.10%	0.013%
47	7.007	1829	1840	1857	rBV	177624	311273	21.97%	2.875%
48	7.216	1902	1905	1907	rVB3	1483	838	0.06%	0.008%
49	7.251	1914	1916	1917	rBV2	1070	422	0.03%	0.004%
50	7.280	1923	1925	1930	rVB5	1424	899	0.06%	0.008%
51	7.338	1930	1943	1963	rBV	648257	1127563	79.59%	10.416%
52	7.582	2014	2019	2023	rBV8	1638	1457	0.10%	0.013%
53	7.643	2028	2038	2053	rVV	121554	207055	14.62%	1.913%
54	7.965	2131	2138	2142	rBV9	3311	4337	0.31%	0.040%
55	8.106	2170	2182	2204	rBV	417068	693000	48.92%	6.402%
56	8.540	2315	2317	2319	rBV3	1250	717	0.05%	0.007%
57	8.579	2325	2329	2332	rBV4	1331	1391	0.10%	0.013%
58	8.675	2356	2359	2361	rVB3	761	423	0.03%	0.004%
59	8.688	2361	2363	2365	rVB2	1161	493	0.03%	0.005%
60	8.711	2367	2370	2373	rBV4	1349	985	0.07%	0.009%
61	8.765	2384	2387	2388	rBV2	834	502	0.04%	0.005%
62	8.875	2409	2421	2436	rBV	655436	1065181	75.19%	9.840%
63	9.029	2466	2469	2470	rBV3	1545	801	0.06%	0.007%
64	9.318	2557	2559	2563	rBV4	1014	778	0.05%	0.007%
65	9.347	2563	2568	2571	rBV7	1812	1800	0.13%	0.017%
66	9.367	2571	2574	2578	rBV5	786	642	0.05%	0.006%
67	9.408	2585	2587	2590	rBV3	1178	651	0.05%	0.006%
68	9.489	2609	2612	2613	rBV3	1082	449	0.03%	0.004%
69	9.498	2613	2615	2618	rVB4	1244	664	0.05%	0.006%
70	9.553	2629	2632	2633	rBV3	1248	832	0.06%	0.008%
71	9.611	2646	2650	2651	rBV3	753	496	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016469.D
 Acq On : 03 Jun 2020 20:08
 Operator : SY/MD
 Sample : L2844-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AF4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	9.675	2664	2670	2674	rBV7	1872	1950	0.14%	0.018%
73	9.707	2677	2680	2681	rBV3	1124	518	0.04%	0.005%
74	9.833	2717	2719	2722	rBV3	1206	596	0.04%	0.006%
75	9.994	2766	2769	2770	rBV4	905	661	0.05%	0.006%
76	10.019	2775	2777	2779	rVV2	993	490	0.03%	0.005%
77	10.068	2790	2792	2797	rVB5	1191	686	0.05%	0.006%
78	10.090	2797	2799	2800	rBV2	1157	393	0.03%	0.004%
79	10.148	2814	2817	2822	rVB6	1628	1108	0.08%	0.010%
80	10.238	2834	2845	2861	rBV	430544	676039	47.72%	6.245%
81	10.637	2967	2969	2971	rBV3	917	312	0.02%	0.003%
82	10.817	3023	3025	3026	rBV2	832	295	0.02%	0.003%
83	10.913	3053	3055	3056	rBV	1026	412	0.03%	0.004%
84	11.048	3095	3097	3098	rBV3	942	221	0.02%	0.002%
85	11.167	3130	3134	3135	rBV3	1586	1249	0.09%	0.012%
86	11.270	3154	3166	3180	rBV	672090	1023308	72.23%	9.453%
87	11.505	3236	3239	3240	rBV3	1268	737	0.05%	0.007%
88	11.646	3270	3283	3301	rBV	676122	1061882	74.96%	9.809%
89	12.106	3423	3426	3427	rBV3	1009	539	0.04%	0.005%
90	12.132	3430	3434	3438	rBV6	1936	1992	0.14%	0.018%
91	12.363	3504	3506	3508	rBV3	1570	910	0.06%	0.008%
92	12.469	3536	3539	3540	rBV3	1080	672	0.05%	0.006%
93	12.553	3563	3565	3567	rBV3	1431	780	0.06%	0.007%
94	12.569	3568	3570	3572	rBV3	2099	1190	0.08%	0.011%
95	12.608	3579	3582	3585	rBV3	1707	1033	0.07%	0.010%
96	12.694	3607	3609	3610	rBV2	1923	871	0.06%	0.008%
97	12.929	3680	3682	3684	rBV3	1418	918	0.06%	0.008%
98	13.328	3803	3806	3808	rBV5	3367	2350	0.17%	0.022%
99	13.633	3896	3901	3909	rBV5	3679	5738	0.41%	0.053%
100	14.456	4153	4157	4158	rBV4	2008	1520	0.11%	0.014%


Sum of corrected areas: 10825426

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060320\
Data File : VV016469.D
Acq On : 03 Jun 2020 20:08
Operator : SY/MD
Sample : L2844-07
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

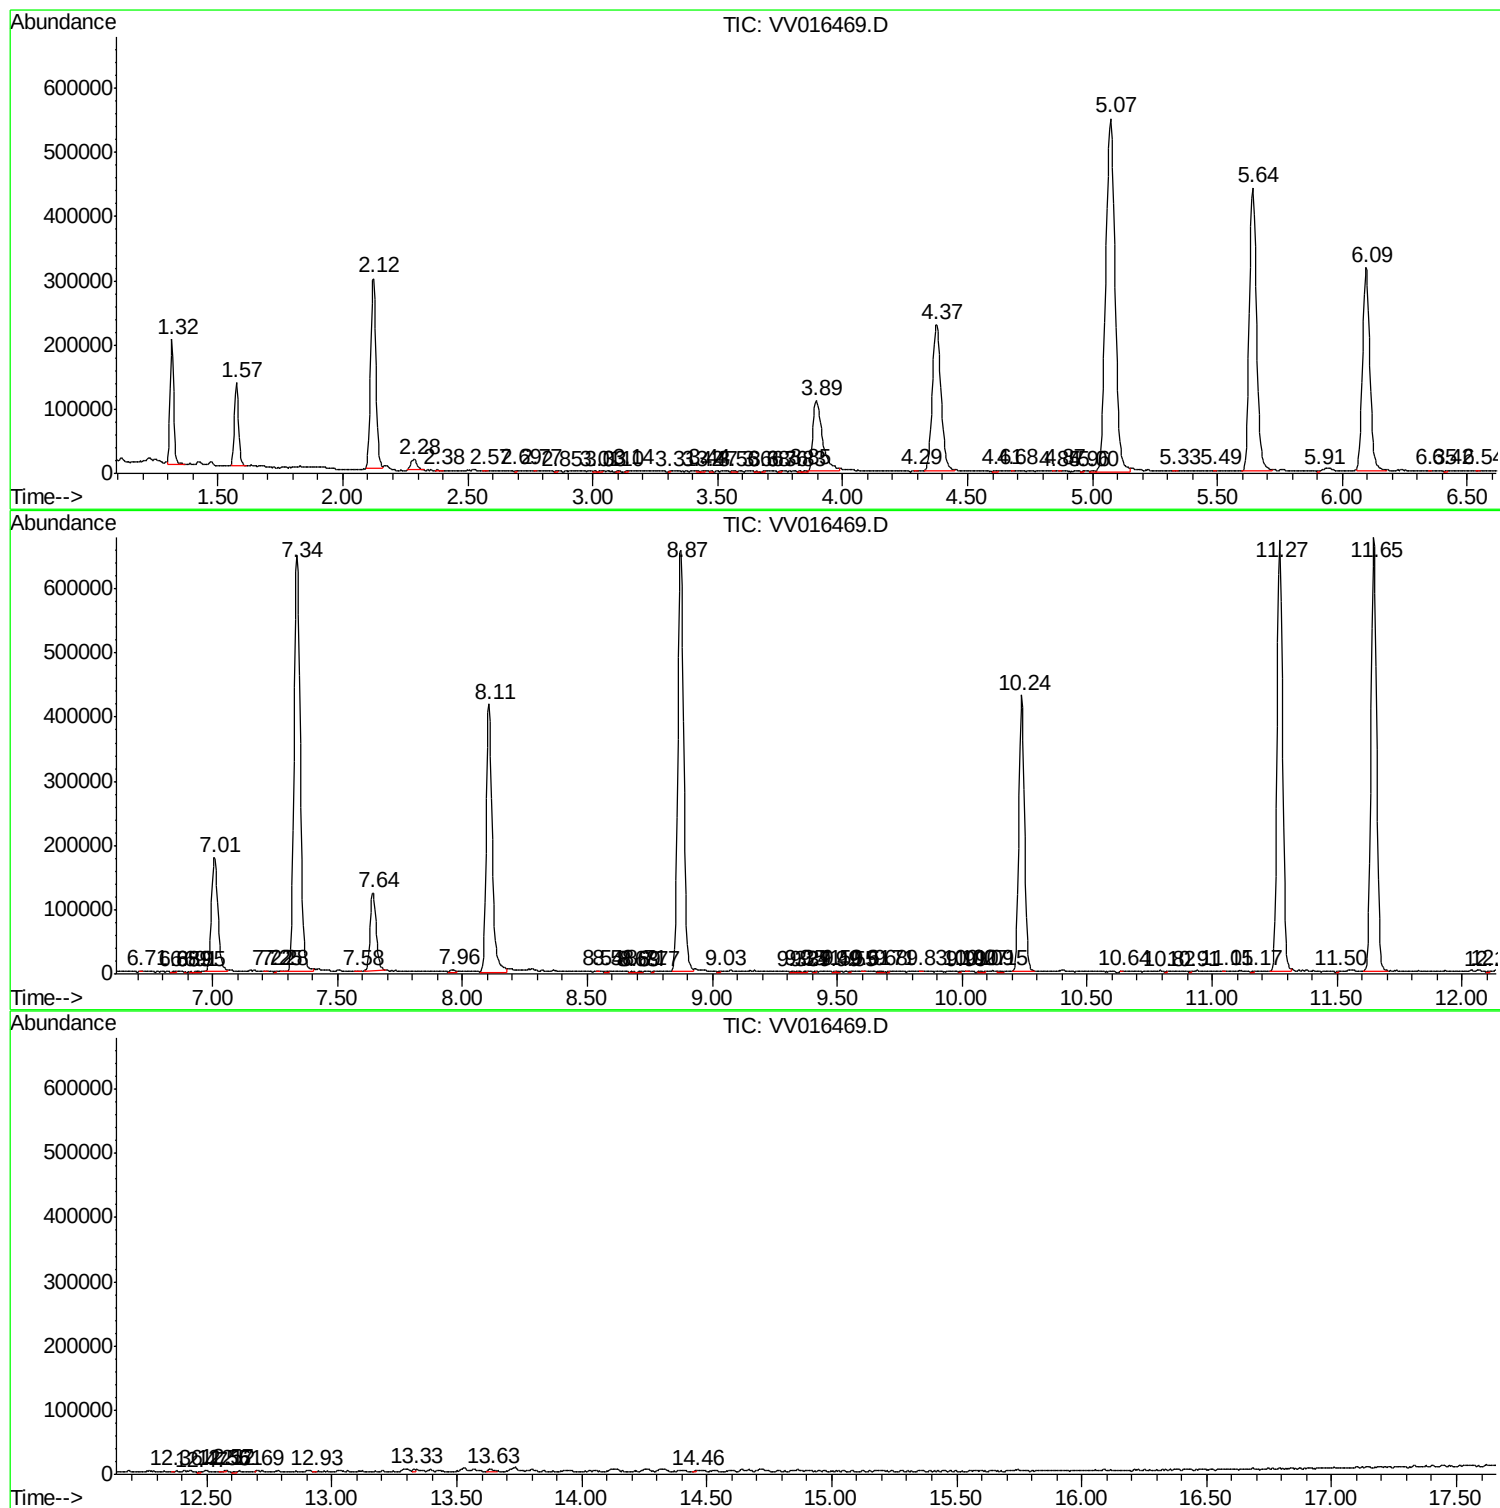

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060320\
Data File : VV016469.D
Acq On : 03 Jun 2020 20:08
Operator : SY/MD
Sample : L2844-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060320\
Data File : VV016469.D
Acq On : 03 Jun 2020 20:08
Operator : SY/MD
Sample : L2844-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AF4

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc