

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016470.D
 Acq On : 03 Jun 2020 20:32
 Operator : SY/MD
 Sample : L2868-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBFG3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	64	70	80	rVB	172844	177645	12.75%	1.661%
2	1.576	144	151	164	rVB	134111	154944	11.12%	1.449%
3	2.123	311	321	332	rBV	288192	418707	30.05%	3.915%
4	2.351	389	392	394	rBV3	1427	997	0.07%	0.009%
5	2.563	455	458	460	rBV2	1311	769	0.06%	0.007%
6	2.647	482	484	486	rBV3	1203	502	0.04%	0.005%
7	2.743	511	514	517	rBV3	1305	1015	0.07%	0.009%
8	2.759	517	519	520	rBV2	1300	525	0.04%	0.005%
9	2.827	538	540	542	rBV2	1124	591	0.04%	0.006%
10	2.840	542	544	547	rVV4	1140	674	0.05%	0.006%
11	3.203	654	657	662	rBV7	707	579	0.04%	0.005%
12	3.270	676	678	681	rBV3	825	499	0.04%	0.005%
13	3.351	699	703	706	rBV5	1329	1188	0.09%	0.011%
14	3.444	730	732	734	rBV2	846	424	0.03%	0.004%
15	3.483	742	744	747	rVB4	1190	479	0.03%	0.004%
16	3.534	756	760	762	rVB4	1495	987	0.07%	0.009%
17	3.550	762	765	766	rBV2	1153	619	0.04%	0.006%
18	3.598	778	780	782	rVB3	1280	383	0.03%	0.004%
19	3.614	782	785	787	rBV4	968	723	0.05%	0.007%
20	3.737	818	823	828	rBV9	1519	1895	0.14%	0.018%
21	3.894	863	872	898	rBV	109204	284453	20.41%	2.659%
22	4.238	976	979	982	rBV3	1488	961	0.07%	0.009%
23	4.377	1008	1022	1048	rVB	225142	544907	39.11%	5.094%
24	4.512	1060	1064	1065	rBV4	2202	1405	0.10%	0.013%
25	4.605	1092	1093	1096	rVB3	1484	697	0.05%	0.007%
26	4.659	1108	1110	1112	rBV2	845	388	0.03%	0.004%
27	4.688	1116	1119	1121	rBV4	1334	945	0.07%	0.009%
28	4.727	1129	1131	1133	rBV3	1186	687	0.05%	0.006%
29	5.071	1220	1238	1267	rBV2	537295	1393402	100.00%	13.027%
30	5.418	1340	1346	1351	rBV8	1801	1957	0.14%	0.018%
31	5.508	1372	1374	1377	rBV4	1215	770	0.06%	0.007%
32	5.563	1388	1391	1395	rBV6	1453	924	0.07%	0.009%
33	5.640	1402	1415	1439	rBV	439232	877768	62.99%	8.206%
34	5.942	1498	1509	1525	rBV3	33553	70461	5.06%	0.659%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016470.D
 Acq On : 03 Jun 2020 20:32
 Operator : SY/MD
 Sample : L2868-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBFG3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.093	1544	1556	1578	rVB	309537	616510	44.24%	5.764%
36	6.405	1649	1653	1654	rBV3	1373	829	0.06%	0.008%
37	6.524	1687	1690	1691	rBV3	926	396	0.03%	0.004%
38	6.550	1696	1698	1703	rBV5	1259	1201	0.09%	0.011%
39	6.598	1711	1713	1716	rBV4	915	417	0.03%	0.004%
40	6.743	1750	1758	1761	rBV8	1095	1252	0.09%	0.012%
41	6.775	1765	1768	1769	rBV3	1148	411	0.03%	0.004%
42	6.785	1769	1771	1774	rVB3	1918	865	0.06%	0.008%
43	6.801	1774	1776	1778	rBV3	1265	503	0.04%	0.005%
44	6.917	1809	1812	1813	rBV3	1019	423	0.03%	0.004%
45	7.007	1825	1840	1857	rBV	170438	307721	22.08%	2.877%
46	7.338	1928	1943	1961	rBV	641233	1103618	79.20%	10.318%
47	7.556	2009	2011	2017	rVB6	1391	1213	0.09%	0.011%
48	7.643	2024	2038	2057	rBV	119128	210516	15.11%	1.968%
49	7.836	2096	2098	2102	rVB3	2096	1398	0.10%	0.013%
50	7.910	2118	2121	2122	rBV3	1212	703	0.05%	0.007%
51	8.061	2165	2168	2171	rBV4	1537	1337	0.10%	0.012%
52	8.106	2172	2182	2215	rVV	408093	681014	48.87%	6.367%
53	8.470	2291	2295	2297	rBV4	1489	1343	0.10%	0.013%
54	8.566	2321	2325	2328	rBV4	1322	1123	0.08%	0.010%
55	8.653	2350	2352	2355	rBV4	1377	755	0.05%	0.007%
56	8.711	2367	2370	2371	rBV3	1012	631	0.05%	0.006%
57	8.781	2390	2392	2394	rBV3	935	446	0.03%	0.004%
58	8.875	2407	2421	2437	rBV	672186	1075966	77.22%	10.059%
59	9.344	2564	2567	2569	rBV5	732	536	0.04%	0.005%
60	9.357	2569	2571	2574	rBV3	1181	710	0.05%	0.007%
61	9.399	2580	2584	2586	rBV3	1212	797	0.06%	0.007%
62	9.415	2586	2589	2590	rBV3	895	477	0.03%	0.004%
63	9.720	2682	2684	2685	rBV2	1080	476	0.03%	0.004%
64	9.759	2694	2696	2698	rBV3	731	442	0.03%	0.004%
65	9.778	2701	2702	2707	rVV4	1247	884	0.06%	0.008%
66	9.814	2711	2713	2715	rVV3	970	468	0.03%	0.004%
67	9.913	2740	2744	2747	rBV5	1322	1331	0.10%	0.012%
68	10.023	2776	2778	2780	rBV3	1117	671	0.05%	0.006%
69	10.113	2803	2806	2809	rBV4	1593	958	0.07%	0.009%
70	10.164	2819	2822	2823	rBV3	1009	463	0.03%	0.004%
71	10.238	2834	2845	2860	rVB	408650	644569	46.26%	6.026%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016470.D
 Acq On : 03 Jun 2020 20:32
 Operator : SY/MD
 Sample : L2868-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBFG3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	10.334	2874	2875	2878	rBV4	1191	698	0.05%	0.007%
73	10.396	2892	2894	2897	rVB3	1465	756	0.05%	0.007%
74	10.425	2901	2903	2909	rBV6	970	702	0.05%	0.007%
75	10.470	2914	2917	2920	rBV5	1291	825	0.06%	0.008%
76	10.531	2934	2936	2939	rBV4	1190	626	0.04%	0.006%
77	10.601	2955	2958	2960	rBV2	1927	1397	0.10%	0.013%
78	10.797	3017	3019	3022	rBV4	1508	808	0.06%	0.008%
79	10.926	3055	3059	3061	rBV5	1122	896	0.06%	0.008%
80	11.135	3122	3124	3127	rVB3	1172	566	0.04%	0.005%
81	11.154	3127	3130	3134	rBV4	1731	1376	0.10%	0.013%
82	11.177	3135	3137	3143	rVV7	1839	1603	0.12%	0.015%
83	11.232	3151	3154	3155	rBV3	1190	650	0.05%	0.006%
84	11.270	3155	3166	3181	rVV	683405	1023351	73.44%	9.567%
85	11.646	3271	3283	3298	rBV	667366	1038944	74.56%	9.713%
86	11.926	3366	3370	3374	rBV5	1080	988	0.07%	0.009%
87	12.129	3428	3433	3439	rVB8	1817	1942	0.14%	0.018%
88	12.238	3465	3467	3468	rBV	1456	668	0.05%	0.006%
89	12.267	3472	3476	3477	rBV3	1473	979	0.07%	0.009%
90	12.540	3559	3561	3563	rBV3	929	413	0.03%	0.004%
91	12.604	3579	3581	3586	rBV6	1043	873	0.06%	0.008%
92	12.785	3636	3637	3641	rBV3	1007	530	0.04%	0.005%
93	13.328	3803	3806	3809	rVB4	1434	784	0.06%	0.007%
94	13.485	3853	3855	3858	rBV4	1085	698	0.05%	0.007%
95	13.527	3865	3868	3870	rBV3	2824	1952	0.14%	0.018%
96	14.090	4039	4043	4047	rVB7	1928	1553	0.11%	0.015%
97	14.161	4063	4065	4068	rBV4	1576	663	0.05%	0.006%
98	14.350	4122	4124	4125	rBV	1585	634	0.05%	0.006%
99	14.402	4136	4140	4144	rBV7	1864	2013	0.14%	0.019%
100	14.704	4231	4234	4236	rBV3	1568	991	0.07%	0.009%


Sum of corrected areas: 10696122

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060320\
Data File : VV016470.D
Acq On : 03 Jun 2020 20:32
Operator : SY/MD
Sample : L2868-01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBFG3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

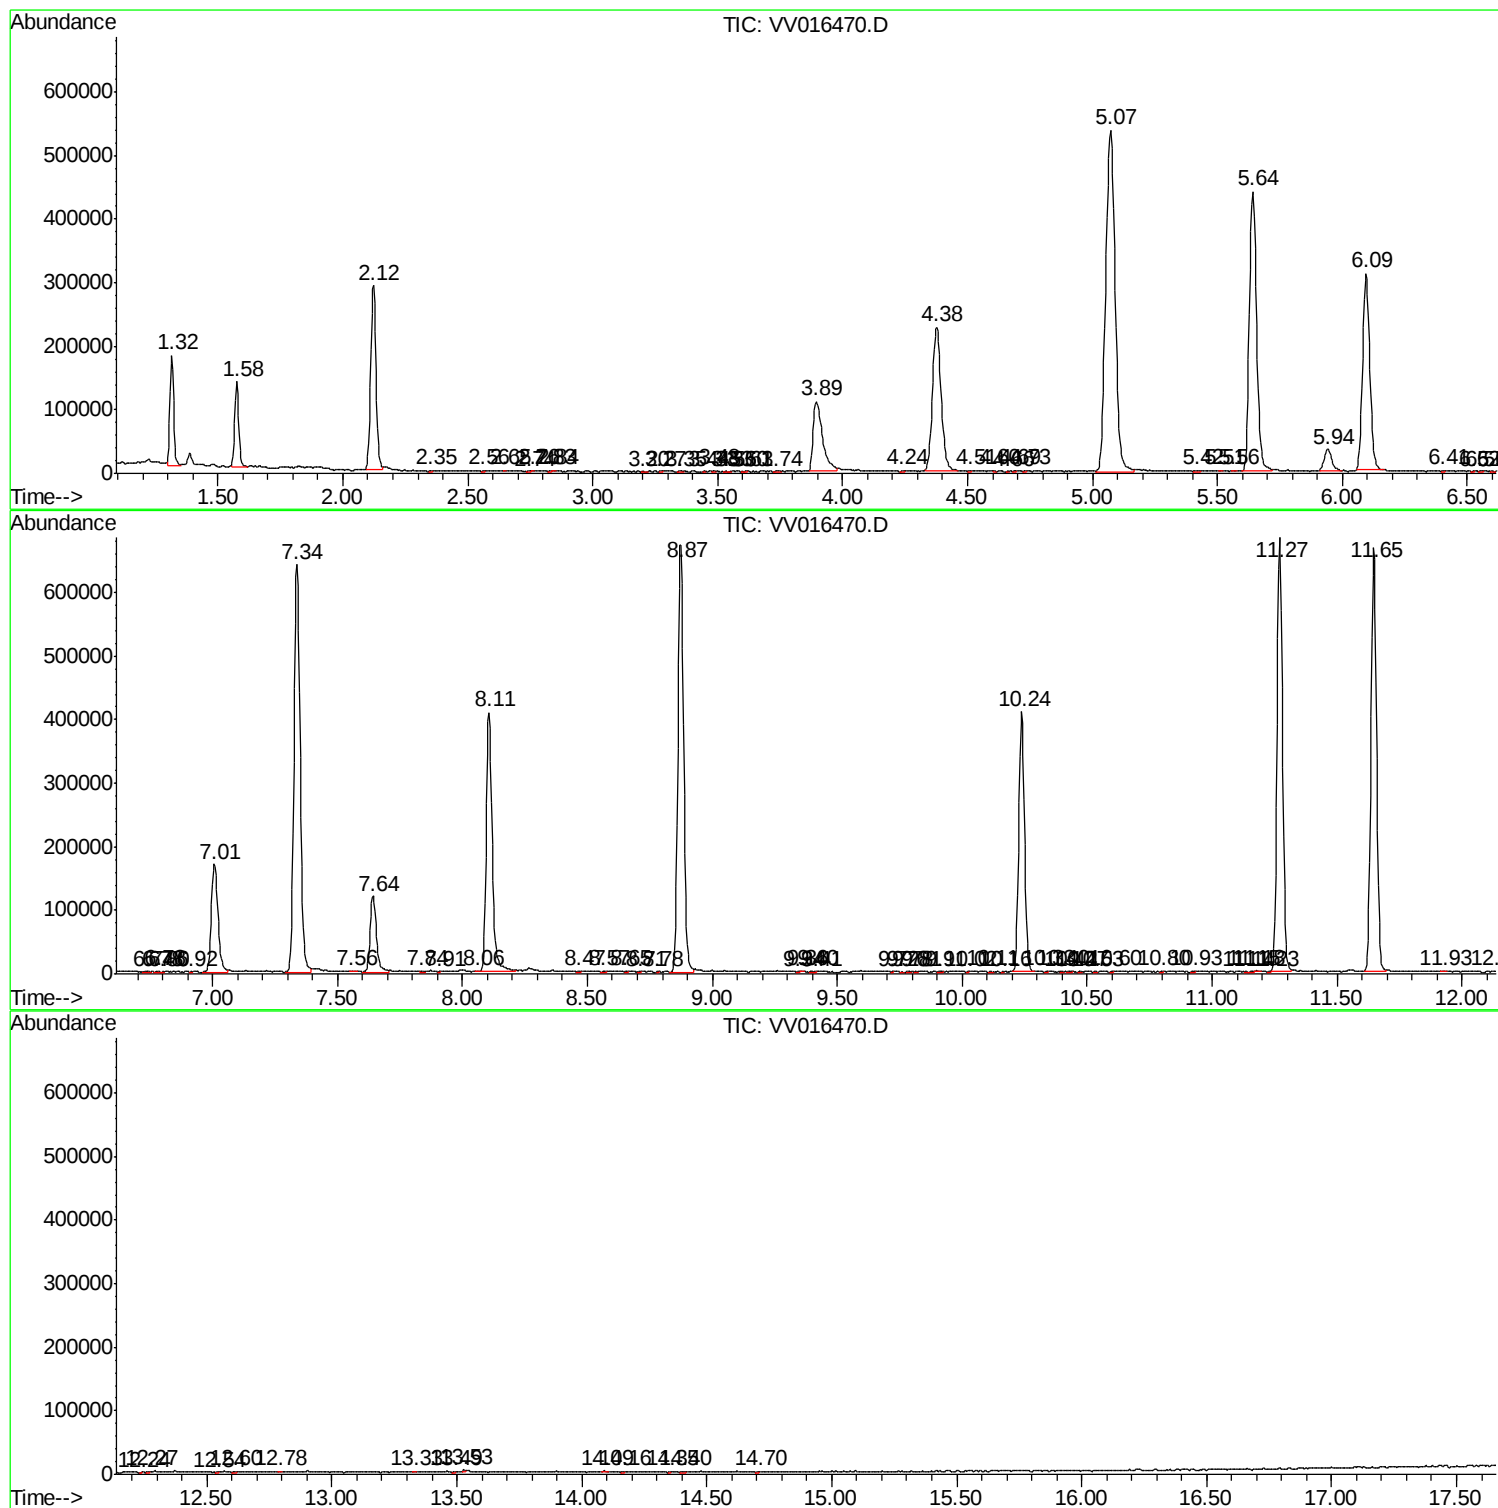

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060320\
Data File : VV016470.D
Acq On : 03 Jun 2020 20:32
Operator : SY/MD
Sample : L2868-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBFG3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060320\
Data File : VV016470.D
Acq On : 03 Jun 2020 20:32
Operator : SY/MD
Sample : L2868-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBFG3

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc