

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016472.D
 Acq On : 03 Jun 2020 22:07
 Operator : SY/MD
 Sample : VV0603WBL03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK66

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	83	rVB	187804	183269	12.67%	1.675%
2	1.573	144	150	164	rVB	148672	172533	11.93%	1.576%
3	2.122	311	321	339	rBV	281022	409853	28.34%	3.745%
4	2.354	391	393	395	rBV3	1199	670	0.05%	0.006%
5	2.521	438	445	446	rBV6	4802	4097	0.28%	0.037%
6	2.592	465	467	470	rBV4	1036	642	0.04%	0.006%
7	2.621	474	476	479	rBV3	1111	690	0.05%	0.006%
8	2.650	482	485	488	rBV5	1482	985	0.07%	0.009%
9	2.843	542	545	546	rBV3	807	498	0.03%	0.005%
10	3.007	593	596	597	rBV2	842	476	0.03%	0.004%
11	3.093	620	623	624	rBV3	829	440	0.03%	0.004%
12	3.116	626	630	632	rVV4	779	490	0.03%	0.004%
13	3.142	636	638	642	rVB2	1192	670	0.05%	0.006%
14	3.196	652	655	657	rBV4	1545	839	0.06%	0.008%
15	3.219	660	662	668	rVB6	1230	684	0.05%	0.006%
16	3.257	672	674	678	rVV4	1178	656	0.05%	0.006%
17	3.402	716	719	721	rBV3	1678	911	0.06%	0.008%
18	3.441	728	731	736	rVB5	1022	860	0.06%	0.008%
19	3.470	736	740	742	rBV4	948	651	0.05%	0.006%
20	3.499	747	749	752	rVB3	1005	579	0.04%	0.005%
21	3.515	752	754	758	rBV3	734	522	0.04%	0.005%
22	3.534	758	760	763	rBV4	1045	507	0.04%	0.005%
23	3.563	766	769	770	rBV3	1542	799	0.06%	0.007%
24	3.637	790	792	797	rVB6	1664	1115	0.08%	0.010%
25	3.659	797	799	801	rBV2	744	431	0.03%	0.004%
26	3.679	801	805	807	rVV4	1673	1102	0.08%	0.010%
27	3.692	807	809	812	rVB4	1271	666	0.05%	0.006%
28	3.711	812	815	816	rBV2	978	430	0.03%	0.004%
29	3.894	861	872	896	rBV	114927	306426	21.19%	2.800%
30	4.187	961	963	969	rBV8	1642	1689	0.12%	0.015%
31	4.376	1007	1022	1052	rVB	235016	571082	39.48%	5.218%
32	4.556	1076	1078	1080	rBV3	1153	640	0.04%	0.006%
33	4.666	1110	1112	1115	rBV3	1248	693	0.05%	0.006%
34	4.843	1165	1167	1171	rBV4	740	600	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016472.D
 Acq On : 03 Jun 2020 22:07
 Operator : SY/MD
 Sample : VV0603WBL03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK66

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	4.968	1203	1206	1209	rVB4	1117	858	0.06%	0.008%
36	5.071	1220	1238	1262	rBV2	560021	1446336	100.00%	13.216%
37	5.376	1331	1333	1338	rVB5	1763	1030	0.07%	0.009%
38	5.640	1403	1415	1436	rBV	432447	851926	58.90%	7.784%
39	5.939	1498	1508	1516	rVV	5609	11862	0.82%	0.108%
40	6.093	1543	1556	1583	rBV	335597	672476	46.50%	6.145%
41	6.322	1623	1627	1631	rBV6	1592	1173	0.08%	0.011%
42	6.370	1640	1642	1643	rBV2	1282	451	0.03%	0.004%
43	6.515	1684	1687	1689	rBV4	1242	884	0.06%	0.008%
44	6.743	1756	1758	1759	rBV2	1260	481	0.03%	0.004%
45	6.781	1767	1770	1772	rBV4	1167	891	0.06%	0.008%
46	6.871	1793	1798	1801	rVB7	1322	1168	0.08%	0.011%
47	6.929	1813	1816	1819	rBV4	1167	933	0.06%	0.009%
48	7.006	1827	1840	1860	rBV2	175676	320290	22.14%	2.927%
49	7.177	1891	1893	1895	rBV4	1534	658	0.05%	0.006%
50	7.338	1930	1943	1961	rBV	676991	1162017	80.34%	10.618%
51	7.643	2028	2038	2053	rBV2	123248	209244	14.47%	1.912%
52	8.068	2167	2170	2171	rBV3	1927	876	0.06%	0.008%
53	8.106	2172	2182	2204	rVV	421000	696867	48.18%	6.367%
54	8.582	2328	2330	2331	rBV2	1380	591	0.04%	0.005%
55	8.653	2349	2352	2357	rBV7	2334	1896	0.13%	0.017%
56	8.675	2357	2359	2360	rBV2	1232	623	0.04%	0.006%
57	8.817	2401	2403	2408	rVB6	1497	920	0.06%	0.008%
58	8.875	2408	2421	2439	rBV	661194	1058670	73.20%	9.673%
59	9.019	2463	2466	2468	rBV4	1784	1261	0.09%	0.012%
60	9.161	2505	2510	2518	rBV4	2131	3575	0.25%	0.033%
61	9.193	2518	2520	2522	rBV3	988	491	0.03%	0.004%
62	9.315	2556	2558	2564	rVB5	1573	1063	0.07%	0.010%
63	9.514	2617	2620	2621	rBV2	1256	626	0.04%	0.006%
64	9.698	2673	2677	2681	rBV6	1338	1501	0.10%	0.014%
65	9.756	2689	2695	2697	rBV7	1517	1455	0.10%	0.013%
66	9.923	2745	2747	2750	rBV4	1369	731	0.05%	0.007%
67	9.965	2758	2760	2762	rBV3	1876	1088	0.08%	0.010%
68	10.019	2774	2777	2781	rVB4	1966	1304	0.09%	0.012%
69	10.125	2809	2810	2812	rBV3	960	497	0.03%	0.005%
70	10.183	2825	2828	2831	rVB5	1414	929	0.06%	0.008%
71	10.238	2833	2845	2864	rVV	454705	705663	48.79%	6.448%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016472.D
 Acq On : 03 Jun 2020 22:07
 Operator : SY/MD
 Sample : VV0603WBL03
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK66

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	10.360	2881	2883	2887	rVB4	1115	703	0.05%	0.006%
73	10.608	2958	2960	2962	rBV3	831	522	0.04%	0.005%
74	10.698	2985	2988	2989	rBV2	1485	798	0.06%	0.007%
75	10.743	2997	3002	3006	rBV7	2041	2031	0.14%	0.019%
76	10.836	3029	3031	3033	rVB3	1252	510	0.04%	0.005%
77	10.932	3057	3061	3062	rBV4	1736	1037	0.07%	0.009%
78	11.119	3114	3119	3124	rBV8	1082	1470	0.10%	0.013%
79	11.145	3124	3127	3131	rVB5	1568	1028	0.07%	0.009%
80	11.164	3131	3133	3136	rBV3	776	423	0.03%	0.004%
81	11.270	3155	3166	3182	rBV	656572	1000338	69.16%	9.140%
82	11.489	3232	3234	3238	rVB5	1332	780	0.05%	0.007%
83	11.646	3271	3283	3300	rBV	715919	1091108	75.44%	9.970%
84	11.874	3350	3354	3359	rBV7	1158	1260	0.09%	0.012%
85	11.926	3368	3370	3372	rVB3	1175	476	0.03%	0.004%
86	11.993	3388	3391	3395	rBV5	1118	1038	0.07%	0.009%
87	12.029	3400	3402	3404	rBV2	1426	719	0.05%	0.007%
88	12.080	3415	3418	3421	rBV3	959	463	0.03%	0.004%
89	12.199	3453	3455	3458	rBV3	1098	587	0.04%	0.005%
90	12.366	3505	3507	3510	rBV4	1338	1063	0.07%	0.010%
91	12.492	3543	3546	3550	rBV6	1579	1097	0.08%	0.010%
92	12.694	3606	3609	3610	rBV3	1019	427	0.03%	0.004%
93	12.714	3613	3615	3618	rBV3	1199	726	0.05%	0.007%
94	12.755	3625	3628	3632	rBV5	1684	1562	0.11%	0.014%
95	12.794	3638	3640	3643	rBV4	1115	552	0.04%	0.005%
96	13.000	3702	3704	3706	rBV2	1129	519	0.04%	0.005%
97	13.350	3810	3813	3814	rBV2	956	454	0.03%	0.004%
98	13.463	3846	3848	3851	rVB3	1549	659	0.05%	0.006%
99	13.736	3931	3933	3934	rBV	1119	455	0.03%	0.004%
100	15.160	4373	4376	4378	rBV5	1596	924	0.06%	0.008%


Sum of corrected areas: 10944229

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060320\
Data File : VV016472.D
Acq On : 03 Jun 2020 22:07
Operator : SY/MD
Sample : VV0603WBL03
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK66

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

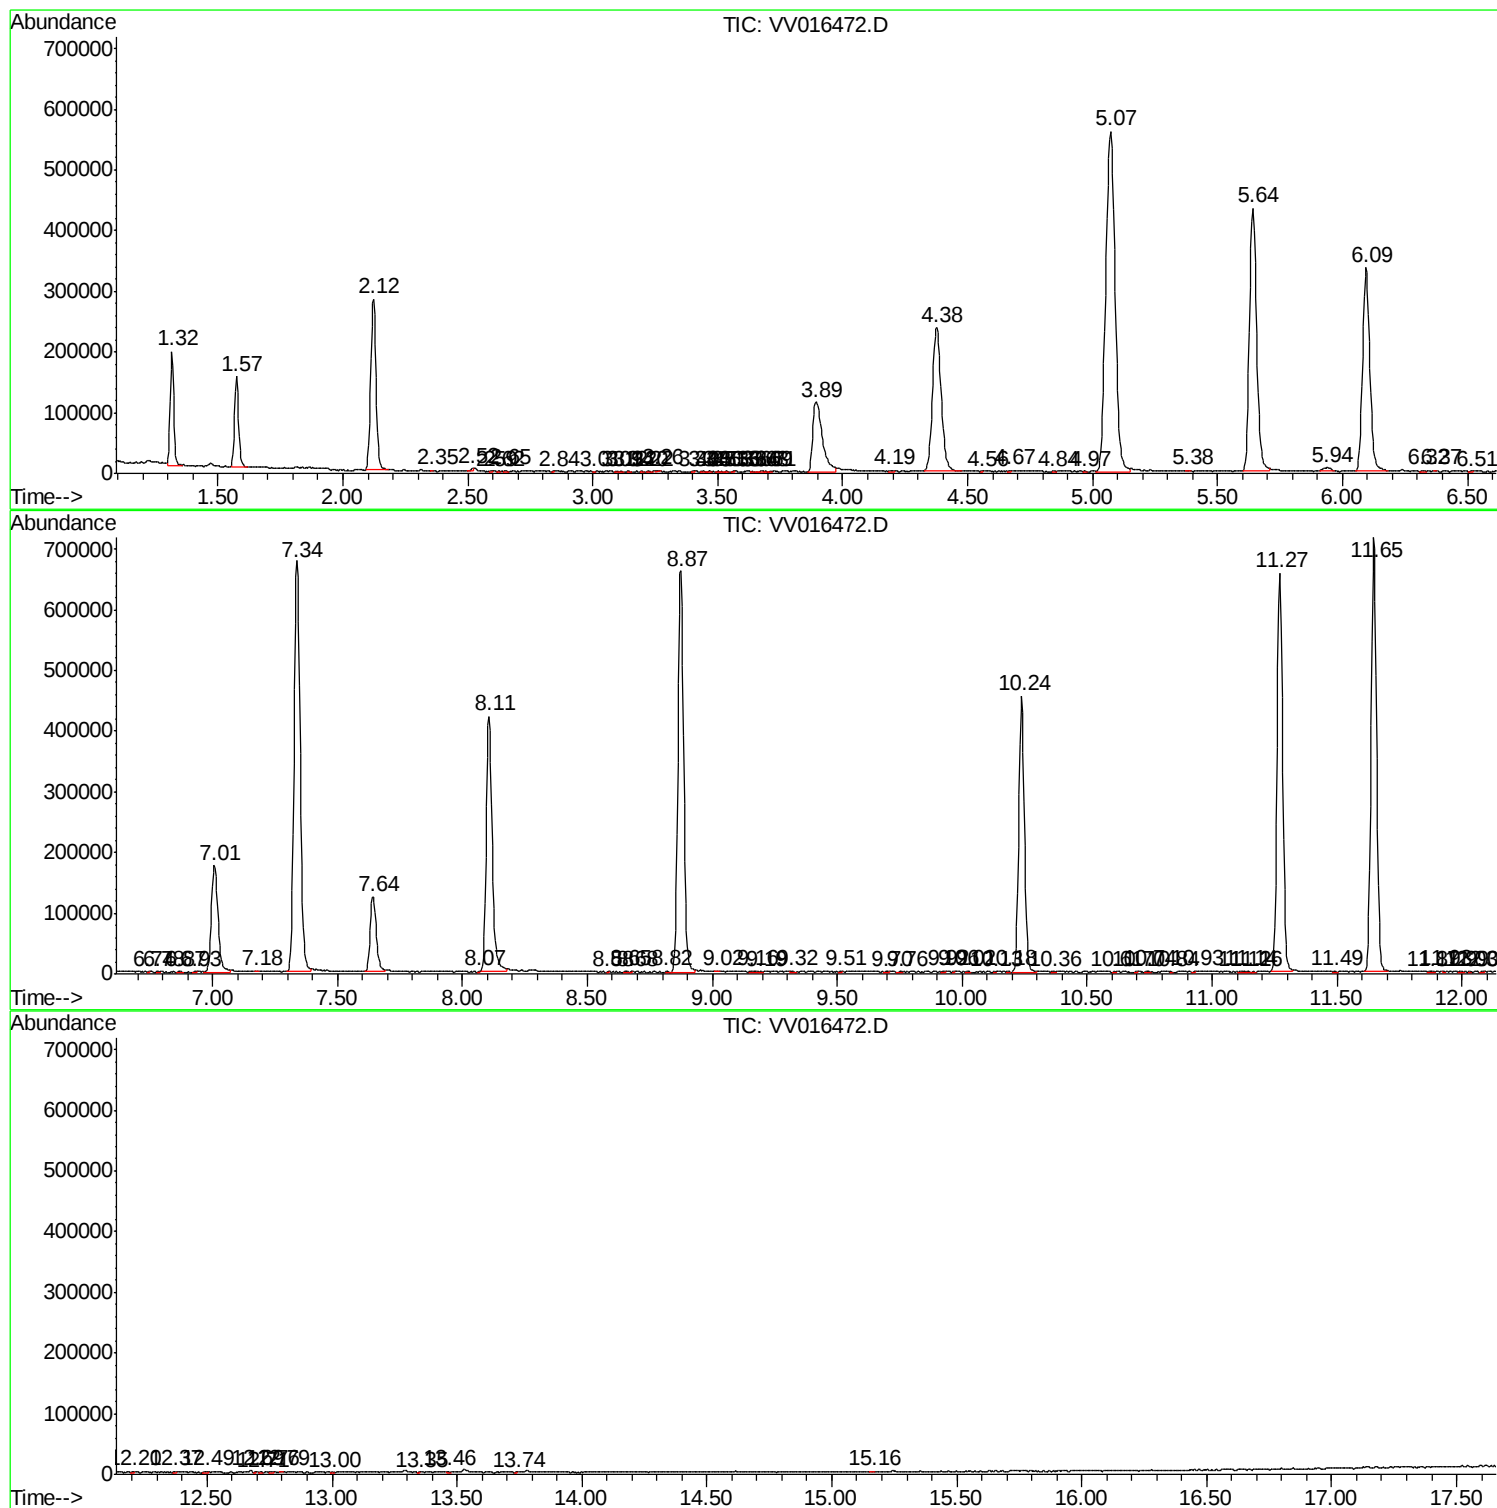

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060320\
Data File : VV016472.D
Acq On : 03 Jun 2020 22:07
Operator : SY/MD
Sample : VV0603WBL03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK66

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060320\
Data File : VV016472.D
Acq On : 03 Jun 2020 22:07
Operator : SY/MD
Sample : VV0603WBL03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK66

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc