

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016477.D
 Acq On : 04 Jun 2020 00:05
 Operator : SY/MD
 Sample : L2869-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBFG7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.316	65	70	82	rVB	175390	179719	2.82%	1.051%
2	1.566	142	148	159	rVB	133012	149271	2.34%	0.873%
3	2.119	311	320	332	rBV	283953	411940	6.46%	2.410%
4	2.939	573	575	577	rBV3	1229	631	0.01%	0.004%
5	2.975	583	586	588	rBV2	1768	1199	0.02%	0.007%
6	3.010	595	597	600	rVB4	1118	496	0.01%	0.003%
7	3.081	616	619	624	rBV7	1921	1452	0.02%	0.008%
8	3.254	669	673	677	rBV4	1534	1518	0.02%	0.009%
9	3.422	723	725	729	rBV4	1072	735	0.01%	0.004%
10	3.508	748	752	756	rBV5	1453	1541	0.02%	0.009%
11	3.573	769	772	774	rVB2	1100	621	0.01%	0.004%
12	3.586	774	776	779	rBV3	783	568	0.01%	0.003%
13	3.666	799	801	805	rBV4	888	574	0.01%	0.003%
14	3.704	811	813	815	rBV3	884	581	0.01%	0.003%
15	3.737	821	823	826	rVB4	1595	869	0.01%	0.005%
16	3.753	826	828	830	rBV3	912	559	0.01%	0.003%
17	3.801	839	843	847	rVB6	1554	1082	0.02%	0.006%
18	3.833	850	853	854	rBV2	879	543	0.01%	0.003%
19	3.897	861	873	878	rBV	110021	224604	3.52%	1.314%
20	4.277	987	991	994	rVB4	1011	748	0.01%	0.004%
21	4.303	994	999	1002	rBV8	1492	1395	0.02%	0.008%
22	4.373	1006	1021	1046	rVV	225224	556523	8.72%	3.255%
23	4.614	1093	1096	1097	rBV3	1268	686	0.01%	0.004%
24	4.650	1104	1107	1109	rBV3	1351	833	0.01%	0.005%
25	4.840	1164	1166	1168	rBV2	1421	796	0.01%	0.005%
26	4.913	1188	1189	1193	rVB3	1880	817	0.01%	0.005%
27	5.071	1219	1238	1268	rVV2	550289	1417821	22.22%	8.293%
28	5.354	1324	1326	1328	rBV3	1191	511	0.01%	0.003%
29	5.425	1345	1348	1349	rBV2	1634	772	0.01%	0.005%
30	5.511	1373	1375	1379	rVB4	2118	1244	0.02%	0.007%
31	5.585	1395	1398	1401	rBV5	1115	943	0.01%	0.006%
32	5.640	1402	1415	1437	rVV	462018	910717	14.27%	5.327%
33	5.936	1493	1507	1534	rBV	3330873	6379878	100.00%	37.318%
34	6.093	1544	1556	1579	rVB	317685	641077	10.05%	3.750%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016477.D
 Acq On : 04 Jun 2020 00:05
 Operator : SY/MD
 Sample : L2869-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBFG7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.370	1640	1642	1644	rVB3	1675	629	0.01%	0.004%
36	6.412	1651	1655	1656	rBV4	1129	919	0.01%	0.005%
37	6.547	1695	1697	1702	rBV6	1376	1240	0.02%	0.007%
38	6.769	1763	1766	1768	rBV4	1156	728	0.01%	0.004%
39	6.830	1780	1785	1789	rBV8	1196	1291	0.02%	0.008%
40	6.933	1815	1817	1819	rBV3	1110	557	0.01%	0.003%
41	6.942	1819	1820	1823	rBV2	864	530	0.01%	0.003%
42	7.007	1829	1840	1866	rVB	167360	304491	4.77%	1.781%
43	7.158	1884	1887	1889	rBV3	1455	919	0.01%	0.005%
44	7.251	1913	1916	1918	rBV3	1195	838	0.01%	0.005%
45	7.338	1931	1943	1962	rBV	653728	1109228	17.39%	6.488%
46	7.499	1991	1993	1995	rBV3	1067	484	0.01%	0.003%
47	7.640	2028	2037	2053	rBV2	118332	202624	3.18%	1.185%
48	7.894	2113	2116	2118	rBV4	1495	985	0.02%	0.006%
49	7.942	2127	2131	2133	rBV3	1722	1399	0.02%	0.008%
50	8.061	2165	2168	2169	rBV4	1286	852	0.01%	0.005%
51	8.106	2172	2182	2203	rBV	406745	681838	10.69%	3.988%
52	8.457	2288	2291	2295	rBV6	1856	1445	0.02%	0.008%
53	8.492	2299	2302	2305	rBV6	995	739	0.01%	0.004%
54	8.701	2361	2367	2370	rBV7	1805	1837	0.03%	0.011%
55	8.736	2377	2378	2381	rBV3	1459	810	0.01%	0.005%
56	8.791	2392	2395	2397	rBV4	1077	676	0.01%	0.004%
57	8.830	2404	2407	2408	rBV3	1336	675	0.01%	0.004%
58	8.875	2409	2421	2437	rVV	681473	1095782	17.18%	6.410%
59	9.029	2465	2469	2473	rBV7	1516	1462	0.02%	0.009%
60	9.206	2520	2524	2525	rBV3	1455	1035	0.02%	0.006%
61	9.238	2532	2534	2536	rBV3	1312	509	0.01%	0.003%
62	9.389	2576	2581	2582	rBV4	1145	694	0.01%	0.004%
63	9.421	2587	2591	2596	rBV8	805	882	0.01%	0.005%
64	9.447	2596	2599	2601	rBV4	926	578	0.01%	0.003%
65	9.560	2631	2634	2635	rBV3	1288	741	0.01%	0.004%
66	9.617	2650	2652	2660	rVB10	1194	1321	0.02%	0.008%
67	9.691	2671	2675	2676	rBV2	1028	682	0.01%	0.004%
68	9.769	2697	2699	2702	rBV3	1331	656	0.01%	0.004%
69	9.804	2707	2710	2711	rBV3	967	525	0.01%	0.003%
70	9.830	2715	2718	2719	rBV3	766	463	0.01%	0.003%
71	9.933	2748	2750	2753	rBV4	1479	1011	0.02%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016477.D
 Acq On : 04 Jun 2020 00:05
 Operator : SY/MD
 Sample : L2869-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBFG7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

72	10.068	2790	2792	2795	rVB4	1047	575	0.01%	0.003%
73	10.158	2817	2820	2825	rBV7	1312	1476	0.02%	0.009%
74	10.238	2833	2845	2859	rVV	418868	652499	10.23%	3.817%
75	10.370	2883	2886	2887	rBV2	1192	581	0.01%	0.003%
76	10.402	2891	2896	2904	rVB2	2362	3175	0.05%	0.019%
77	10.592	2953	2955	2957	rBV3	1178	639	0.01%	0.004%
78	10.839	3030	3032	3034	rBV3	881	558	0.01%	0.003%
79	10.923	3054	3058	3060	rVB5	1150	758	0.01%	0.004%
80	11.045	3094	3096	3099	rBV4	1570	824	0.01%	0.005%
81	11.177	3132	3137	3139	rBV6	1403	1374	0.02%	0.008%
82	11.270	3154	3166	3186	rBV	691831	1056265	16.56%	6.178%
83	11.428	3209	3215	3220	rBV10	2471	2830	0.04%	0.017%
84	11.646	3272	3283	3298	rBV	668372	1045453	16.39%	6.115%
85	11.965	3381	3382	3385	rBV	824	474	0.01%	0.003%
86	12.129	3431	3433	3436	rVB3	1366	526	0.01%	0.003%
87	12.231	3461	3465	3467	rBV3	990	960	0.02%	0.006%
88	12.531	3556	3558	3563	rVB4	973	537	0.01%	0.003%
89	12.621	3580	3586	3587	rBV5	1745	1673	0.03%	0.010%
90	12.698	3608	3610	3613	rBV3	855	472	0.01%	0.003%
91	12.836	3648	3653	3655	rBV5	1614	1260	0.02%	0.007%
92	12.871	3659	3664	3665	rBV5	1362	897	0.01%	0.005%
93	13.026	3710	3712	3714	rBV3	1151	632	0.01%	0.004%
94	13.196	3761	3765	3768	rBV5	1545	1199	0.02%	0.007%
95	13.238	3776	3778	3780	rBV2	1298	471	0.01%	0.003%
96	13.498	3856	3859	3861	rBV4	1227	867	0.01%	0.005%
97	13.566	3878	3880	3882	rBV3	977	588	0.01%	0.003%
98	14.151	4058	4062	4064	rBV4	1325	868	0.01%	0.005%
99	14.212	4079	4081	4084	rBV4	1414	882	0.01%	0.005%
100	14.383	4130	4134	4137	rBV4	1853	1306	0.02%	0.008%


Sum of corrected areas: 17095958

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060320\
Data File : VV016477.D
Acq On : 04 Jun 2020 00:05
Operator : SY/MD
Sample : L2869-07
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 56 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
DBFG7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

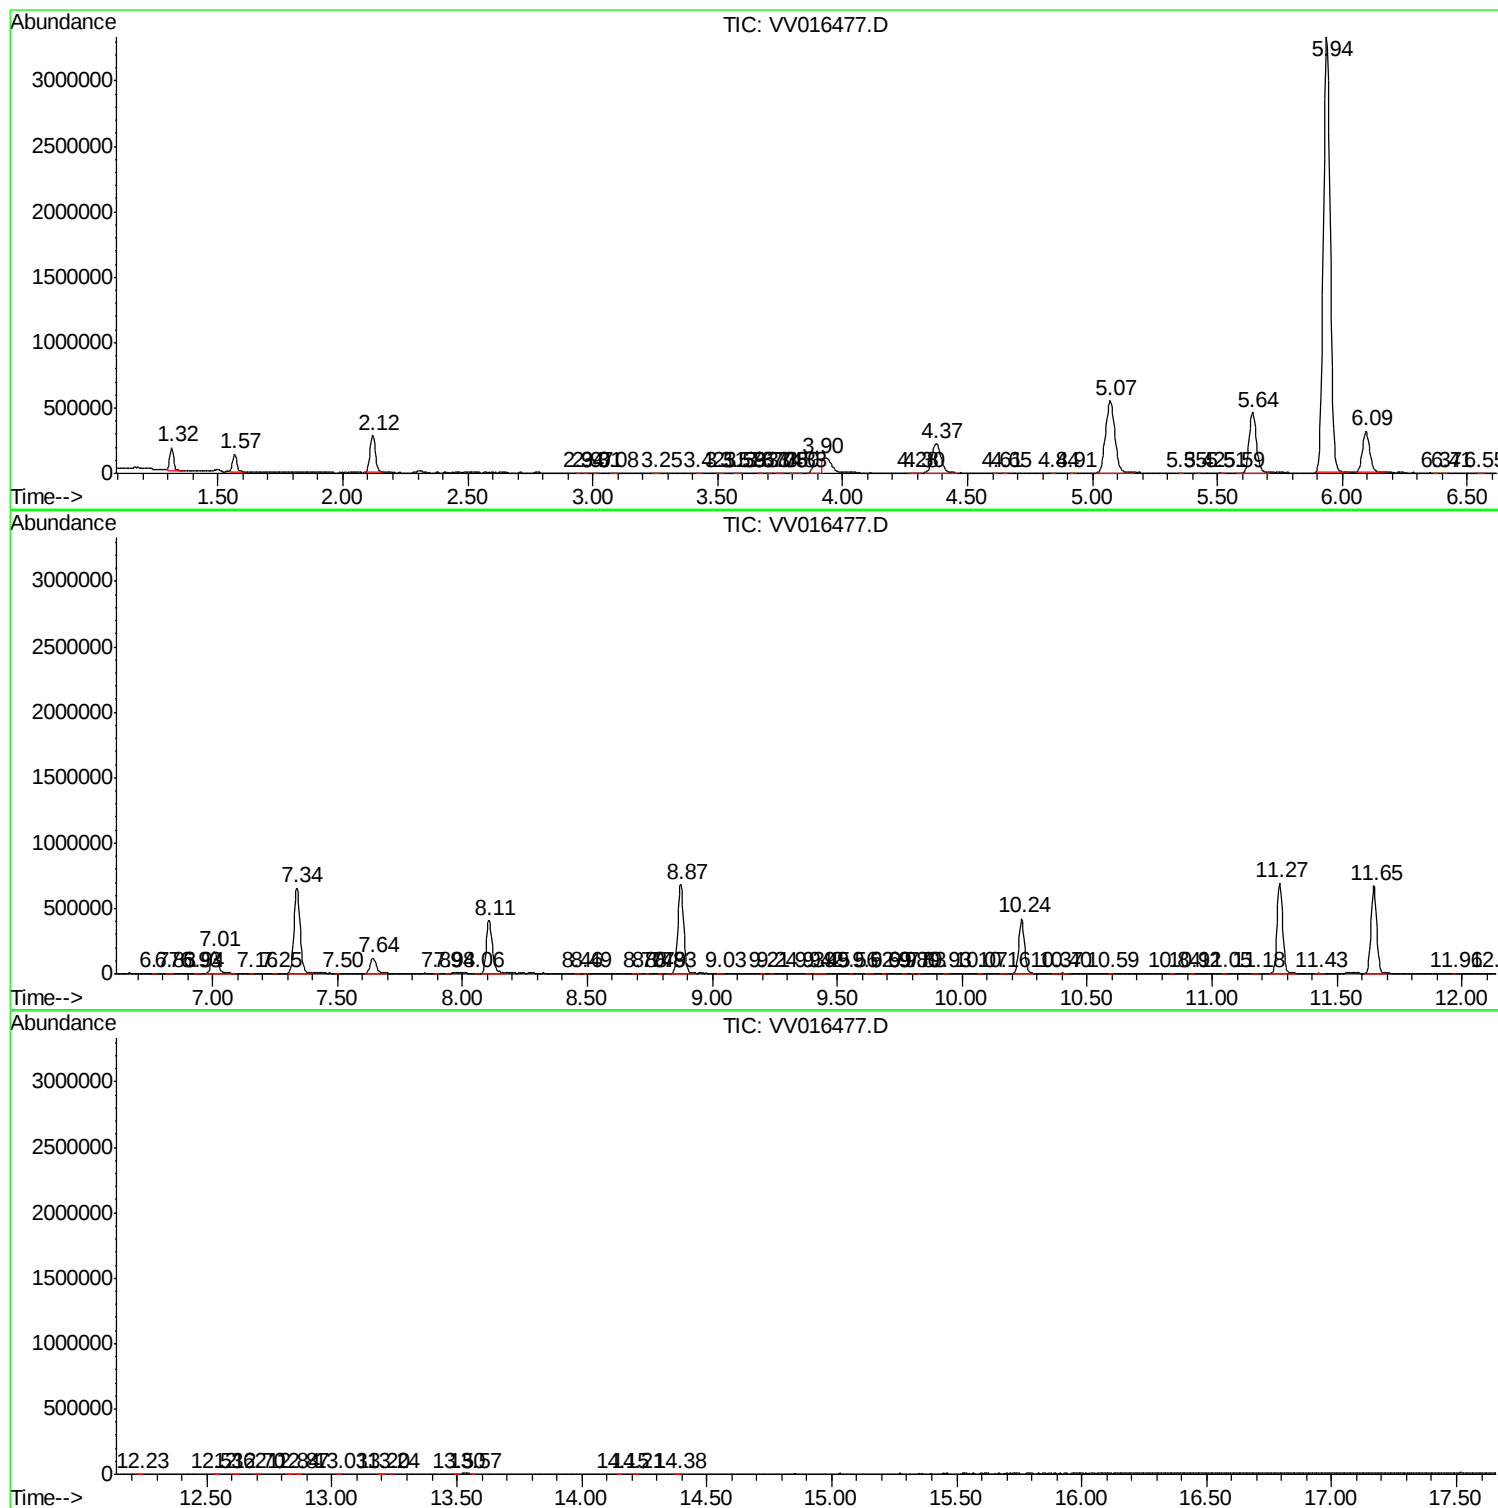

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060320\
Data File : VV016477.D
Acq On : 04 Jun 2020 00:05
Operator : SY/MD
Sample : L2869-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 56 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBFG7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060320\
Data File : VV016477.D
Acq On : 04 Jun 2020 00:05
Operator : SY/MD
Sample : L2869-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 56 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBFG7

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc