

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016480.D
 Acq On : 04 Jun 2020 01:16
 Operator : SY/MD
 Sample : L2849-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETP6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	64	71	89	rVB	3675351	3722111	28.23%	13.662%
2	1.573	143	150	161	rVB	143293	162130	1.23%	0.595%
3	2.122	312	321	333	rBV2	311315	460819	3.49%	1.691%
4	2.778	513	525	541	rBV2	23295	45946	0.35%	0.169%
5	2.878	555	556	558	rBV2	712	219	0.00%	0.001%
6	2.891	558	560	561	rBV2	1120	350	0.00%	0.001%
7	2.952	576	579	580	rBV2	1292	676	0.01%	0.002%
8	3.071	614	616	621	rVB5	1665	1199	0.01%	0.004%
9	3.093	621	623	626	rBV3	1122	666	0.01%	0.002%
10	3.184	648	651	654	rBV4	1732	1307	0.01%	0.005%
11	3.315	689	692	696	rBV5	1158	772	0.01%	0.003%
12	3.457	734	736	737	rBV2	1004	375	0.00%	0.001%
13	3.579	772	774	779	rBV4	783	491	0.00%	0.002%
14	3.659	796	799	801	rBV3	750	430	0.00%	0.002%
15	3.675	801	804	807	rBV5	1294	902	0.01%	0.003%
16	3.708	812	814	818	rBV4	1915	1572	0.01%	0.006%
17	3.936	862	885	917	rBV	5398046	13185859	100.00%	48.398%
18	4.376	1008	1022	1049	rVB	227558	554503	4.21%	2.035%
19	4.765	1141	1143	1146	rBV4	1286	951	0.01%	0.003%
20	4.920	1189	1191	1193	rVB4	1137	333	0.00%	0.001%
21	4.945	1197	1199	1202	rBV3	1159	703	0.01%	0.003%
22	4.981	1208	1210	1211	rBV2	981	407	0.00%	0.001%
23	5.071	1220	1238	1263	rBV2	547404	1425080	10.81%	5.231%
24	5.495	1368	1370	1374	rBV4	1613	838	0.01%	0.003%
25	5.537	1382	1383	1385	rBV2	1256	518	0.00%	0.002%
26	5.640	1402	1415	1439	rBV	438588	861971	6.54%	3.164%
27	5.942	1495	1509	1523	rBV6	19790	46948	0.36%	0.172%
28	6.035	1535	1538	1541	rVB5	2410	1333	0.01%	0.005%
29	6.093	1541	1556	1581	rBV2	318308	649825	4.93%	2.385%
30	6.315	1623	1625	1628	rBV4	1134	708	0.01%	0.003%
31	6.498	1678	1682	1684	rBV5	1403	1110	0.01%	0.004%
32	6.553	1696	1699	1700	rBV2	999	493	0.00%	0.002%
33	6.724	1750	1752	1755	rBV4	999	637	0.00%	0.002%
34	6.933	1815	1817	1819	rBV3	934	441	0.00%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
 Data File : VV016480.D
 Acq On : 04 Jun 2020 01:16
 Operator : SY/MD
 Sample : L2849-01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETPP6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
 Title : VOC Analysis

35	6.965	1825	1827	1829	rBV3	1150	621	0.00%	0.002%
36	7.007	1829	1840	1854	rVV	156061	280456	2.13%	1.029%
37	7.338	1931	1943	1962	rBV	664041	1128186	8.56%	4.141%
38	7.643	2027	2038	2055	rBV2	111218	192901	1.46%	0.708%
39	7.955	2131	2135	2138	rBV5	1968	1430	0.01%	0.005%
40	8.106	2172	2182	2202	rBV	407722	675753	5.12%	2.480%
41	8.486	2298	2300	2302	rVB3	1144	411	0.00%	0.002%
42	8.511	2306	2308	2311	rBV3	1072	681	0.01%	0.002%
43	8.579	2328	2329	2334	rBV4	1307	1095	0.01%	0.004%
44	8.691	2359	2364	2368	rBV7	1659	1910	0.01%	0.007%
45	8.871	2409	2420	2446	rBV	647618	1063902	8.07%	3.905%
46	9.106	2492	2493	2497	rVB3	1233	703	0.01%	0.003%
47	9.267	2540	2543	2545	rBV4	1028	705	0.01%	0.003%
48	9.408	2584	2587	2591	rBV4	1634	1550	0.01%	0.006%
49	9.707	2679	2680	2682	rBV	886	406	0.00%	0.001%
50	9.736	2685	2689	2694	rBV8	1232	1328	0.01%	0.005%
51	9.778	2701	2702	2705	rBV3	795	474	0.00%	0.002%
52	9.813	2712	2713	2714	rBV	896	272	0.00%	0.001%
53	10.019	2772	2777	2779	rBV5	1432	1191	0.01%	0.004%
54	10.045	2783	2785	2789	rBV4	1033	897	0.01%	0.003%
55	10.116	2803	2807	2808	rBV3	1086	751	0.01%	0.003%
56	10.161	2819	2821	2822	rBV	1532	614	0.00%	0.002%
57	10.238	2832	2845	2859	rBV	427149	663853	5.03%	2.437%
58	10.685	2982	2984	2986	rBV3	848	251	0.00%	0.001%
59	10.704	2986	2990	2992	rBV4	1029	805	0.01%	0.003%
60	10.730	2997	2998	2999	rBV	856	226	0.00%	0.001%
61	11.042	3093	3095	3096	rBV3	1230	464	0.00%	0.002%
62	11.061	3100	3101	3105	rVB3	781	543	0.00%	0.002%
63	11.270	3155	3166	3184	rBV	670196	1014102	7.69%	3.722%
64	11.518	3240	3243	3246	rBV4	1648	1011	0.01%	0.004%
65	11.646	3272	3283	3299	rBV	688251	1061624	8.05%	3.897%
66	11.897	3358	3361	3362	rBV3	889	500	0.00%	0.002%
67	12.170	3441	3446	3449	rBV6	1950	1754	0.01%	0.006%
68	12.453	3532	3534	3536	rBV3	1180	610	0.00%	0.002%
69	12.534	3556	3559	3561	rBV3	1448	770	0.01%	0.003%
70	12.627	3582	3588	3589	rBV5	1193	1138	0.01%	0.004%
71	12.807	3642	3644	3646	rBV3	941	490	0.00%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060320\
Data File : VV016480.D
Acq On : 04 Jun 2020 01:16
Operator : SY/MD
Sample : L2849-01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 59 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTP6

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Title : VOC Analysis

72	13.032	3711	3714	3717	rBV3	1913	1214	0.01%	0.004%
73	13.347	3810	3812	3816	rBV5	1719	1282	0.01%	0.005%
74	13.823	3957	3960	3964	rBV4	1252	968	0.01%	0.004%
75	14.135	4055	4057	4062	rBV5	1908	1758	0.01%	0.006%
76	14.228	4085	4086	4088	rBV2	1079	332	0.00%	0.001%
77	15.312	4421	4423	4424	rBV2	1719	796	0.01%	0.003%
78	15.550	4495	4497	4501	rBV4	1983	1064	0.01%	0.004%


Sum of corrected areas: 27244415

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060320\
Data File : VV016480.D
Acq On : 04 Jun 2020 01:16
Operator : SY/MD
Sample : L2849-01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 59 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTP6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

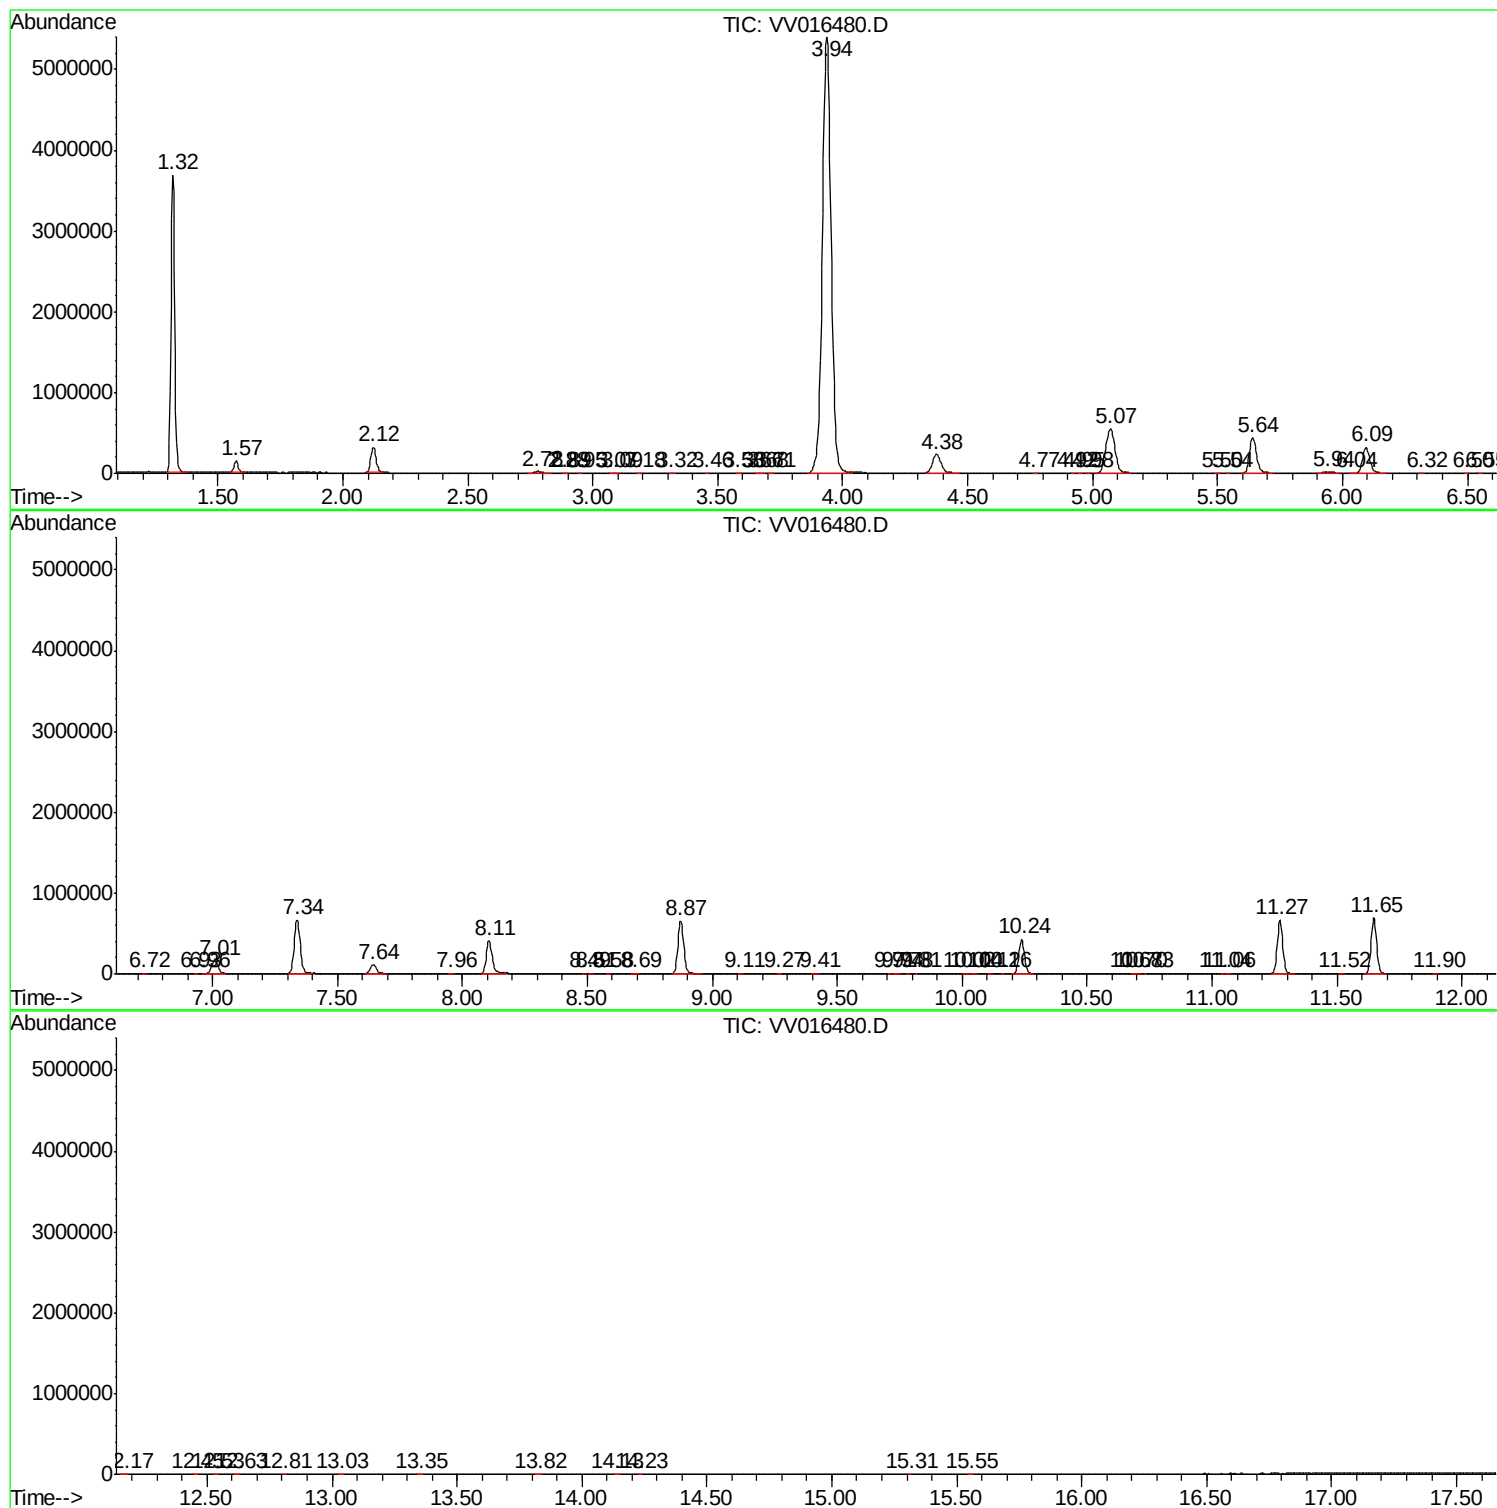

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060320\
Data File : VV016480.D
Acq On : 04 Jun 2020 01:16
Operator : SY/MD
Sample : L2849-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 59 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETTP6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV060320\
Data File : VV016480.D
Acq On : 04 Jun 2020 01:16
Operator : SY/MD
Sample : L2849-01
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 59 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
ETTP6

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM060320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc